

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071025\
 Data File : P0112201.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jul 2025 19:23
 Operator : YP/AJ
 Sample : Q2551-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 VNJ-204

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/11/2025
 Supervised By :mohammad ahmed 07/11/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 22:56:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 10:50:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.670	3.664	285.8E6	216.9E6	28.885m	34.043
2) SA Decachlor...	8.698	8.648	109.3E6	32319361	15.984m	18.753m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071025\
Data File : PO112201.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jul 2025 19:23
Operator : YP/AJ
Sample : Q2551-02
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
VNJ-204


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/11/2025
Supervised By :mohammad ahmed 07/11/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 22:56:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 09 10:50:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

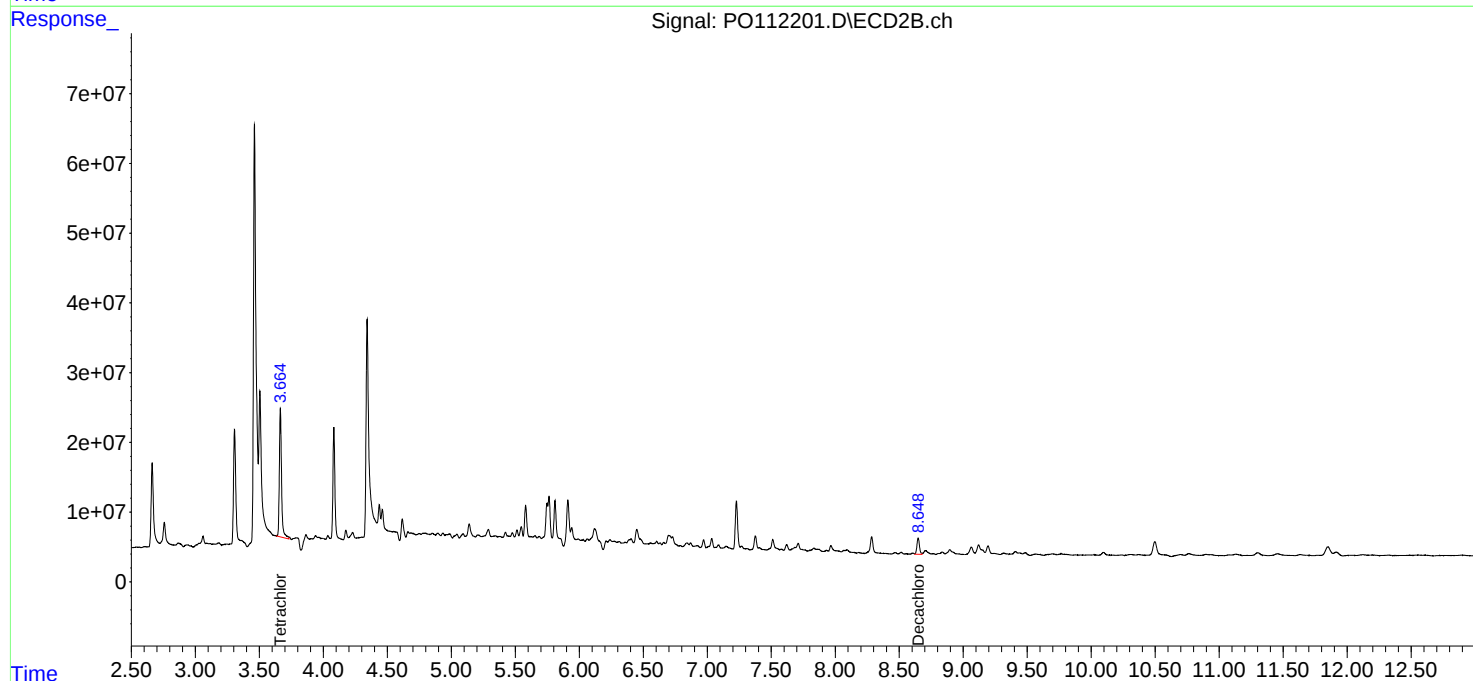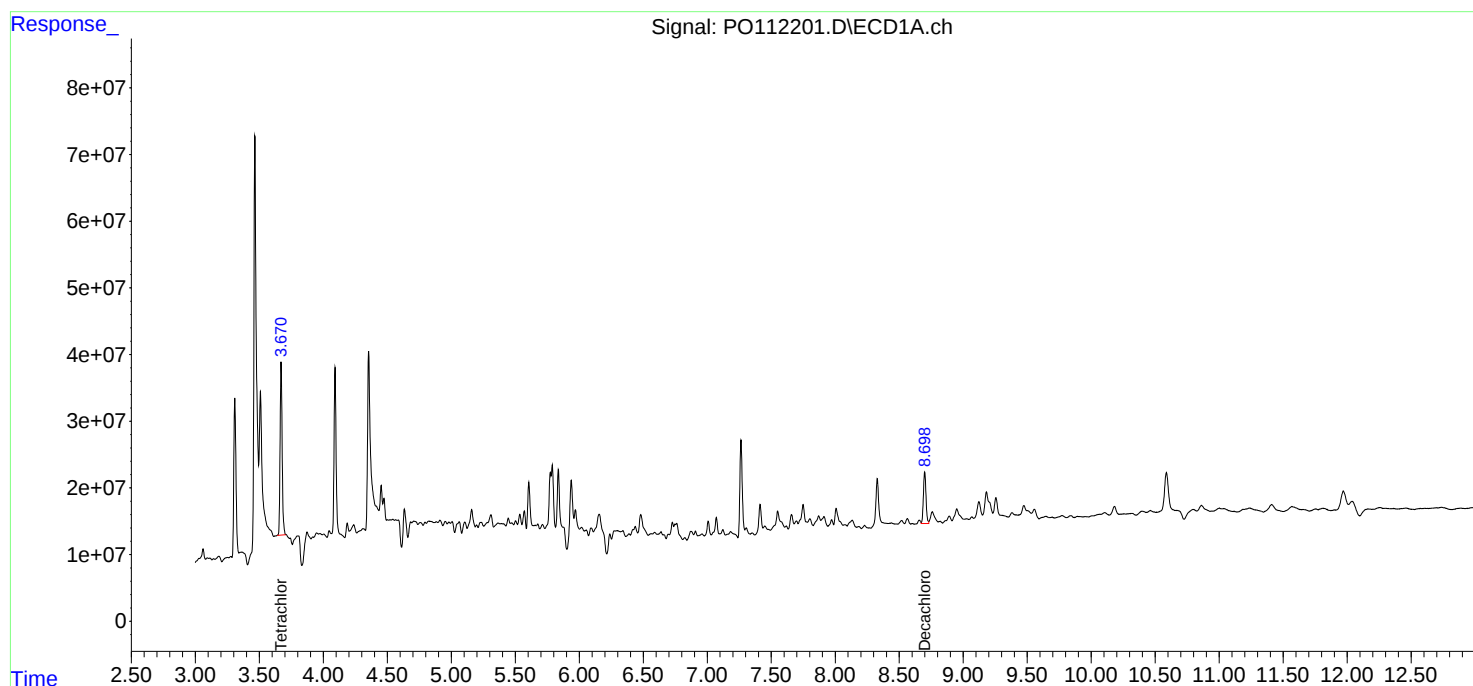

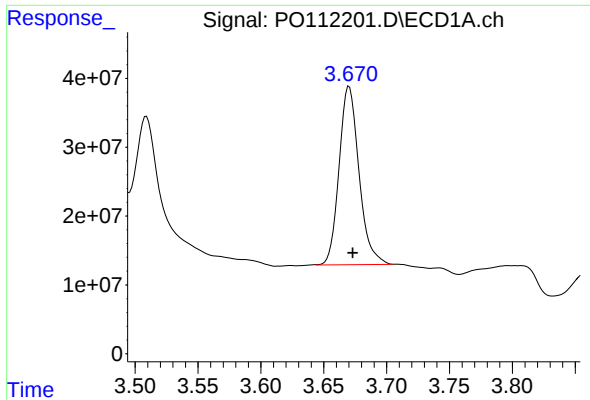


#1 Tetrachloro-m-xylene

R.T.: 3.670 min
Delta R.T.: -0.003 min
Response: 285808811
Conc: 28.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
VNJ-204


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/11/2025
Supervised By :mohammad ahmed 07/11/2025

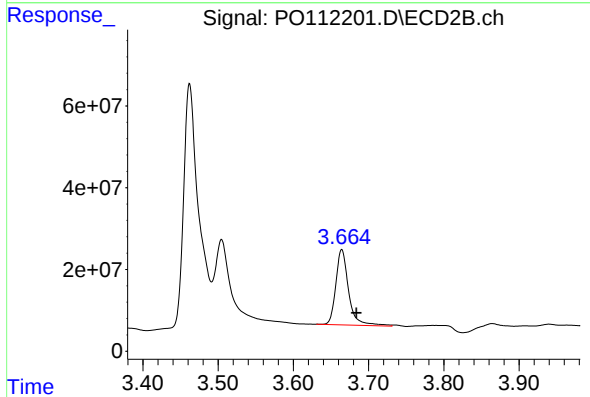


#1 Tetrachloro-m-xylene

R.T.: 3.664 min
Delta R.T.: -0.019 min
Response: 216890784
Conc: 34.04 ng/ml

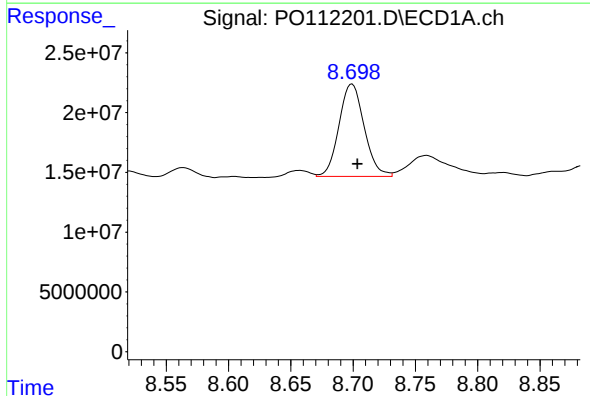

#2 Decachlorobiphenyl

R.T.: 8.698 min
Delta R.T.: -0.005 min
Response: 109286262
Conc: 15.98 ng/ml m

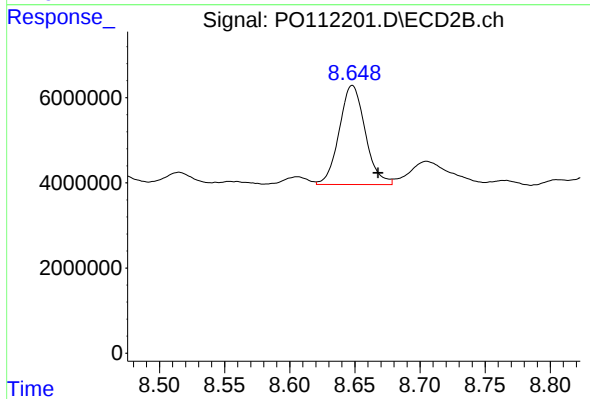

#2 Decachlorobiphenyl

R.T.: 8.648 min
Delta R.T.: -0.020 min
Response: 32319361
Conc: 18.75 ng/ml m