

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0071118\
Data File : P0046575.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Jul 2018 20:11
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 04:17:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.205	3.532	4719792	4757874	19.749	22.400
2) SA Decachlor...	9.732	8.460	3789385	3718148	19.881	19.168

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0071118\
Data File : P0046575.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Jul 2018 20:11
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 04:17:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

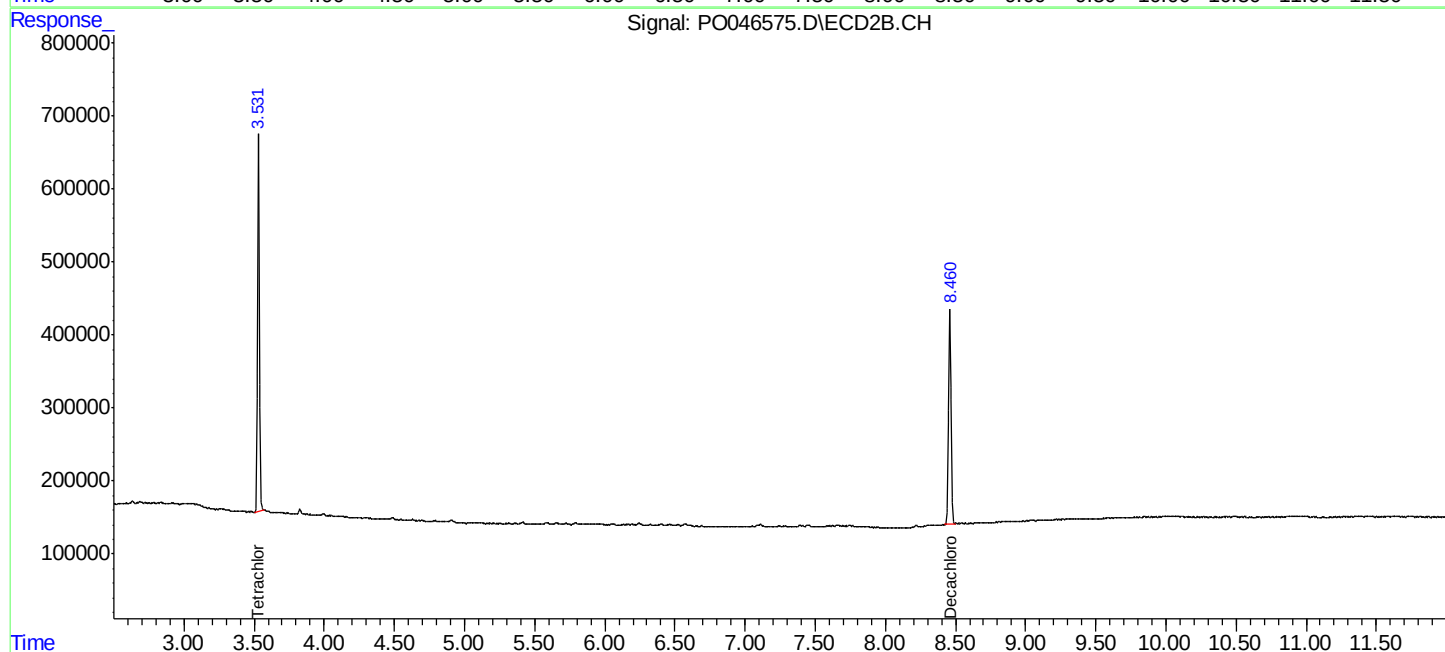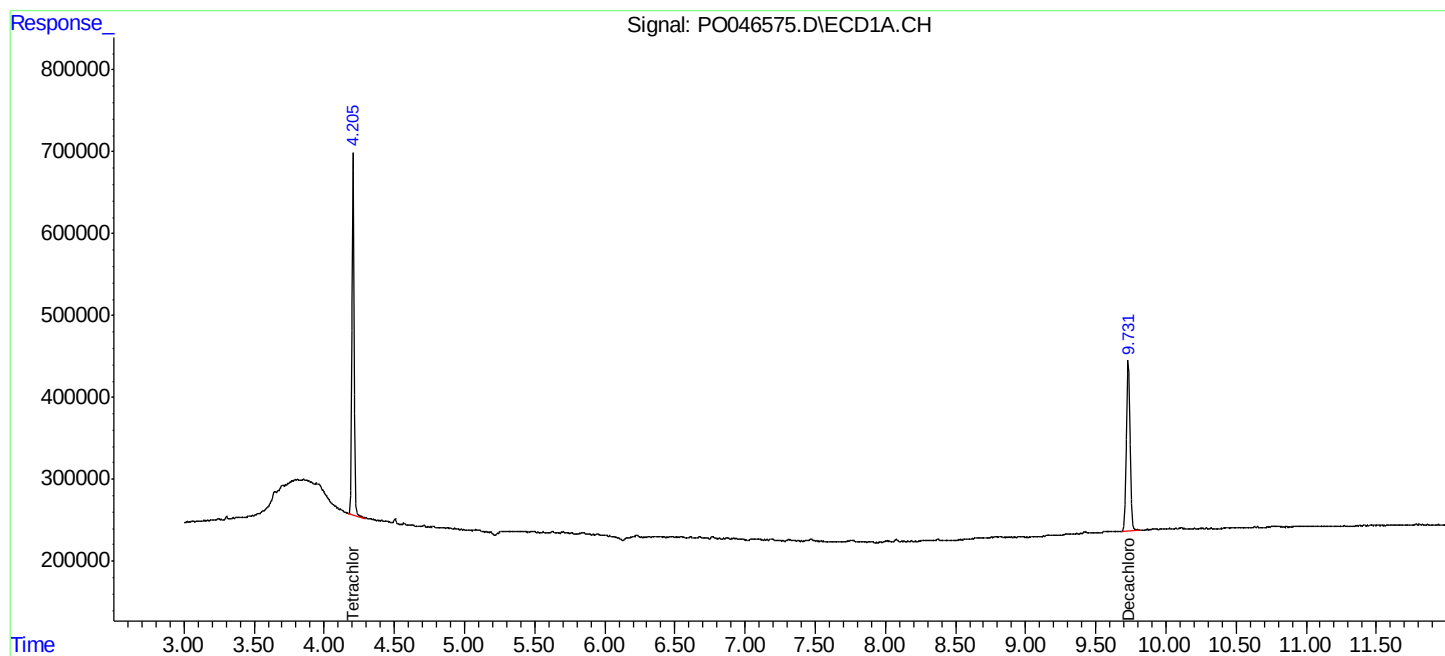


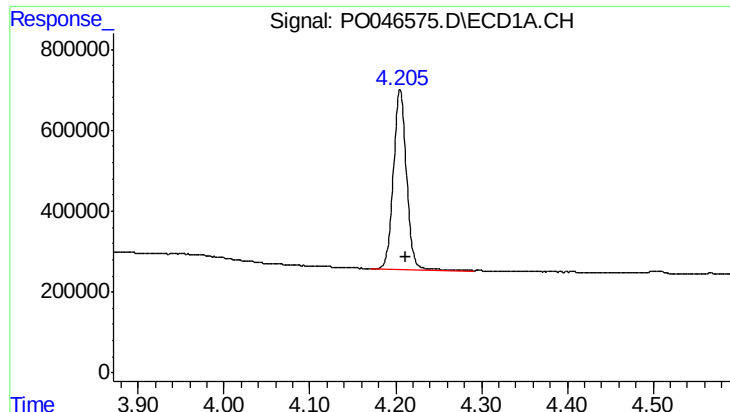

#1 Tetrachloro-m-xylene


R.T.: 4.205 min
Delta R.T.: -0.007 min
Response: 4719792
Conc: 19.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

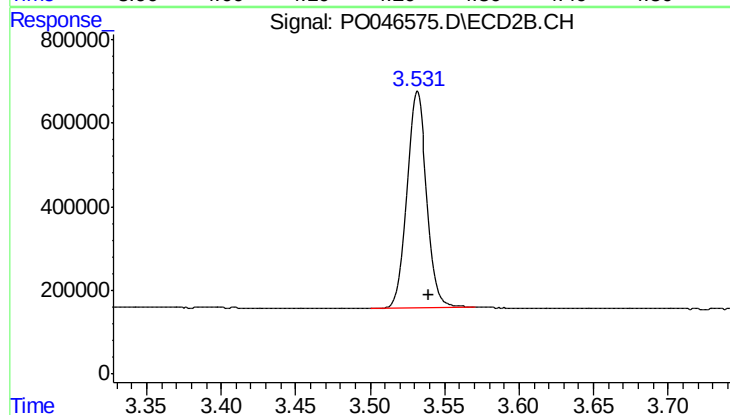


#1 Tetrachloro-m-xylene

R.T.: 3.532 min
Delta R.T.: -0.008 min
Response: 4757874
Conc: 22.40 ng/ml

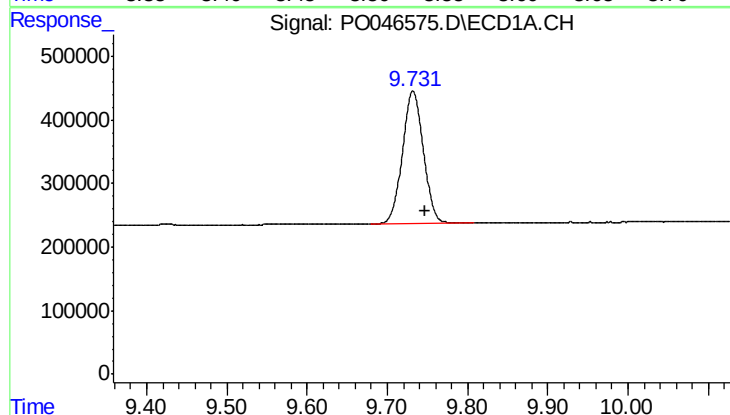

#2 Decachlorobiphenyl

R.T.: 9.732 min
Delta R.T.: -0.016 min
Response: 3789385
Conc: 19.88 ng/ml

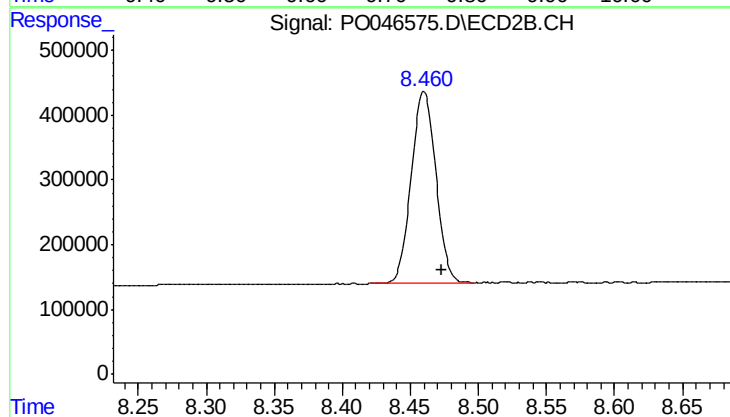

#2 Decachlorobiphenyl

R.T.: 8.460 min
Delta R.T.: -0.013 min
Response: 3718148
Conc: 19.17 ng/ml