

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0071118\
 Data File : P0046580.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Jul 2018 21:31
 Operator : SM/SJ
 Sample : J3906-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CB-7-8-6-ST-WW-1@3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 05:24:11 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 09 15:27:34 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.204	3.529	4690145	4607648	19.625	21.693
2) SA Decachlor...	9.730	8.459	2849556	2757871	14.950	14.217

Target Compounds



 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0071118\
Data File : P0046580.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Jul 2018 21:31
Operator : SM/SJ
Sample : J3906-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CB-7-8-6-ST-WW-1@3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 05:24:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

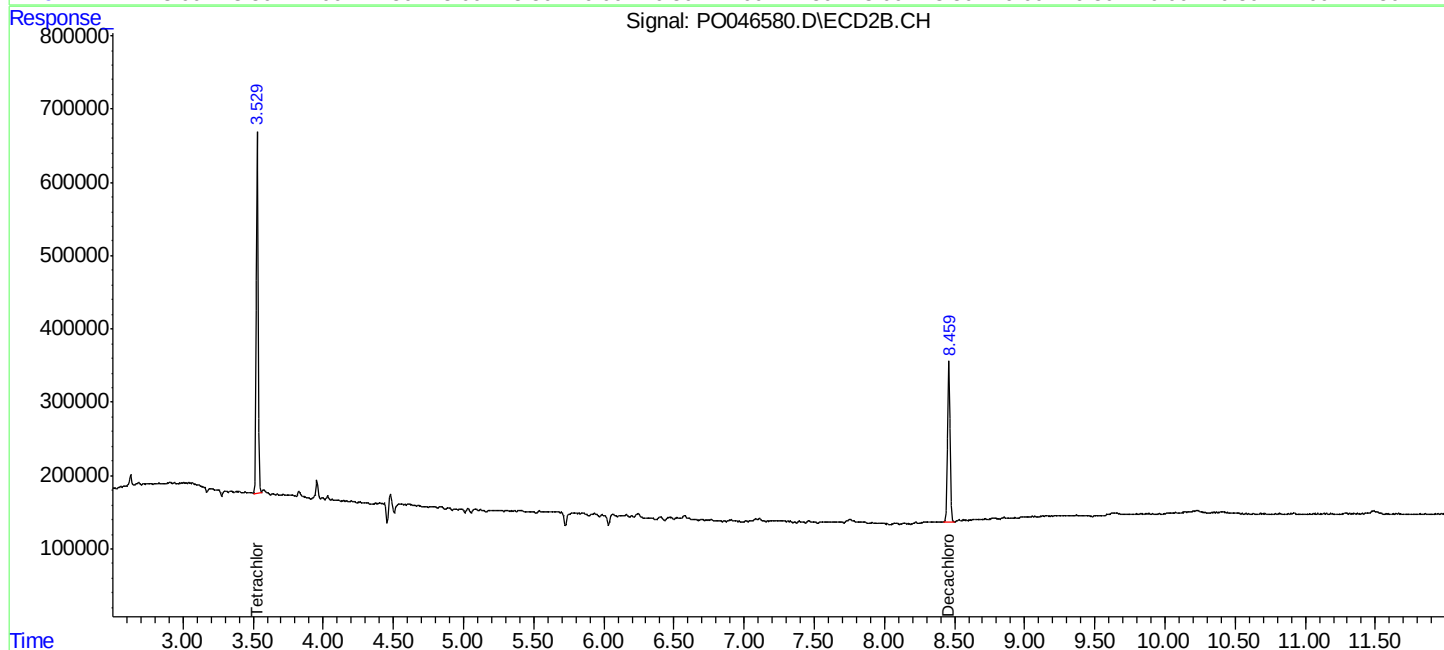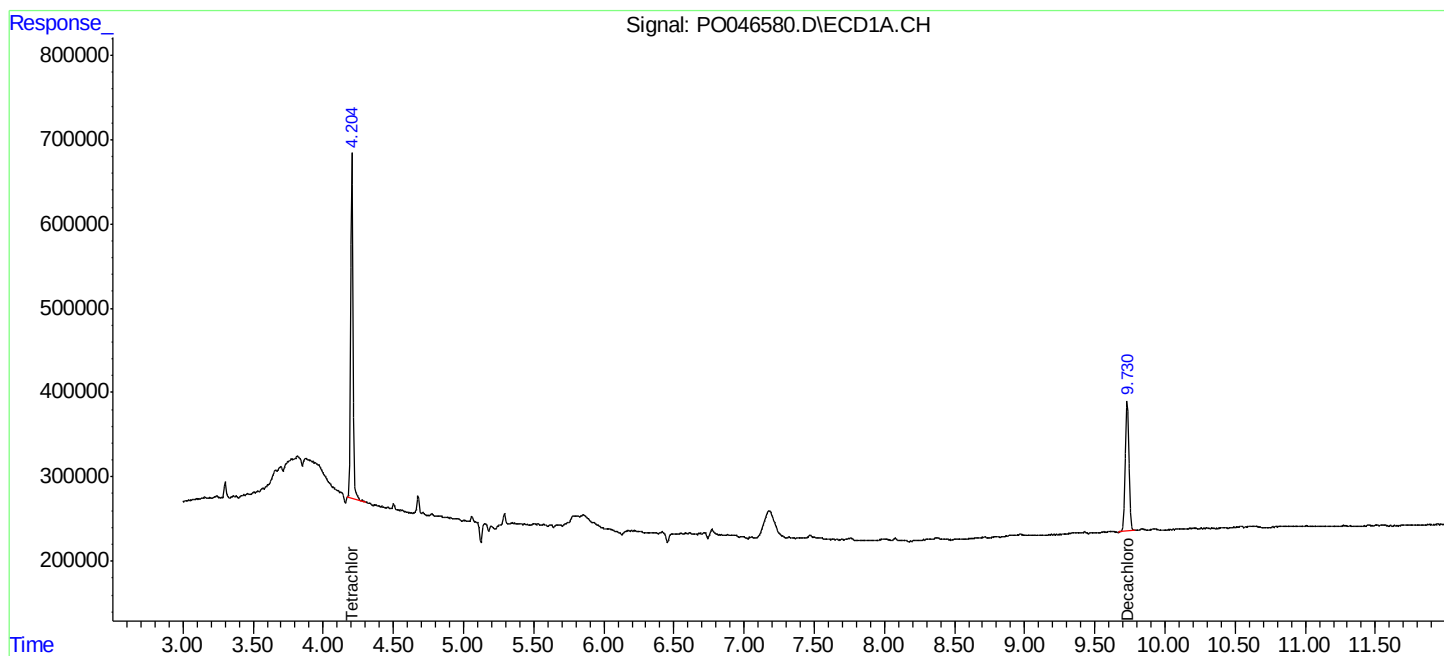


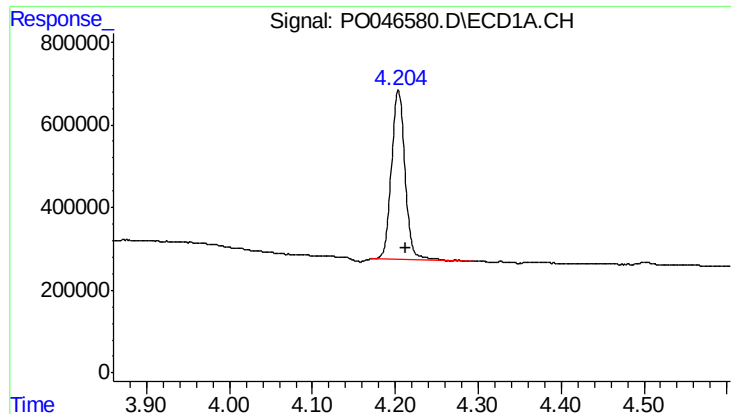

#1 Tetrachloro-m-xylene


R.T.: 4.204 min
Delta R.T.: -0.008 min
Response: 4690145
Conc: 19.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
CB-7-8-6-ST-WW-1@3

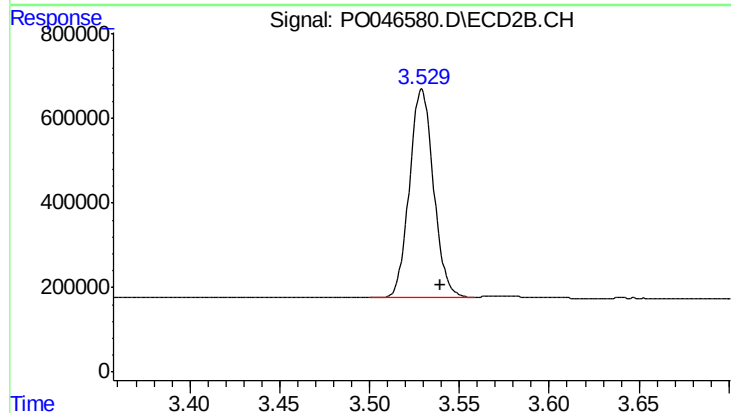


#1 Tetrachloro-m-xylene

R.T.: 3.529 min
Delta R.T.: -0.010 min
Response: 4607648
Conc: 21.69 ng/ml

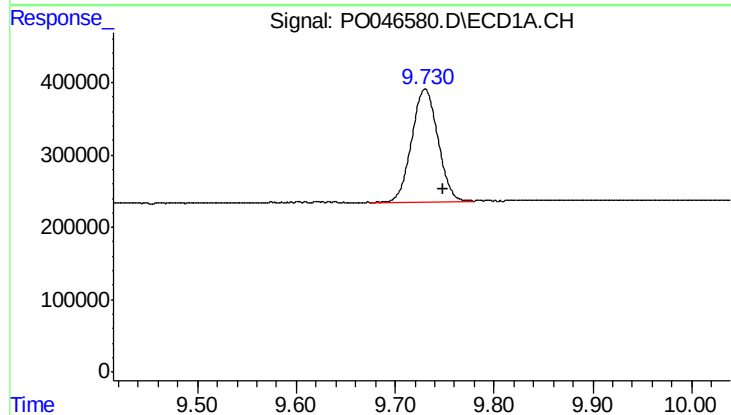

#2 Decachlorobiphenyl

R.T.: 9.730 min
Delta R.T.: -0.018 min
Response: 2849556
Conc: 14.95 ng/ml

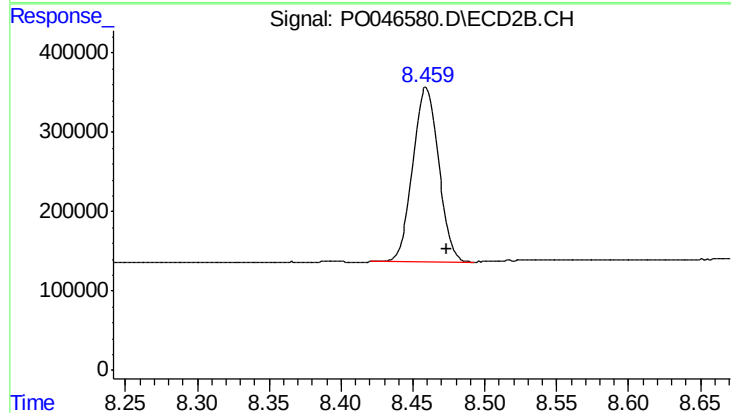

#2 Decachlorobiphenyl

R.T.: 8.459 min
Delta R.T.: -0.014 min
Response: 2757871
Conc: 14.22 ng/ml