

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0071118\
 Data File : P0046581.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Jul 2018 21:47
 Operator : SM/SJ
 Sample : J3906-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CB-7-8-6-ST-EW-1@3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 05:25:01 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 09 15:27:34 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.203	3.529	4663840	4620229	19.515	21.752
2) SA Decachlor...	9.729	8.459	2457381	2404296	12.893	12.394

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0071118\
Data File : P0046581.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Jul 2018 21:47
Operator : SM/SJ
Sample : J3906-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CB-7-8-6-ST-EW-1@3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 05:25:01 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

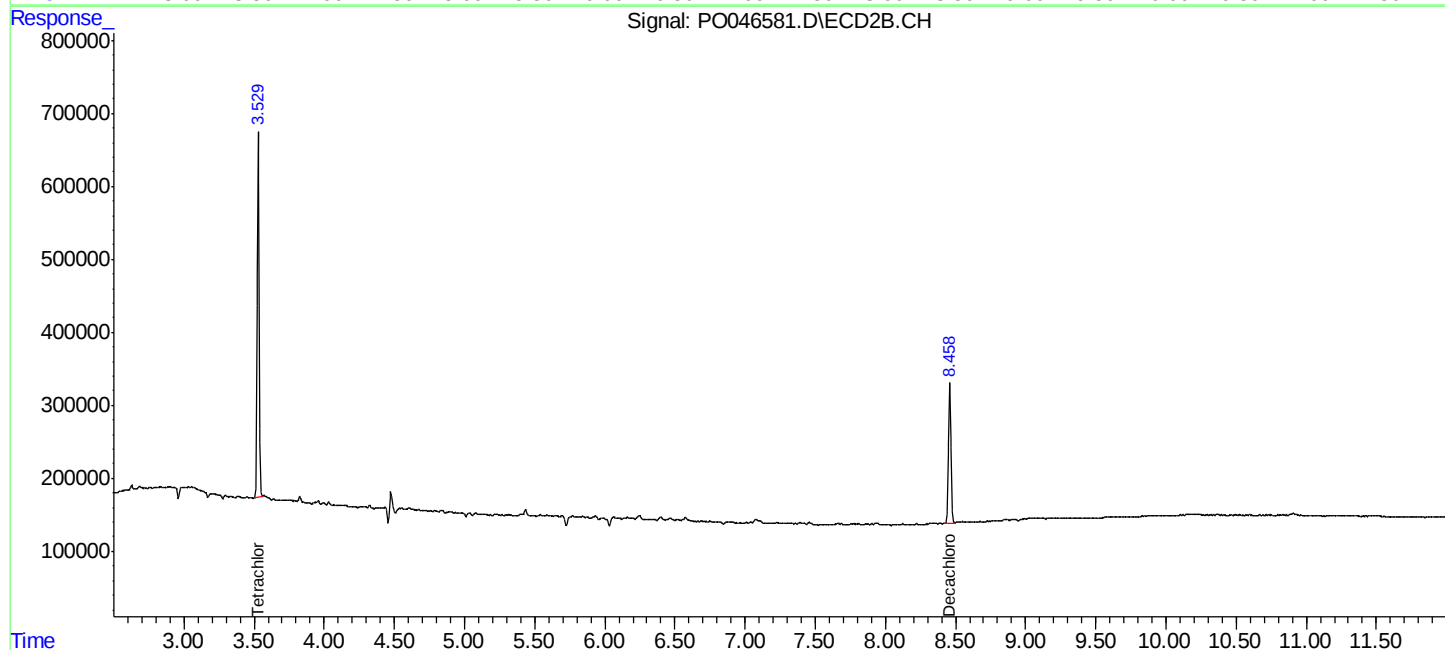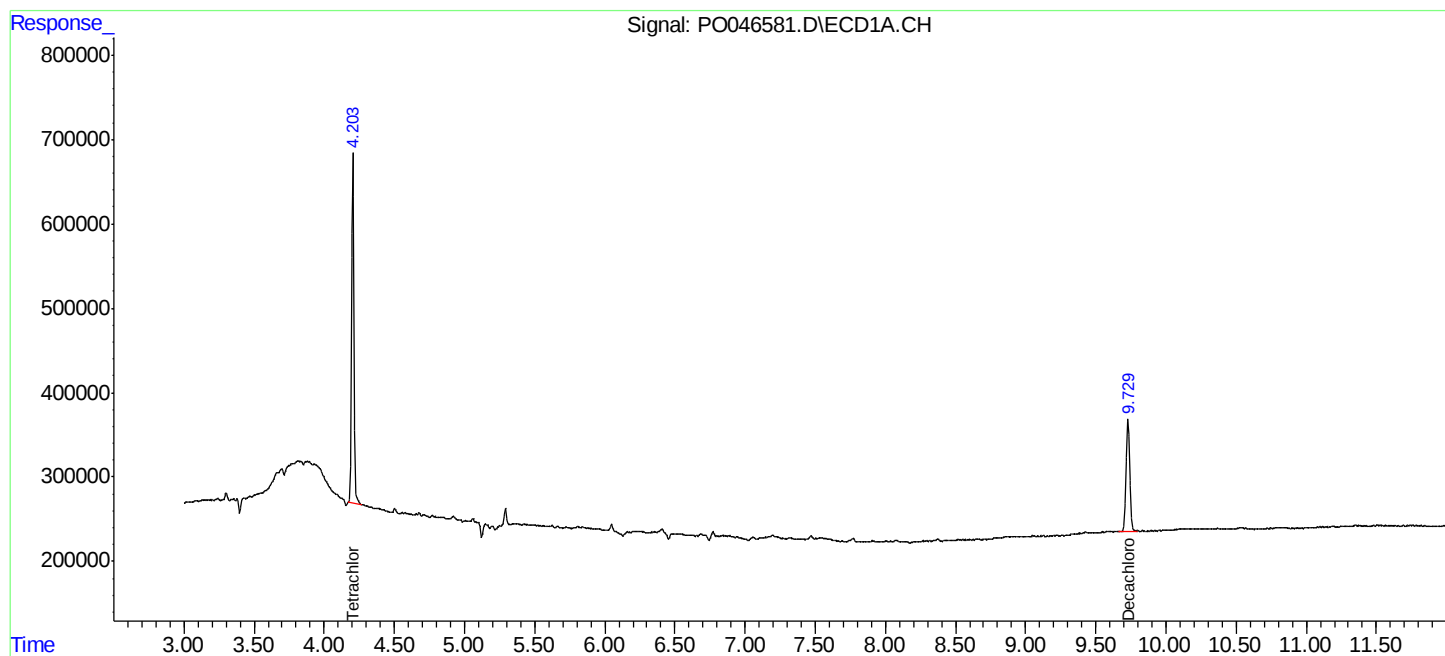


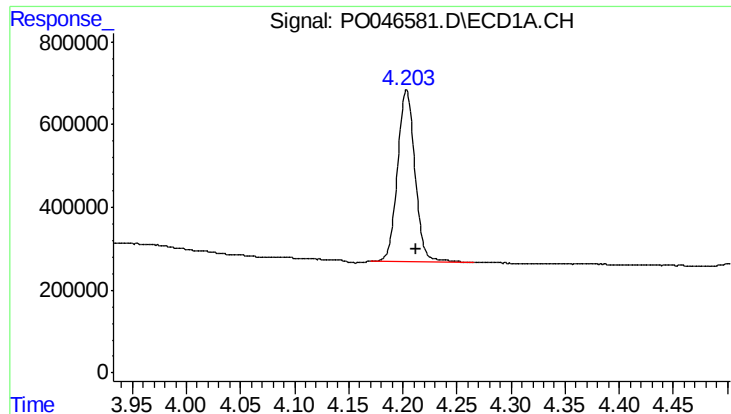

#1 Tetrachloro-m-xylene


R.T.: 4.203 min
Delta R.T.: -0.009 min
Response: 4663840
Conc: 19.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
CB-7-8-6-ST-EW-1@3

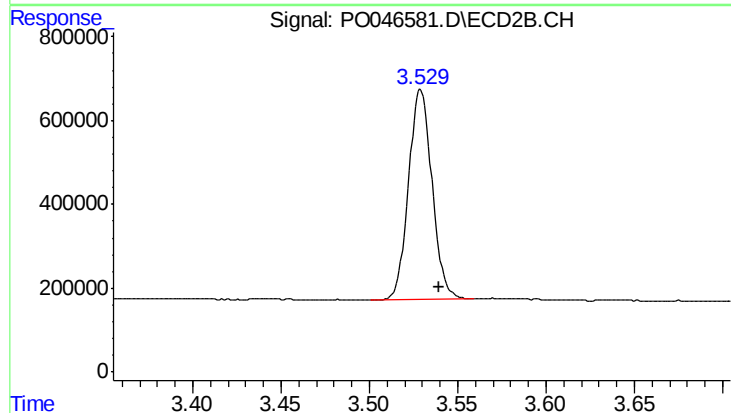


#1 Tetrachloro-m-xylene

R.T.: 3.529 min
Delta R.T.: -0.011 min
Response: 4620229
Conc: 21.75 ng/ml

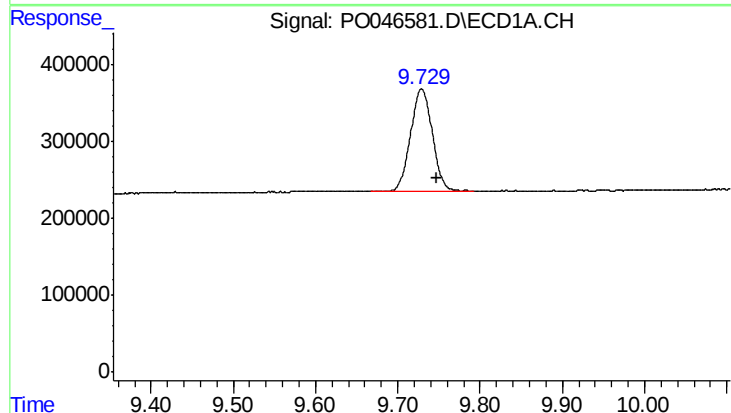

#2 Decachlorobiphenyl

R.T.: 9.729 min
Delta R.T.: -0.019 min
Response: 2457381
Conc: 12.89 ng/ml

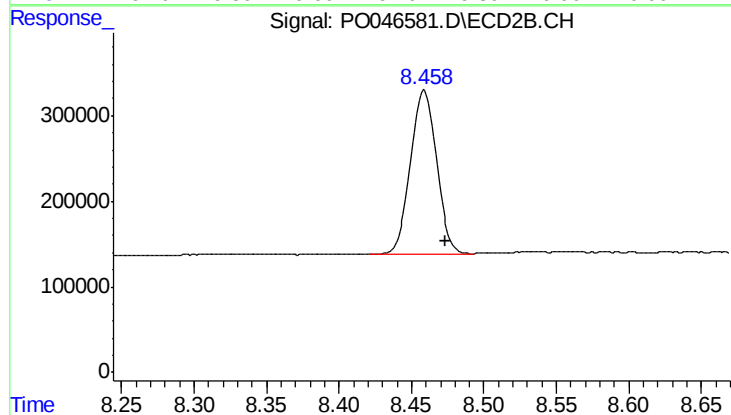

#2 Decachlorobiphenyl

R.T.: 8.459 min
Delta R.T.: -0.015 min
Response: 2404296
Conc: 12.39 ng/ml