

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0071118\
Data File : P0046586.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Jul 2018 23:06
Operator : SM/SJ
Sample : J3906-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CB-7-8-6-ST-BOTTOM-1@3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 05:27:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.204	3.529	5260095	5279334	22.010	24.855
2) SA Decachlor...	9.729	8.458	3045972	3003522	15.981	15.484

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0071118\
Data File : P0046586.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Jul 2018 23:06
Operator : SM/SJ
Sample : J3906-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CB-7-8-6-ST-BOTTOM-1@3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 05:27:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

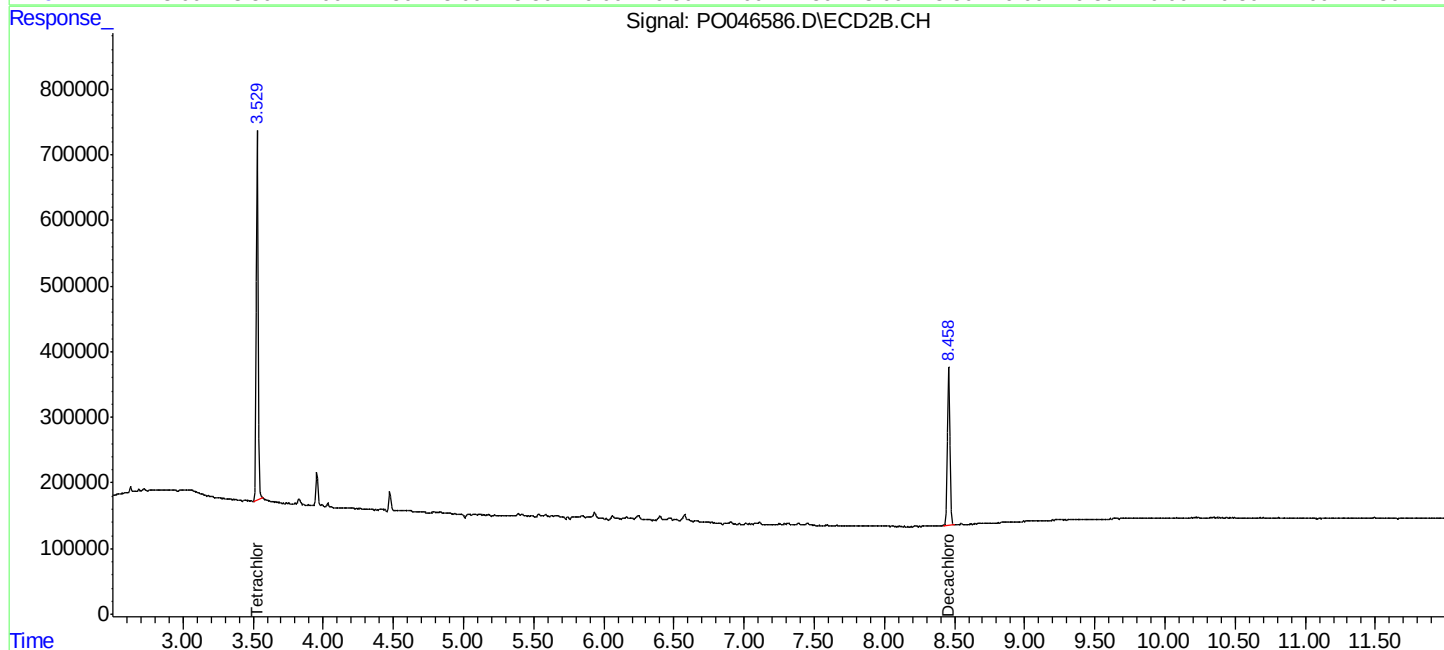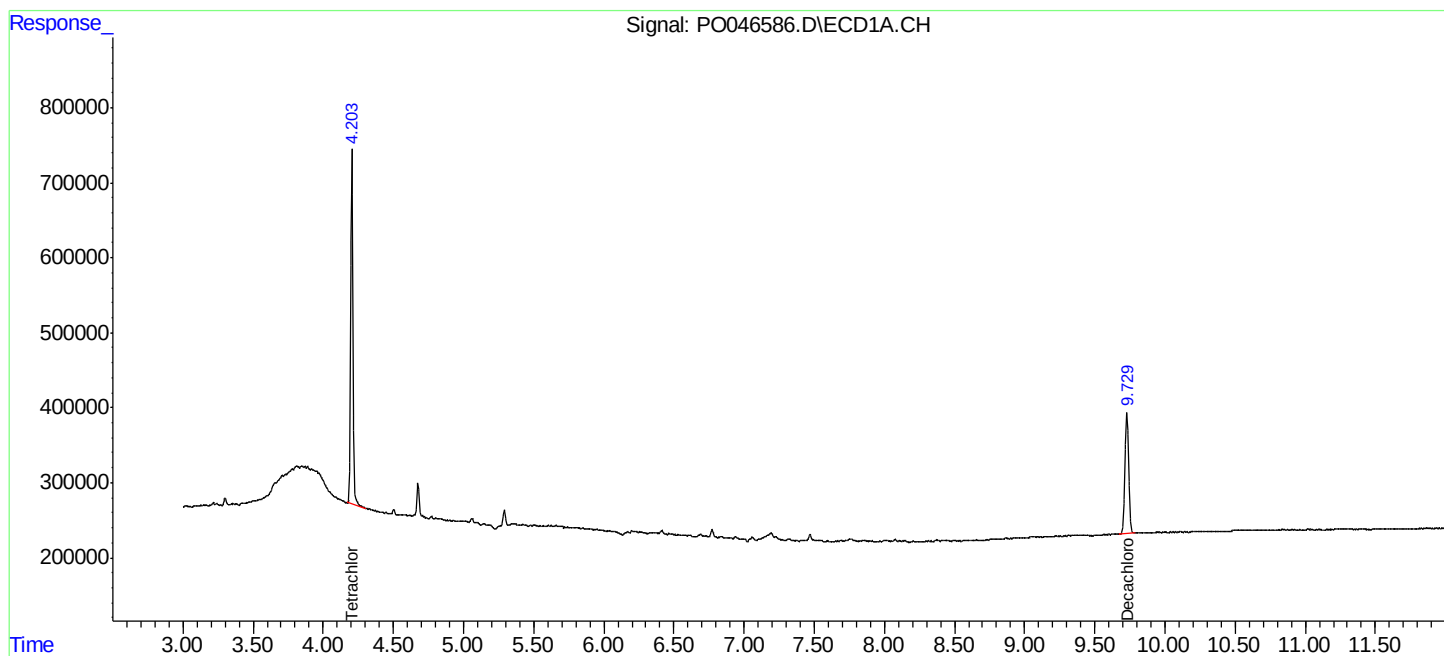


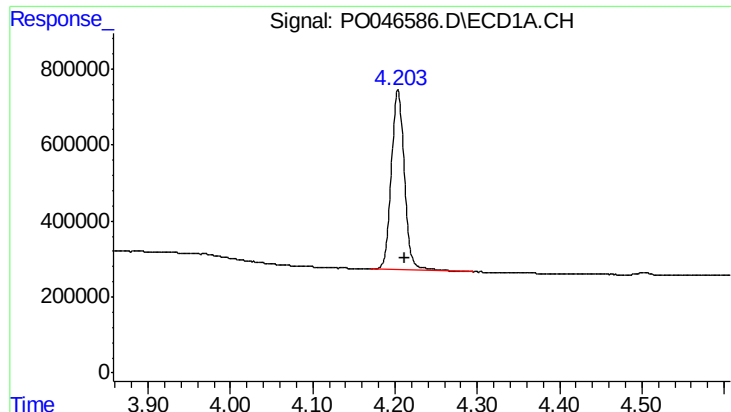

#1 Tetrachloro-m-xylene


R.T.: 4.204 min
Delta R.T.: -0.009 min
Response: 5260095
Conc: 22.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
CB-7-8-6-ST-BOTTOM-1@3

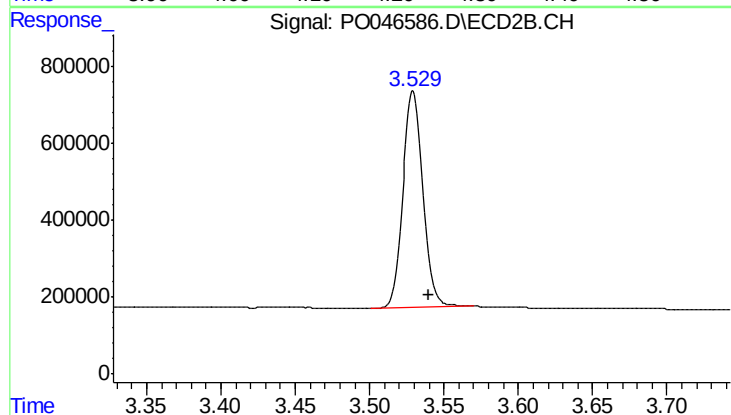


#1 Tetrachloro-m-xylene

R.T.: 3.529 min
Delta R.T.: -0.010 min
Response: 5279334
Conc: 24.85 ng/ml

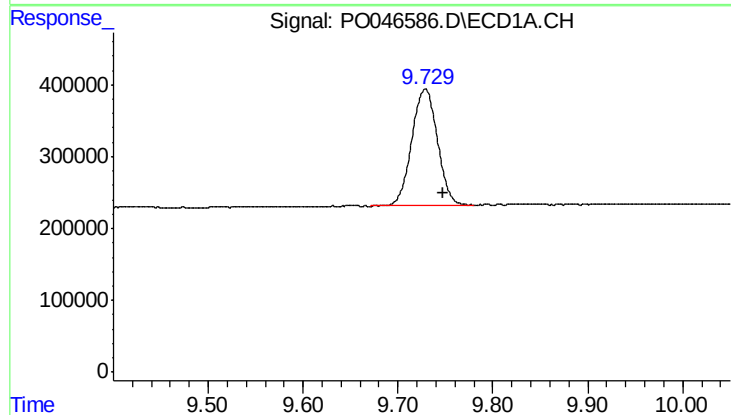

#2 Decachlorobiphenyl

R.T.: 9.729 min
Delta R.T.: -0.019 min
Response: 3045972
Conc: 15.98 ng/ml

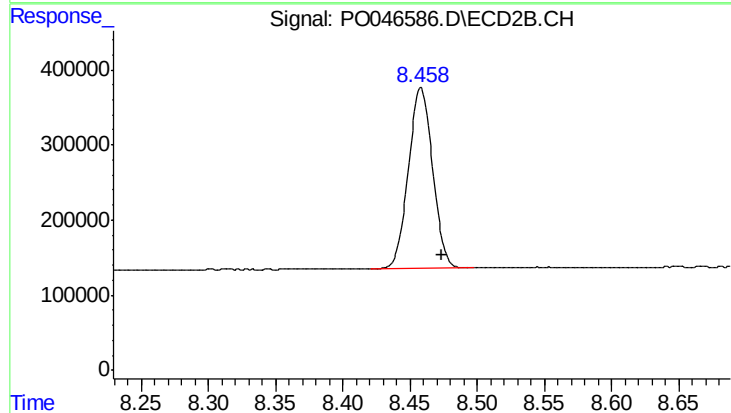

#2 Decachlorobiphenyl

R.T.: 8.458 min
Delta R.T.: -0.015 min
Response: 3003522
Conc: 15.48 ng/ml