

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071124\
 Data File : P0104745.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2024 06:07
 Operator : YP/AJ
 Sample : P3195-01
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 34806

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/12/2024
 Supervised By :Ankita Jodhani 07/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 06:23:42 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070224.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 02 16:29:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.427	3.543	163.6E6	51024810	18.267	15.639m
2) SA Decachlor...	10.233	8.463	89409642	20571340	14.579m	9.809m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071124\
Data File : PO104745.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2024 06:07
Operator : YP/AJ
Sample : P3195-01
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
34806


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/12/2024
Supervised By :Ankita Jodhani 07/12/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 06:23:42 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO070224.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 02 16:29:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

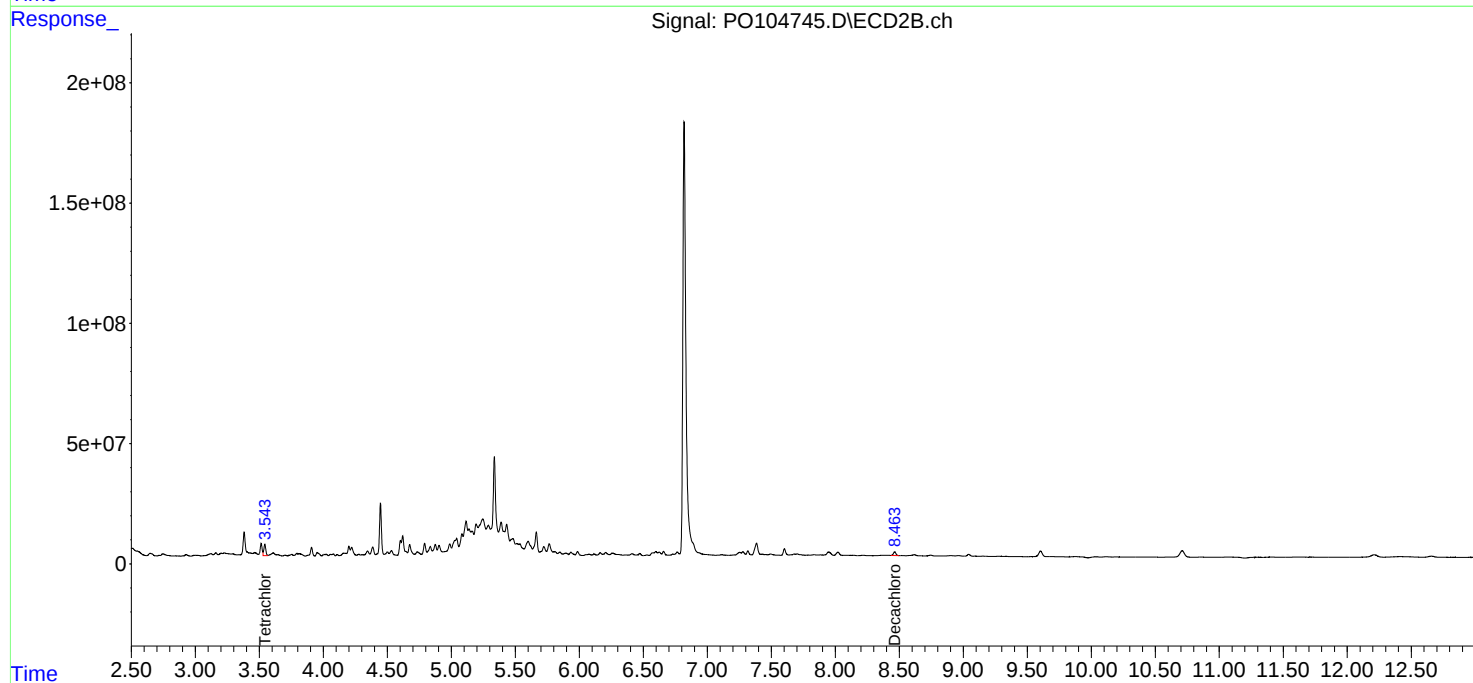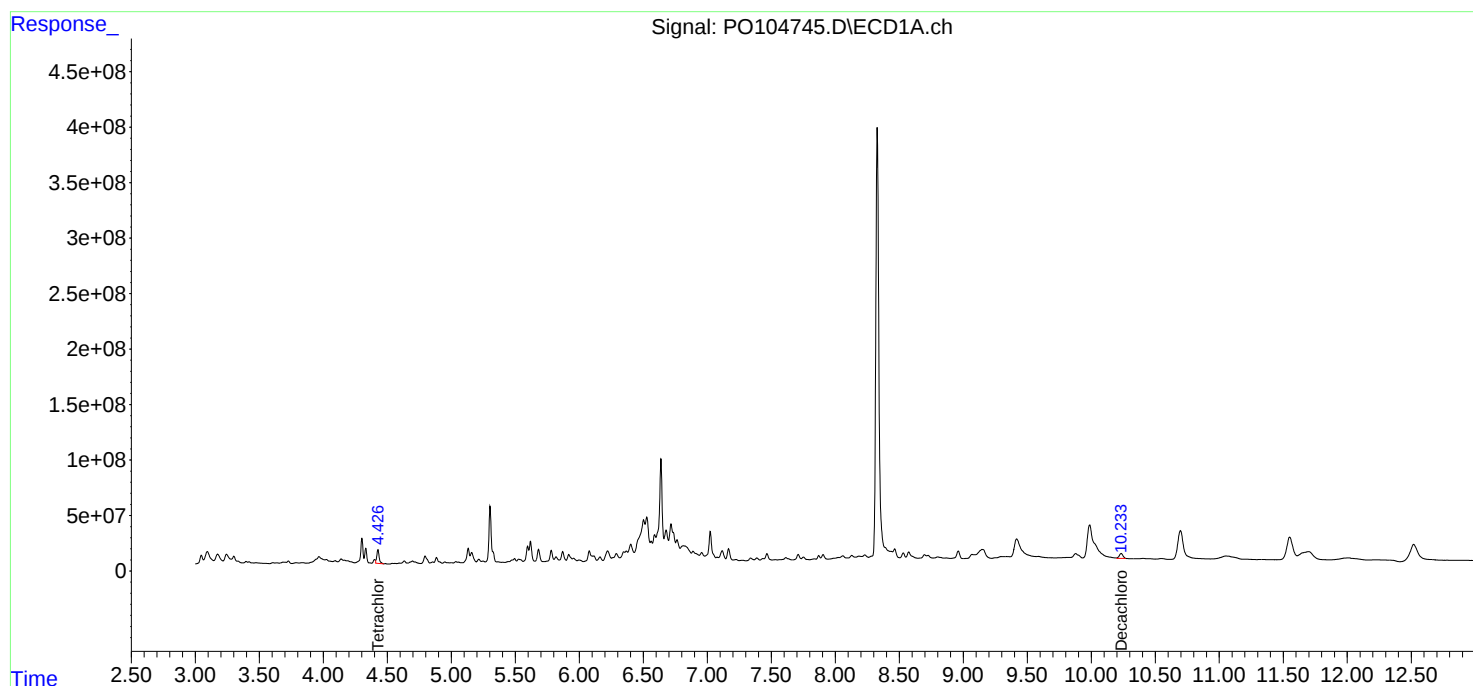

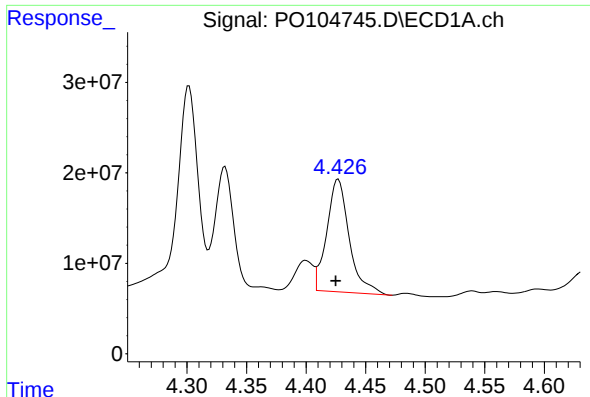

#1 Tetrachloro-m-xylene

R.T.: 4.427 min
Delta R.T.: 0.002 min
Response: 163551346
Conc: 18.27 ng/ml


Instrument :

ECD_O

ClientSampleId :
34806


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/12/2024
Supervised By :Ankita Jodhani 07/12/2024

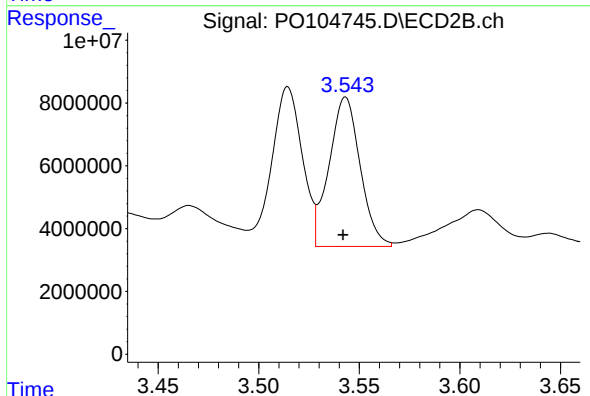


#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: 0.000 min
Response: 51024810
Conc: 15.64 ng/ml m

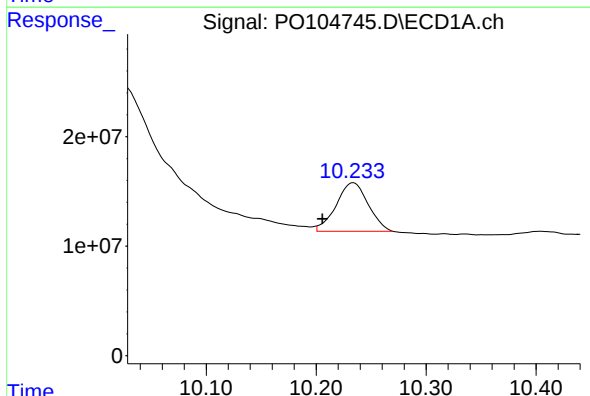

#2 Decachlorobiphenyl

R.T.: 10.233 min
Delta R.T.: 0.027 min
Response: 89409642
Conc: 14.58 ng/ml m

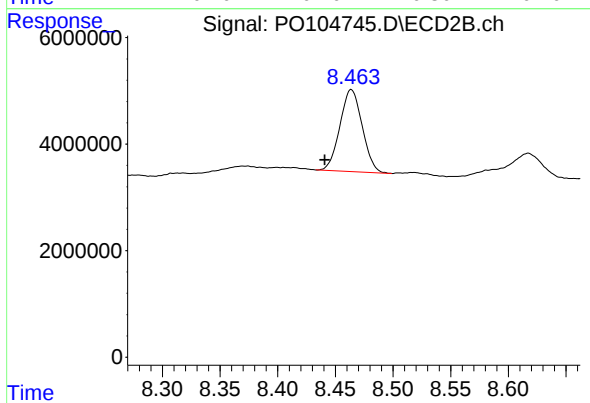

#2 Decachlorobiphenyl

R.T.: 8.463 min
Delta R.T.: 0.022 min
Response: 20571340
Conc: 9.81 ng/ml m