

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071124\
 Data File : P0104746.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2024 06:25
 Operator : YP/AJ
 Sample : P3208-09
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 3042

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/12/2024
 Supervised By :Ankita Jodhani 07/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 08:05:56 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070224.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 02 16:29:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.429	3.545	133.1E6	53901624	14.864	16.521
2) SA Decachlor...	10.224	8.450	54336357	20915369	8.860m	9.973

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071124\
Data File : PO104746.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2024 06:25
Operator : YP/AJ
Sample : P3208-09
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
3042


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/12/2024
Supervised By :Ankita Jodhani 07/12/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 08:05:56 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO070224.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 02 16:29:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

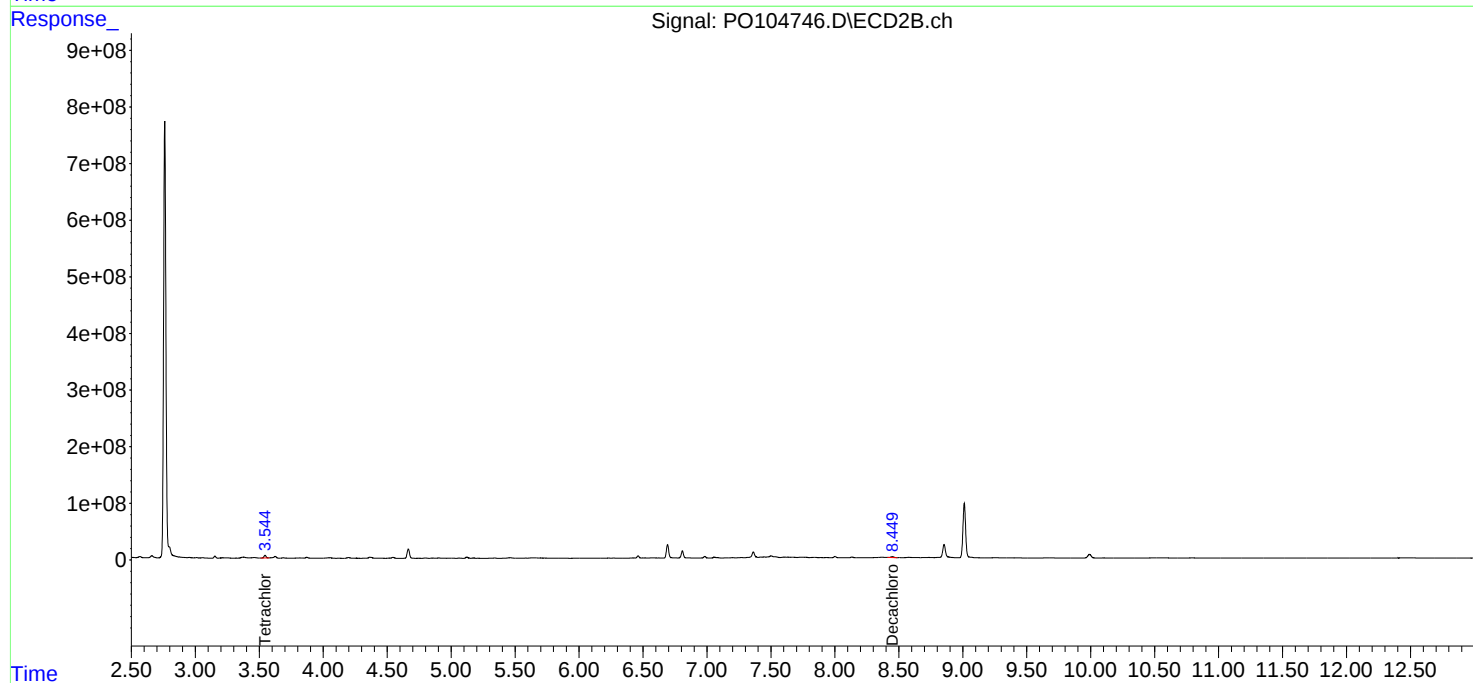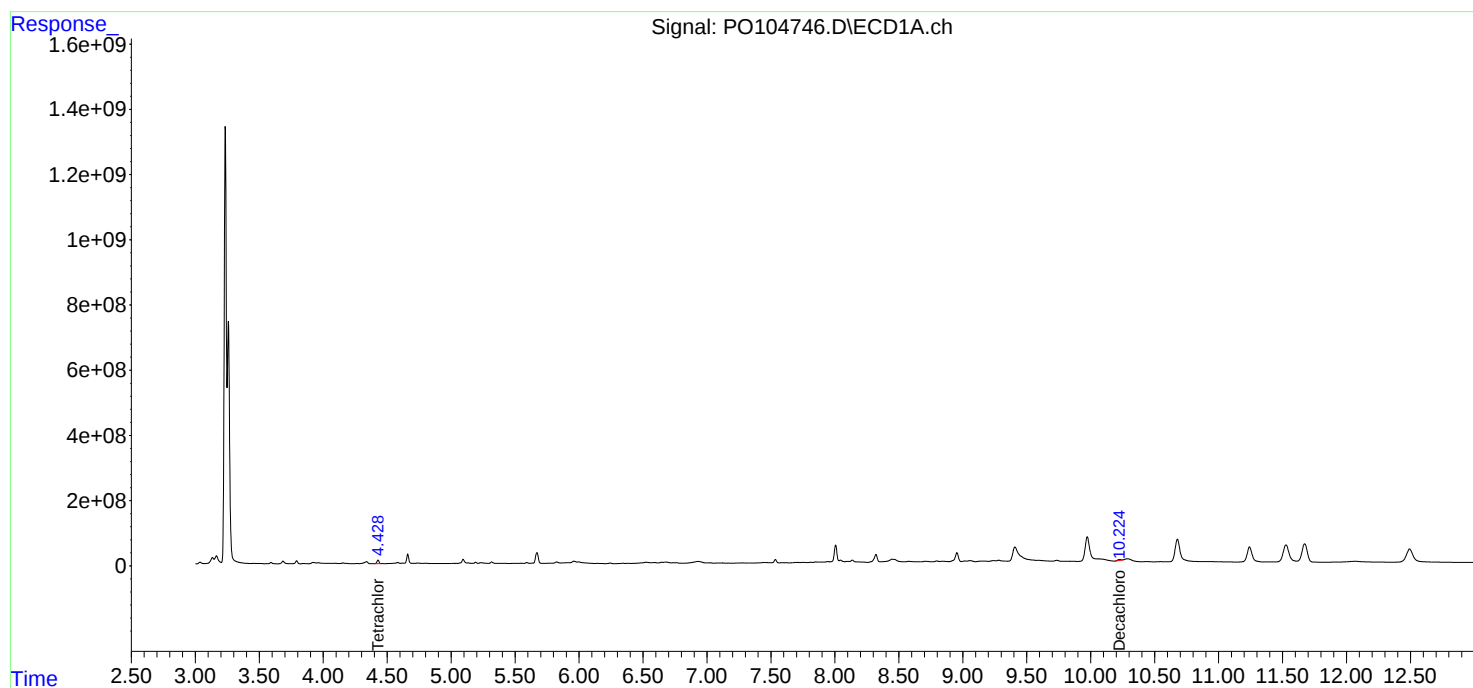

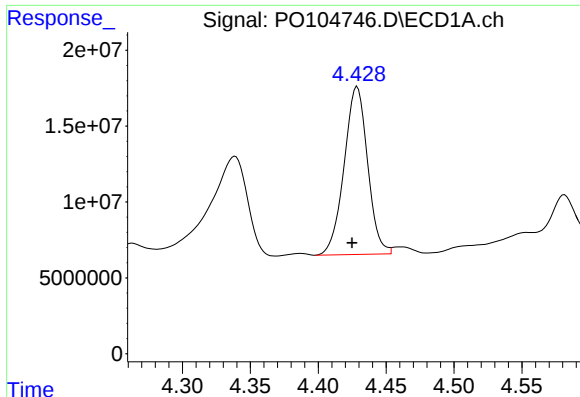


#1 Tetrachloro-m-xylene

R.T.: 4.429 min
Delta R.T.: 0.004 min
Response: 133086151
Conc: 14.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
3042


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/12/2024
Supervised By :Ankita Jodhani 07/12/2024

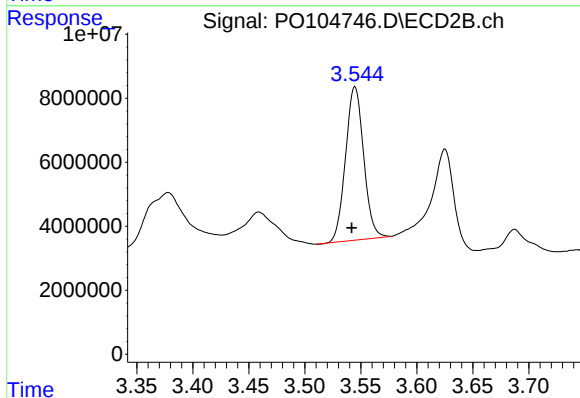


#1 Tetrachloro-m-xylene

R.T.: 3.545 min
Delta R.T.: 0.003 min
Response: 53901624
Conc: 16.52 ng/ml

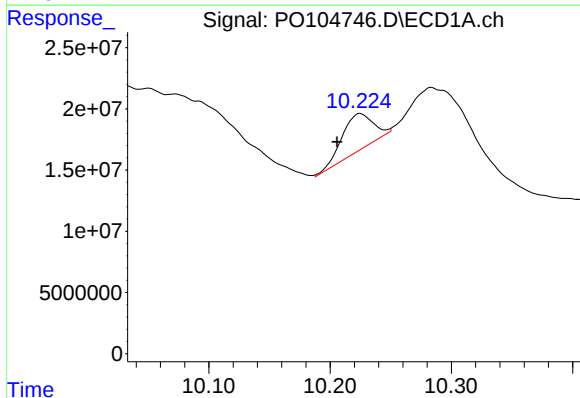

#2 Decachlorobiphenyl

R.T.: 10.224 min
Delta R.T.: 0.018 min
Response: 54336357
Conc: 8.86 ng/ml m

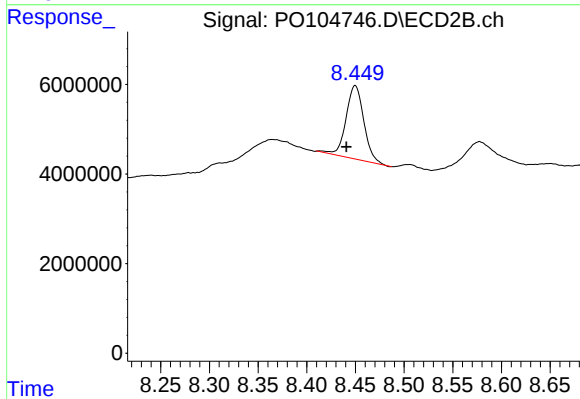

#2 Decachlorobiphenyl

R.T.: 8.450 min
Delta R.T.: 0.009 min
Response: 20915369
Conc: 9.97 ng/ml