

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0071218\
 Data File : P0046619.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Jul 2018 13:12
 Operator : SM/SJ
 Sample : J3912-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 GS-CONCRETE-PIPE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 15:00:48 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 09 15:27:34 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.208	3.532	4002595	4352085	16.748	20.489
2) SA Decachlor...	9.733	8.461	2677552	2709650	14.048	13.969

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071218\
Data File : P0046619.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jul 2018 13:12
Operator : SM/SJ
Sample : J3912-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
GS-CONCRETE-PIPE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 15:00:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

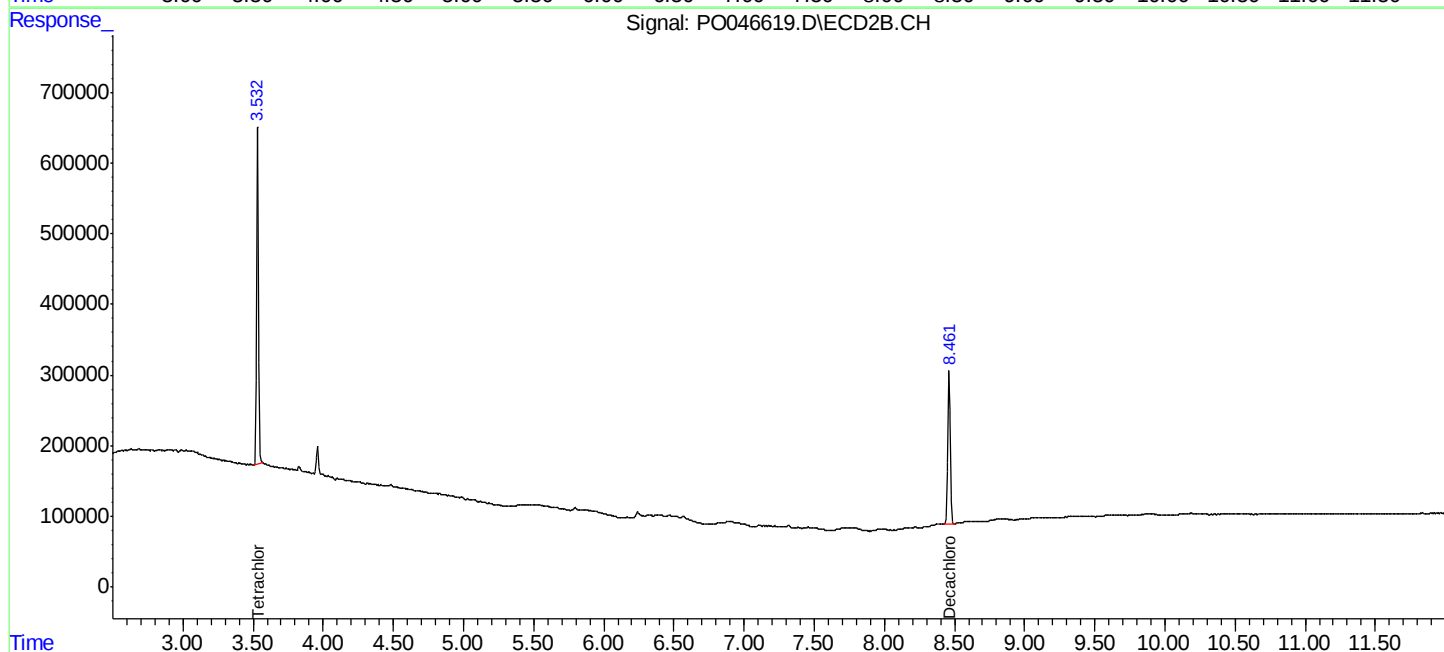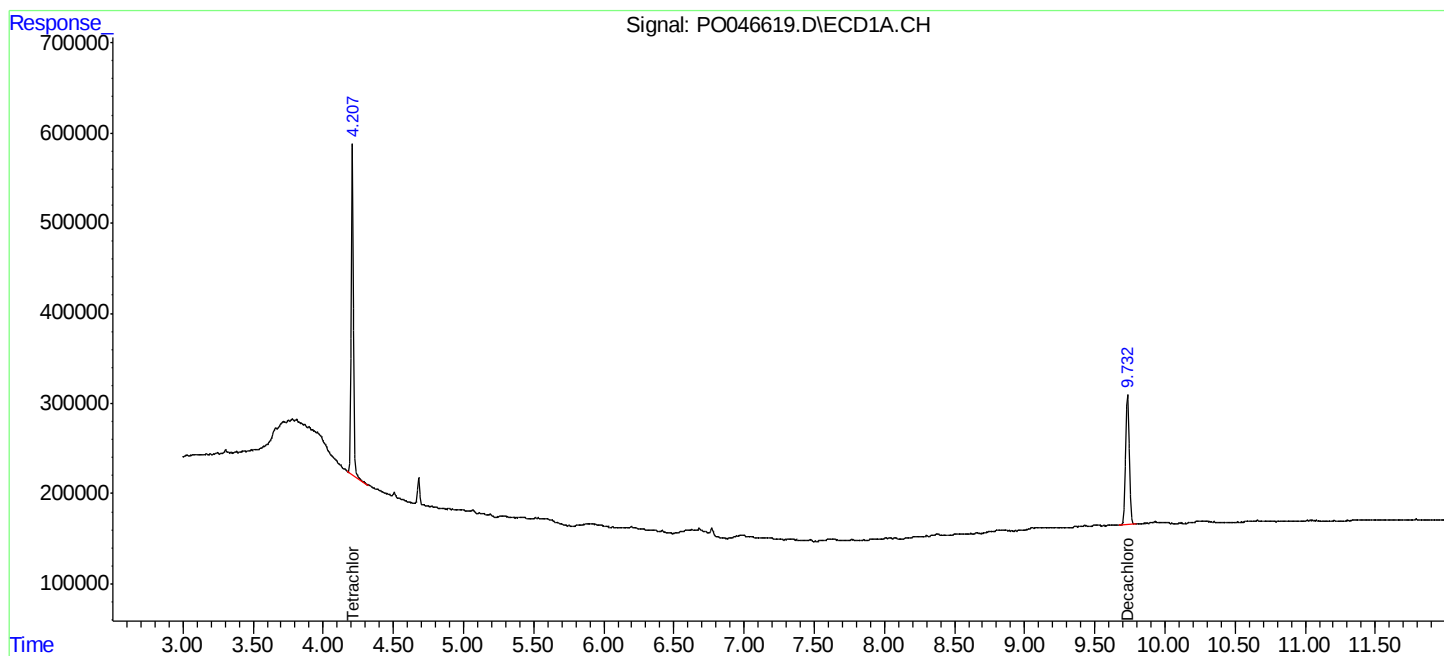


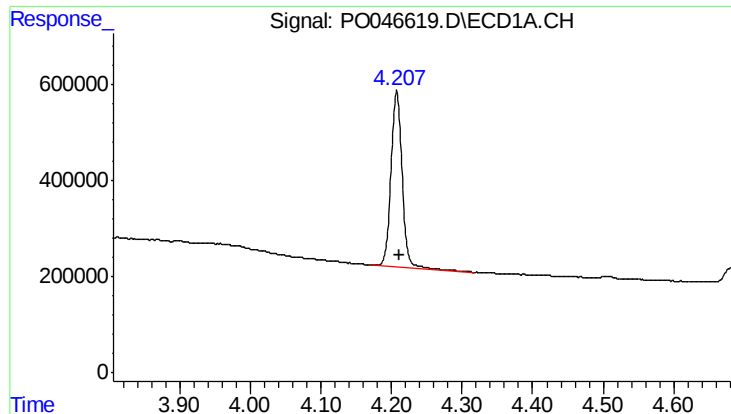

#1 Tetrachloro-m-xylene


R.T.: 4.208 min
Delta R.T.: -0.005 min
Response: 4002595
Conc: 16.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
GS-CONCRETE-PIPE

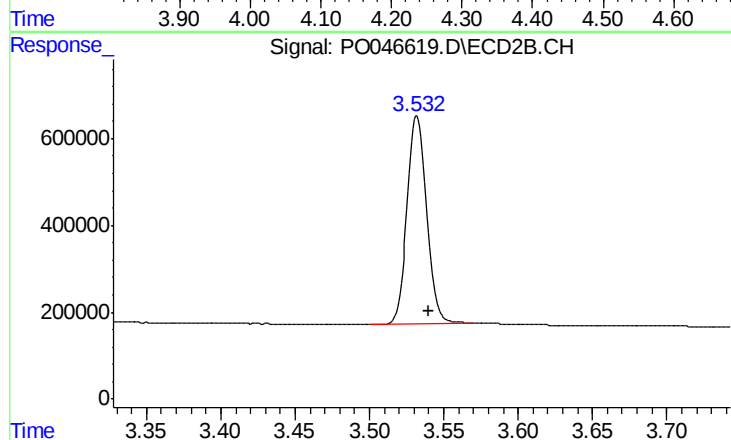


#1 Tetrachloro-m-xylene

R.T.: 3.532 min
Delta R.T.: -0.008 min
Response: 4352085
Conc: 20.49 ng/ml

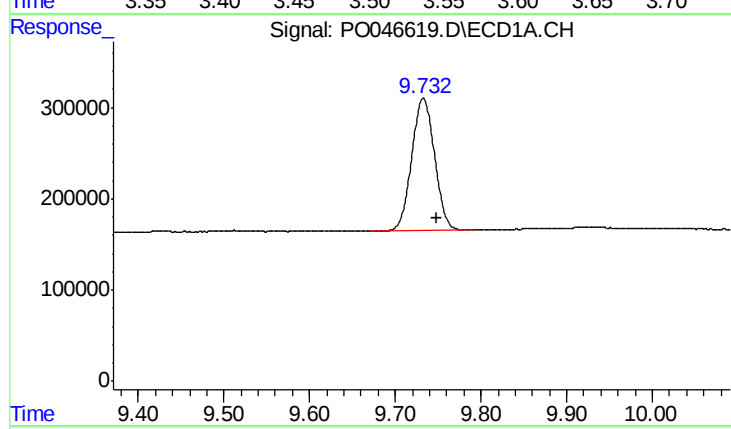

#2 Decachlorobiphenyl

R.T.: 9.733 min
Delta R.T.: -0.015 min
Response: 2677552
Conc: 14.05 ng/ml

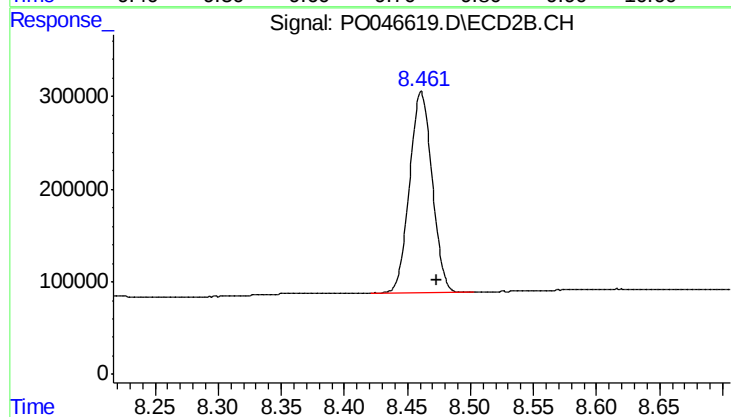

#2 Decachlorobiphenyl

R.T.: 8.461 min
Delta R.T.: -0.012 min
Response: 2709650
Conc: 13.97 ng/ml