

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0071218\
Data File : P0046631.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jul 2018 19:11
Operator : SM/SJ
Sample : J3934-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TS-BASELINE-WATER

Manual Integrations
APPROVED

Sohil
7/13/2018 2:19:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 04:46:17 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.207	3.531	2399347	2630445	10.040m	12.384m
2) SA Decachlor...	9.731	8.459	948972	1043279	4.979m	5.378

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071218\
Data File : P0046631.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jul 2018 19:11
Operator : SM/SJ
Sample : J3934-01
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TS-BASELINE-WATER


Manual Integrations
APPROVED

Sohil
7/13/2018 2:19:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 04:46:17 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

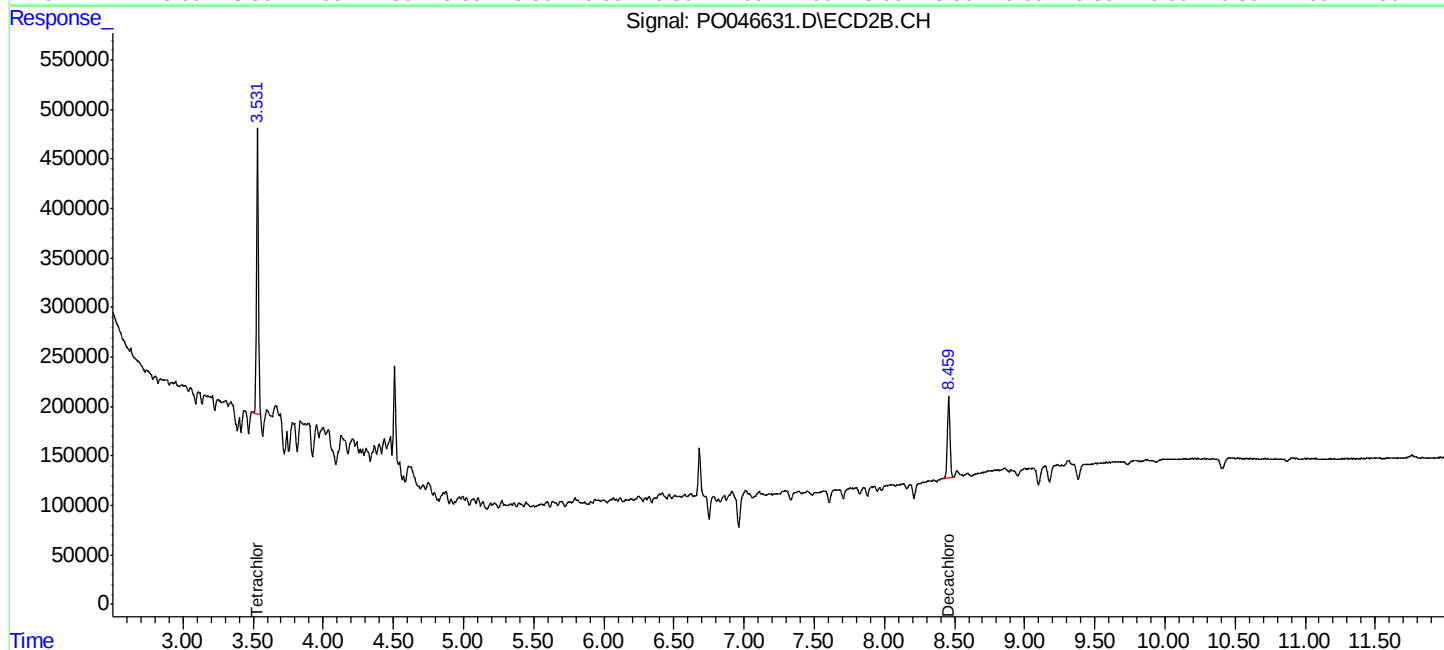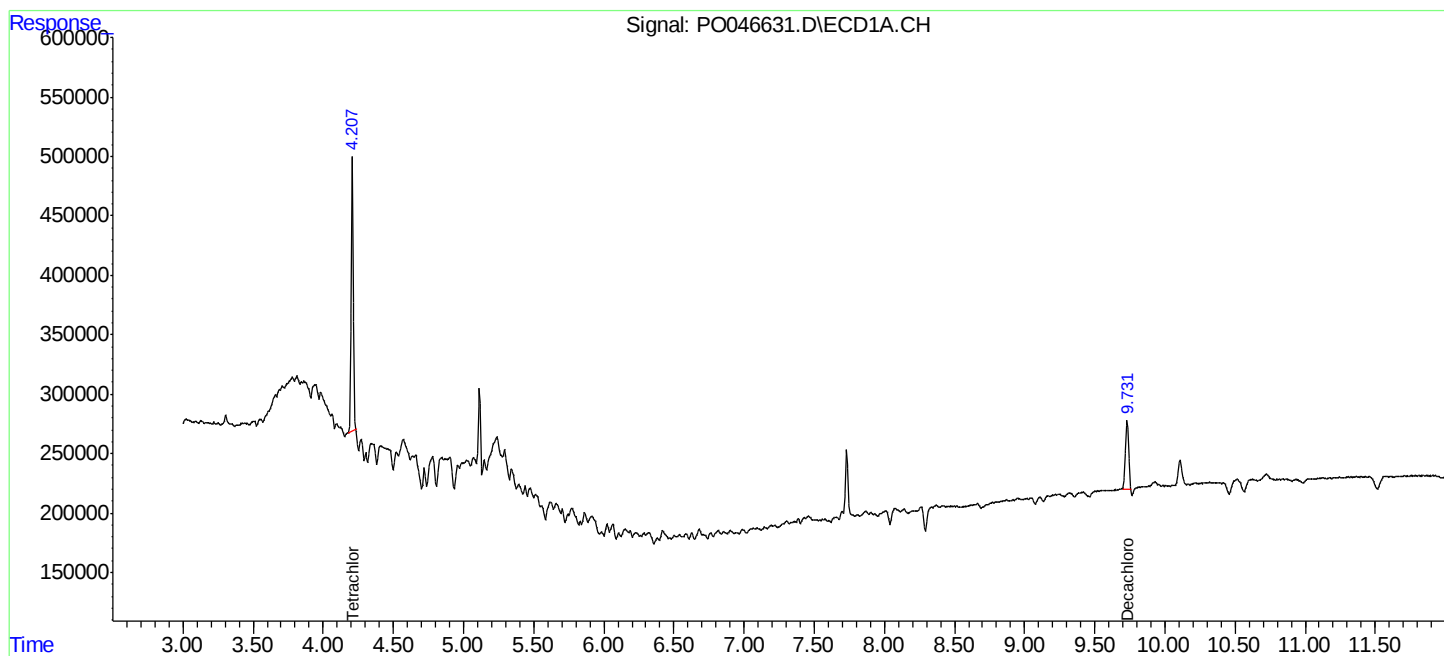

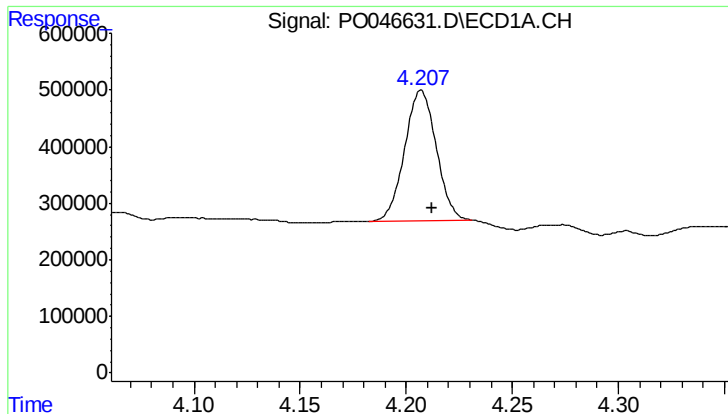


#1 Tetrachloro-m-xylene

R.T.: 4.207 min
Delta R.T.: -0.006 min
Response: 2399347
Conc: 10.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
TS-BASELINE-WATER


Manual Integrations
APPROVED

Sohil
7/13/2018 2:19:27 PM

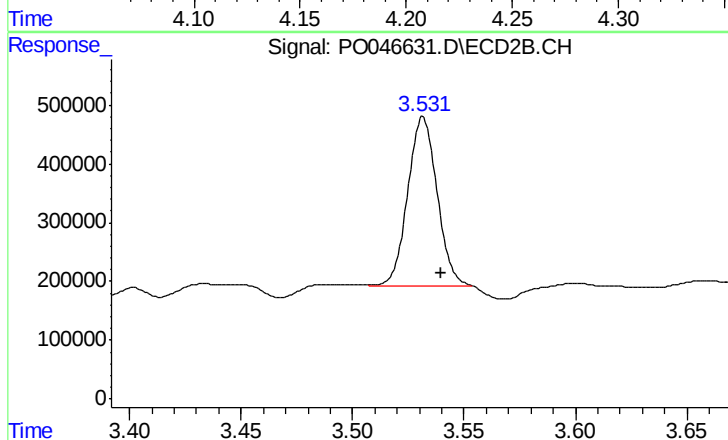


#1 Tetrachloro-m-xylene

R.T.: 3.531 min
Delta R.T.: -0.008 min
Response: 2630445
Conc: 12.38 ng/ml m

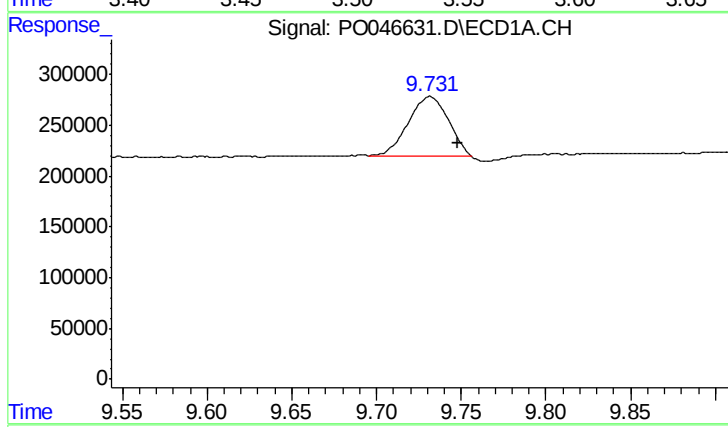

#2 Decachlorobiphenyl

R.T.: 9.731 min
Delta R.T.: -0.017 min
Response: 948972
Conc: 4.98 ng/ml m

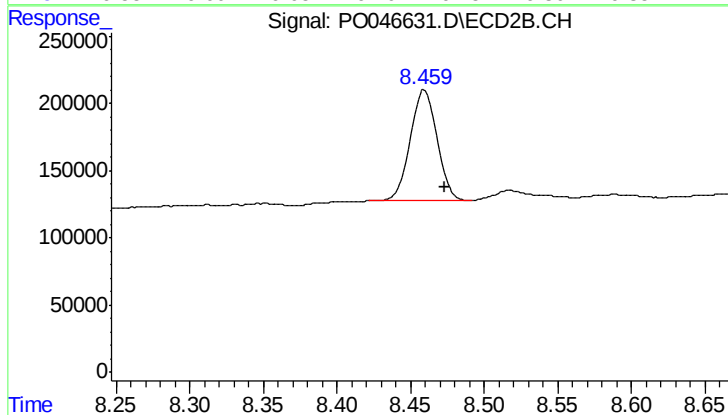

#2 Decachlorobiphenyl

R.T.: 8.459 min
Delta R.T.: -0.014 min
Response: 1043279
Conc: 5.38 ng/ml