

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0071218\
Data File : P0046677.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jul 2018 11:40
Operator : SM/SJ
Sample : J3903-03
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
KS-T-3

Manual Integrations
APPROVED

Sohil
7/13/2018 2:38:29 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 14:18:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.199	3.523	4225395	3569847	17.681m	16.807
2) SA Decachlor...	9.721	8.451	2815223	2819710	14.770	14.536

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0071218\
Data File : P0046677.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jul 2018 11:40
Operator : SM/SJ
Sample : J3903-03
Misc :
ALS Vial : 56 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KS-T-3


Manual Integrations
APPROVED

Sohil
7/13/2018 2:38:29 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 14:18:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

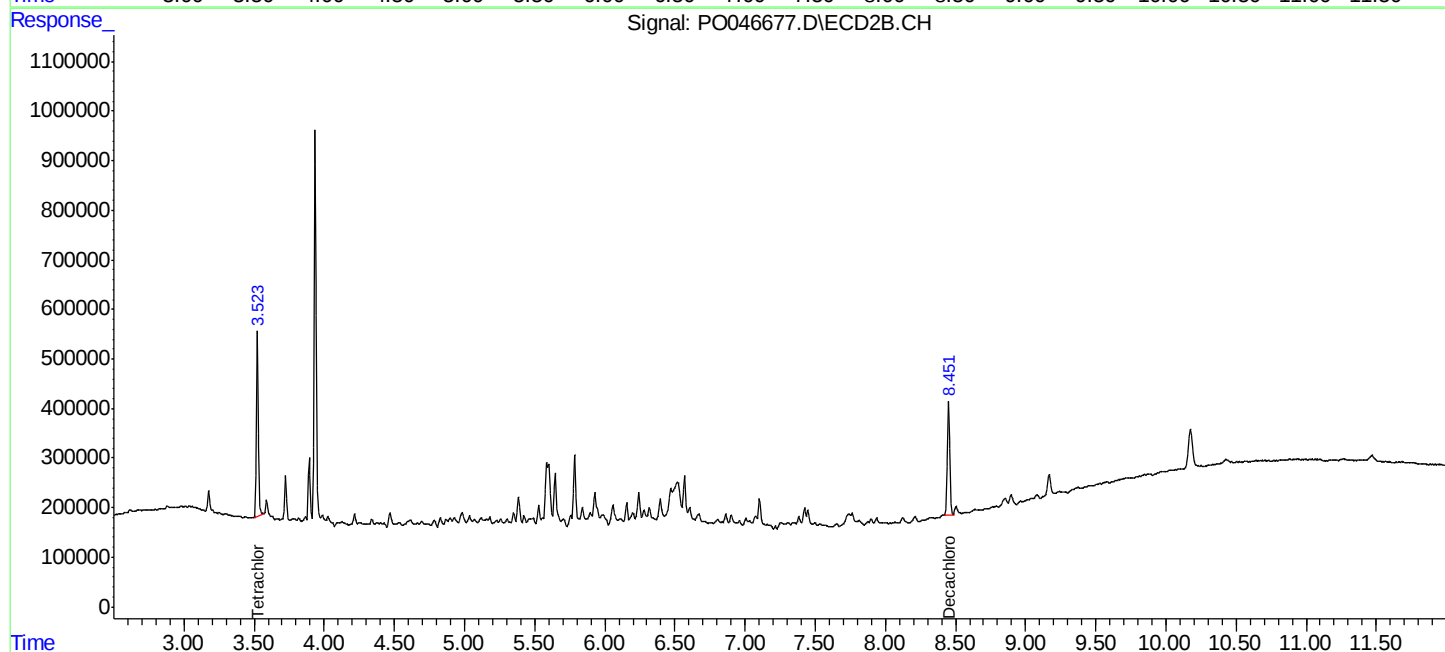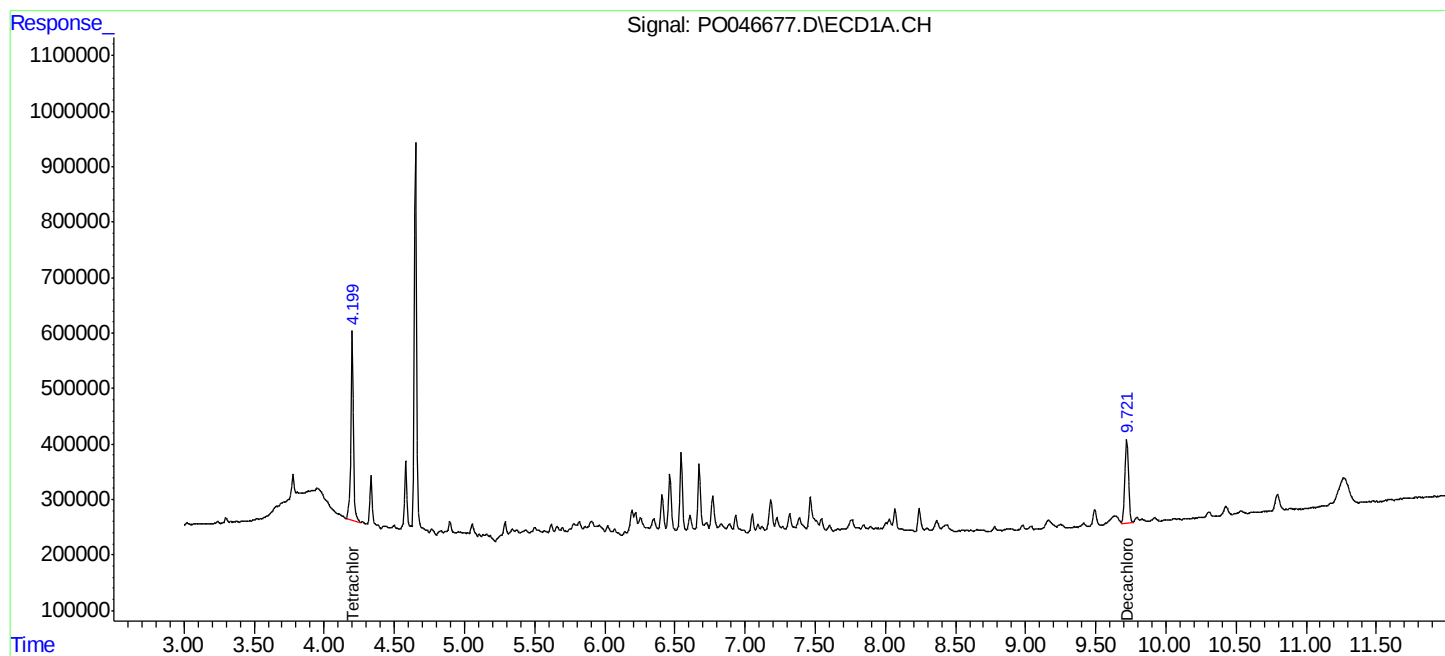

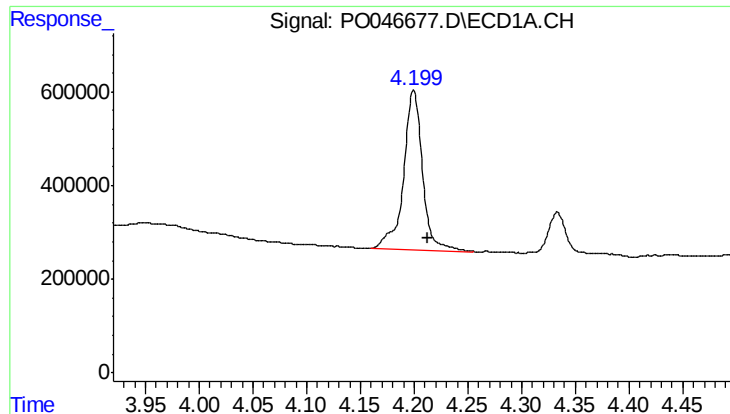


#1 Tetrachloro-m-xylene

R.T.: 4.199 min
Delta R.T.: -0.013 min
Response: 4225395
Conc: 17.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
KS-T-3


Manual Integrations
APPROVED

Sohil
7/13/2018 2:38:29 PM

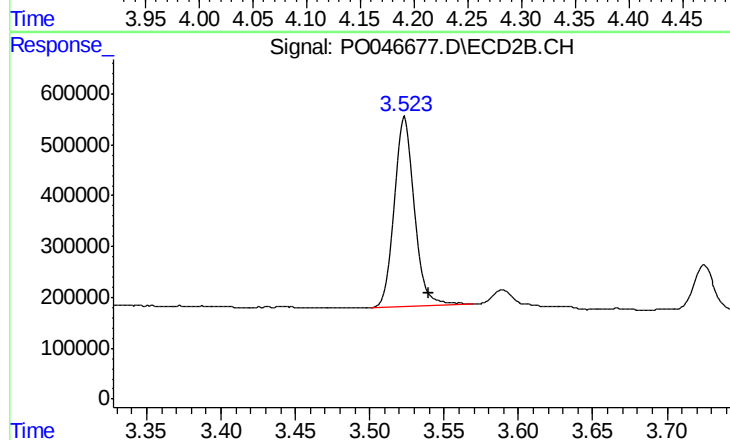


#1 Tetrachloro-m-xylene

R.T.: 3.523 min
Delta R.T.: -0.016 min
Response: 3569847
Conc: 16.81 ng/ml

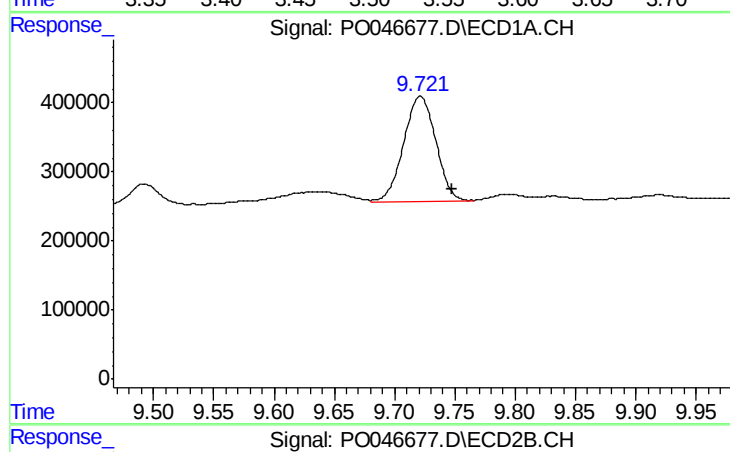

#2 Decachlorobiphenyl

R.T.: 9.721 min
Delta R.T.: -0.027 min
Response: 2815223
Conc: 14.77 ng/ml

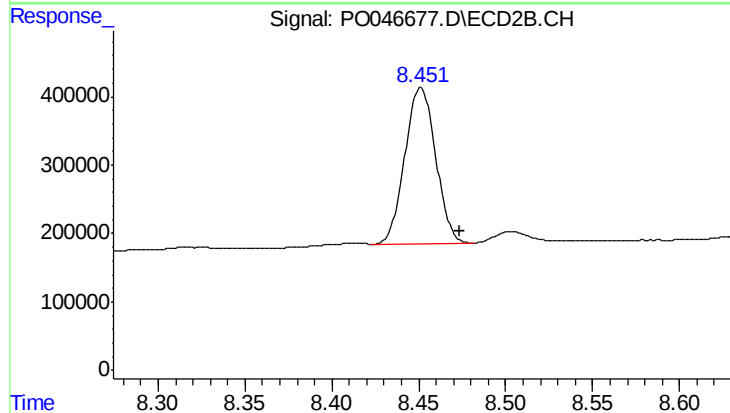

#2 Decachlorobiphenyl

R.T.: 8.451 min
Delta R.T.: -0.022 min
Response: 2819710
Conc: 14.54 ng/ml