

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0071218\
 Data File : P0046679.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jul 2018 12:11
 Operator : SM/SJ
 Sample : J3981-01 10X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 A460198

Manual Integrations
 APPROVED

Sohil
 7/13/2018 2:38:31 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 13:29:28 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 09 15:27:34 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.197	3.549	443131	96418	1.854	0.454m#
2) SA Decachlor...	9.720	8.452	283517	254448	1.487m	1.312m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071218\
Data File : P0046679.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jul 2018 12:11
Operator : SM/SJ
Sample : J3981-01 10X
Misc :
ALS Vial : 58 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
A460198


Manual Integrations
APPROVED

Sohil
7/13/2018 2:38:31 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 13:29:28 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

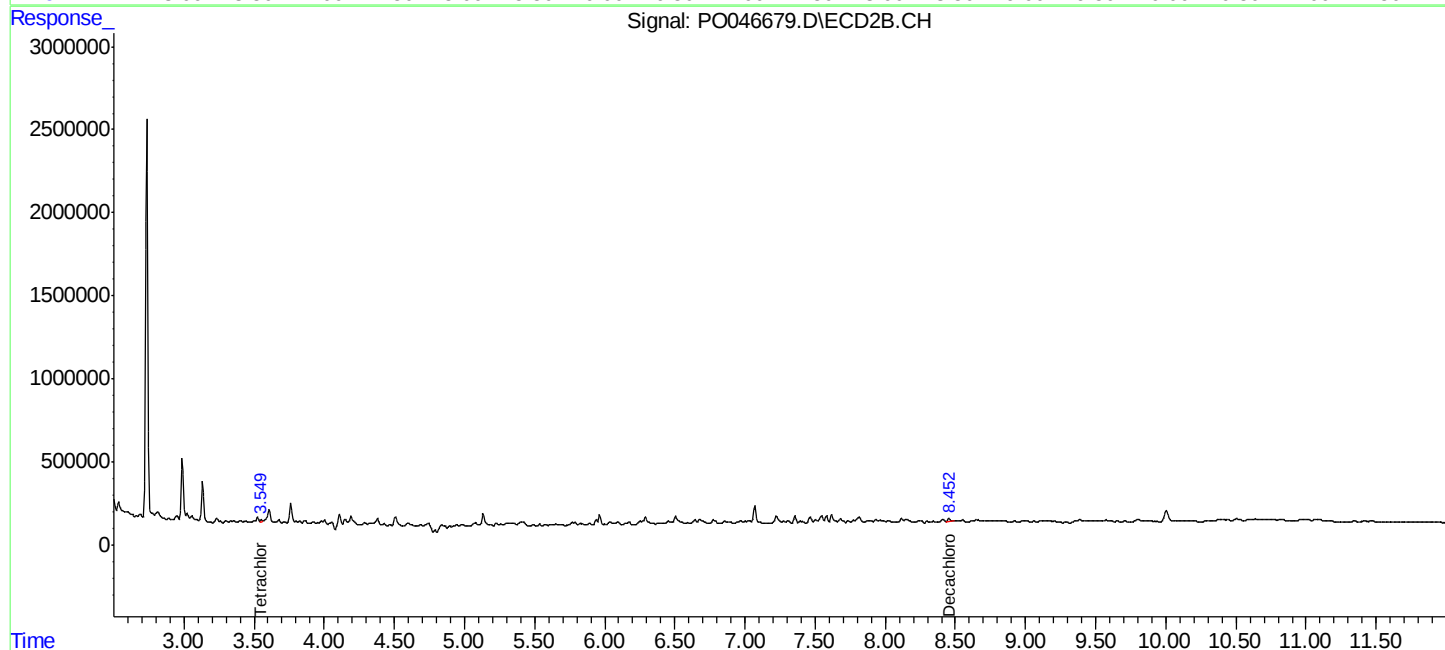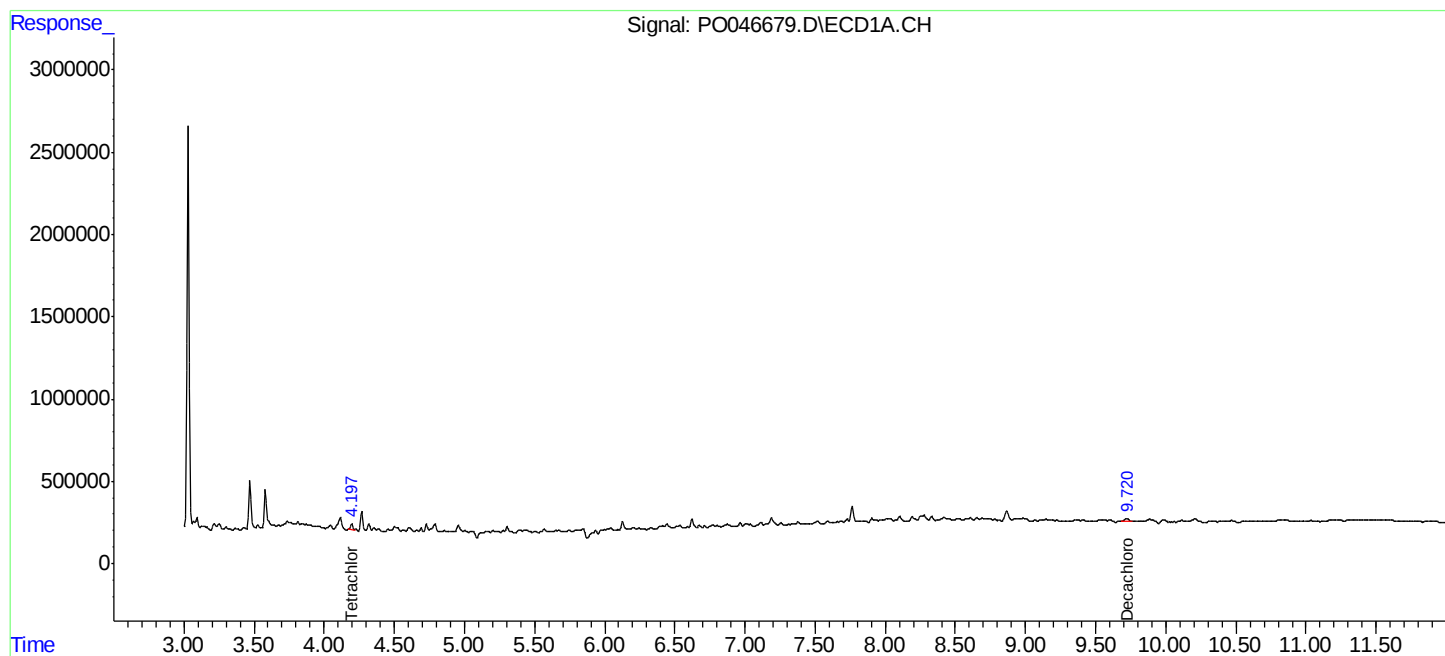

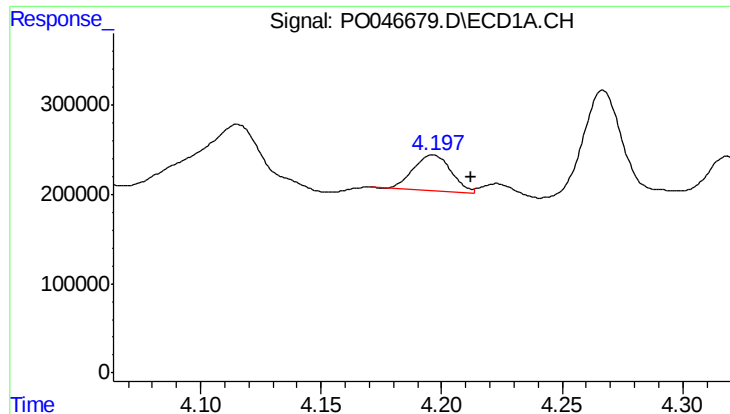


#1 Tetrachloro-m-xylene

R.T.: 4.197 min
Delta R.T.: -0.016 min
Response: 443131
Conc: 1.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
A460198


Manual Integrations
APPROVED

Sohil
7/13/2018 2:38:31 PM

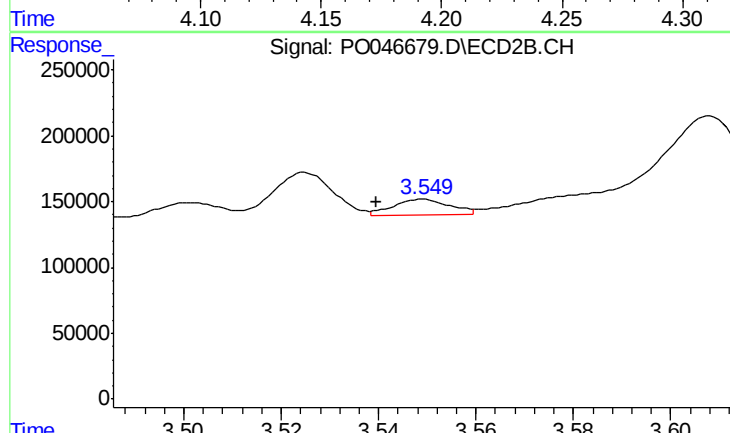


#1 Tetrachloro-m-xylene

R.T.: 3.549 min
Delta R.T.: 0.010 min
Response: 96418
Conc: 0.45 ng/ml m

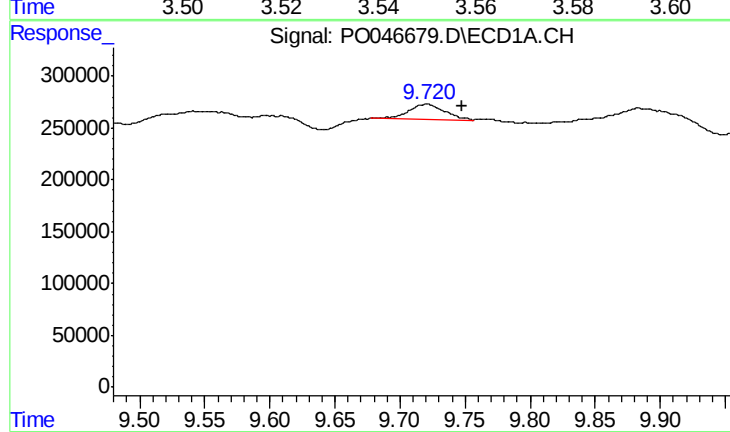

#2 Decachlorobiphenyl

R.T.: 9.720 min
Delta R.T.: -0.028 min
Response: 283517
Conc: 1.49 ng/ml m

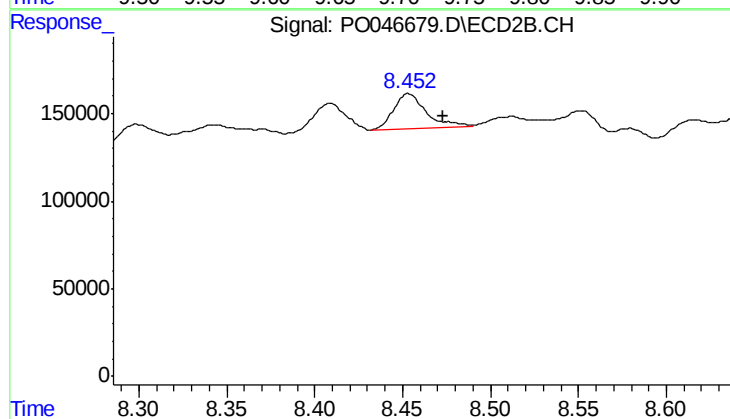

#2 Decachlorobiphenyl

R.T.: 8.452 min
Delta R.T.: -0.021 min
Response: 254448
Conc: 1.31 ng/ml m