

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071221\
 Data File : P0079511.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Jul 2021 18:27
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 07:05:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 10 00:52:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.021	4.230	1452906	582582	21.731	20.316
2)	SA Decachlor...	11.143	9.680	1165520	560051	22.916	21.162
Target Compounds							
8)	L2 AR-1221-1	5.274	0.000	35128	0	49.575	N.D. #
9)	L2 AR-1221-2	5.378	0.000	17455	0	33.669	N.D. #
15)	L3 AR-1232-5	6.643	0.000	20754	0	43.770	N.D. #
22)	L5 AR-1248-2	6.643	0.000	20754	0	11.164	N.D. #
24)	L5 AR-1248-4	7.270f	0.000	11847	0	4.872	N.D. #
26)	L6 AR-1254-1	7.270	0.000	11847	0	5.129	N.D. #
28)	L6 AR-1254-3	7.894	0.000	16018	0	4.259	N.D. #
32)	L7 AR-1260-2	8.319	0.000	5789	0	1.838	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071221\
Data File : P0079511.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jul 2021 18:27
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 07:05:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 10 00:52:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

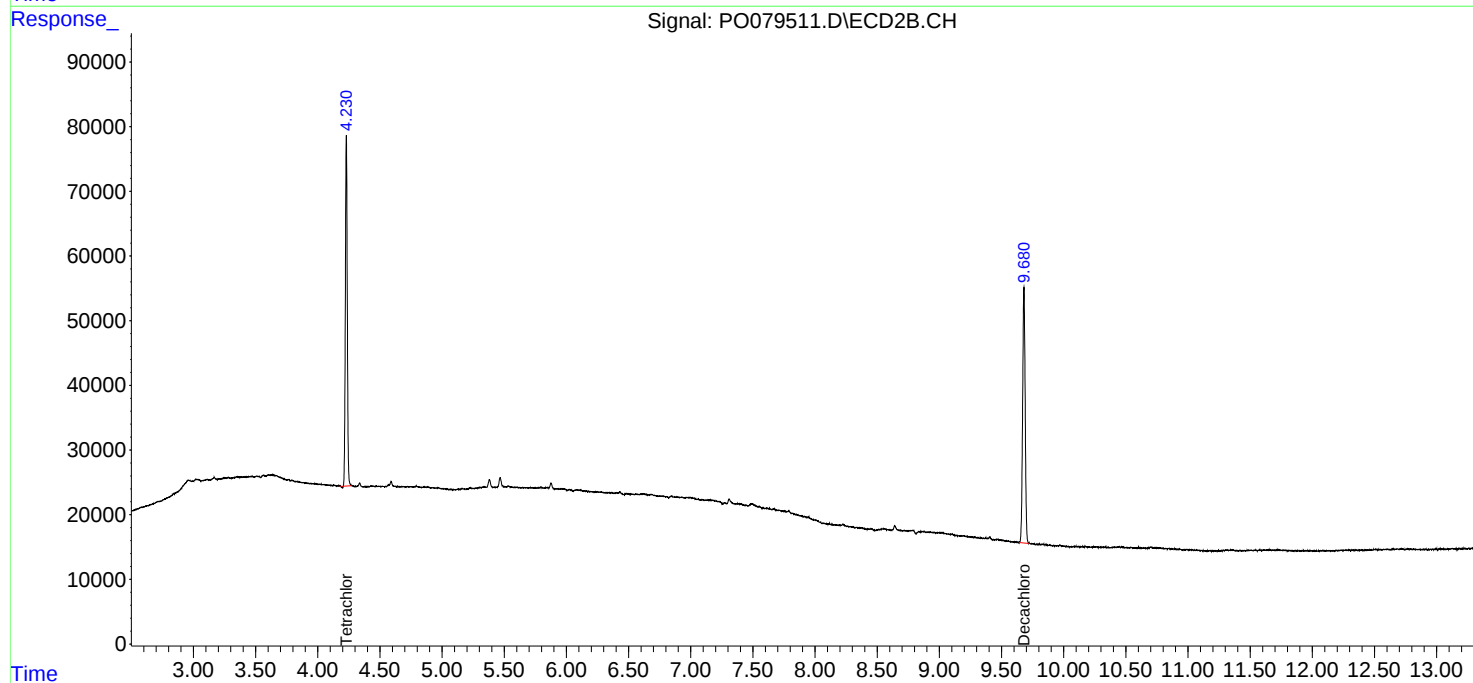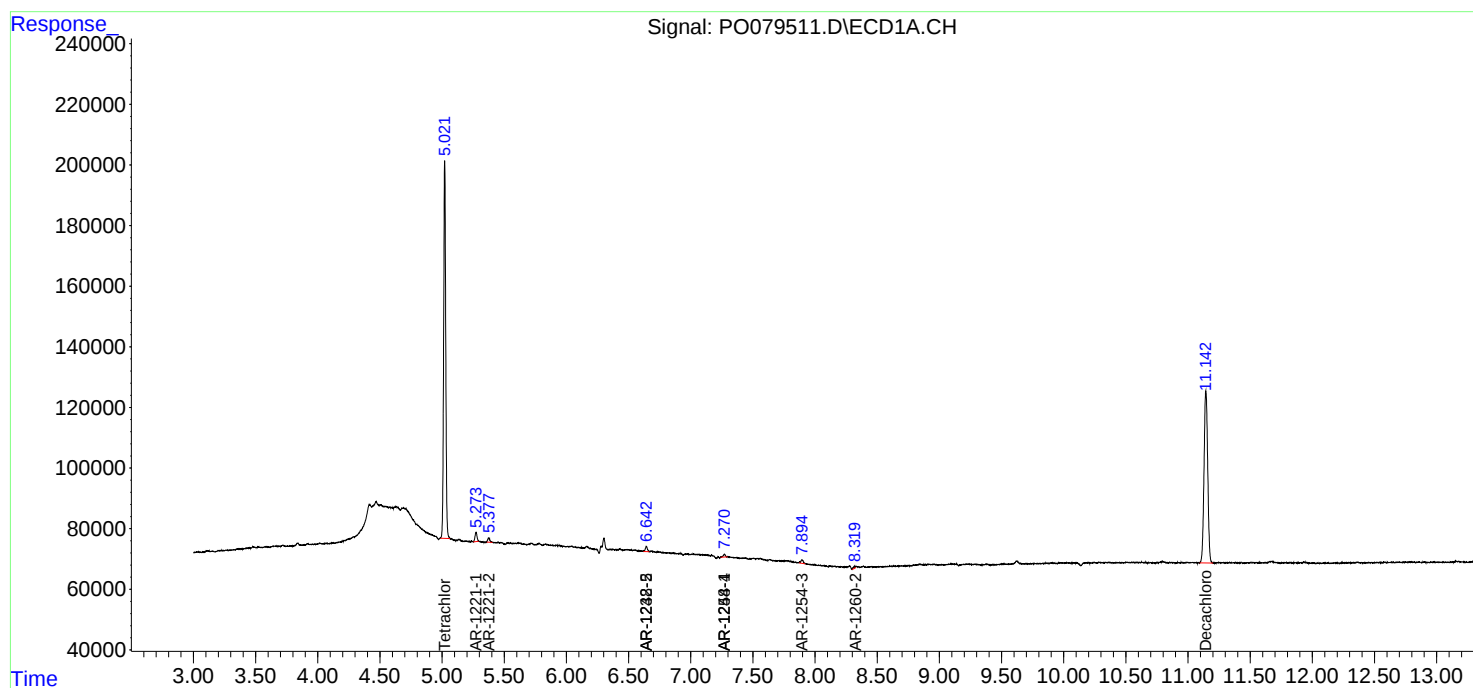


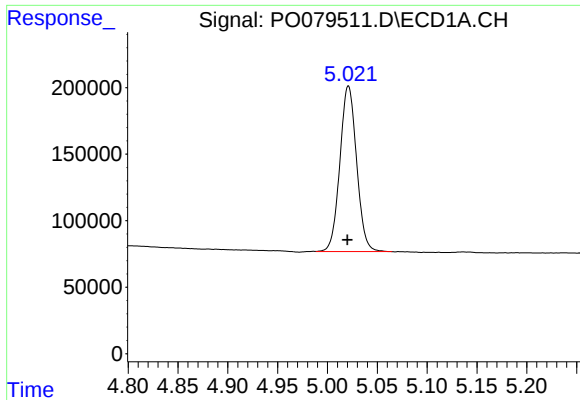

#1 Tetrachloro-m-xylene


R.T.: 5.021 min
Delta R.T.: 0.001 min
Response: 1452906
Conc: 21.73 ng/ml

Instrument :
ECD_O
ClientSampleId :

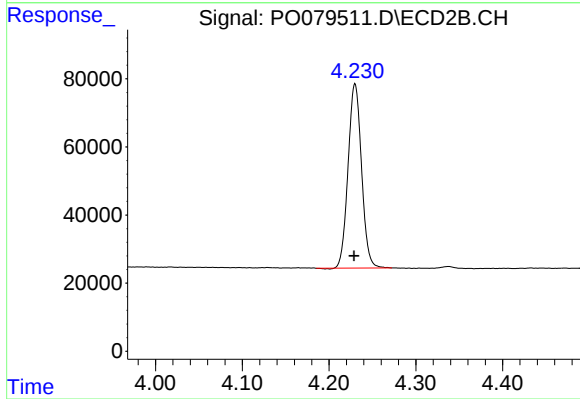


#1 Tetrachloro-m-xylene

R.T.: 4.230 min
Delta R.T.: 0.001 min
Response: 582582
Conc: 20.32 ng/ml

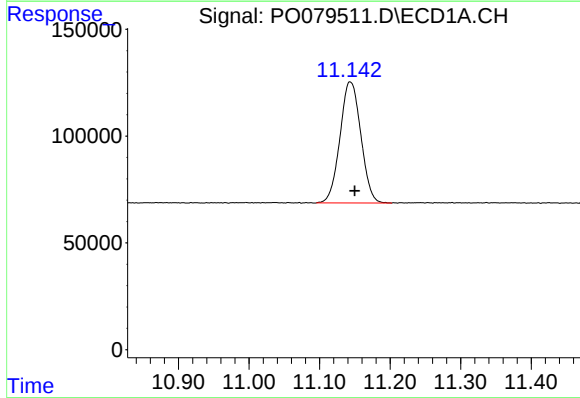


#2 Decachlorobiphenyl

R.T.: 11.143 min
Delta R.T.: -0.007 min
Response: 1165520
Conc: 22.92 ng/ml

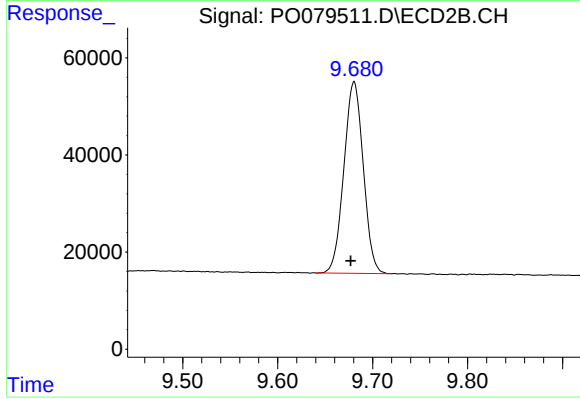

#2 Decachlorobiphenyl


R.T.: 9.680 min
Delta R.T.: 0.003 min
Response: 560051
Conc: 21.16 ng/ml

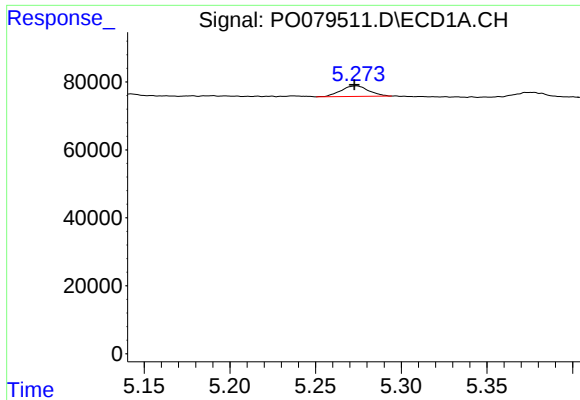

#8 AR-1221-1


R.T.: 5.274 min
Delta R.T.: 0.001 min
Response: 35128
Conc: 49.58 ng/ml

Instrument :
ECD_O
ClientSampleId :

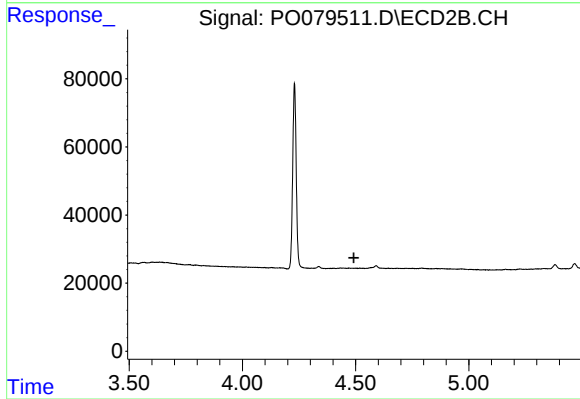


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.492 min
Response: 0
Conc: N.D.

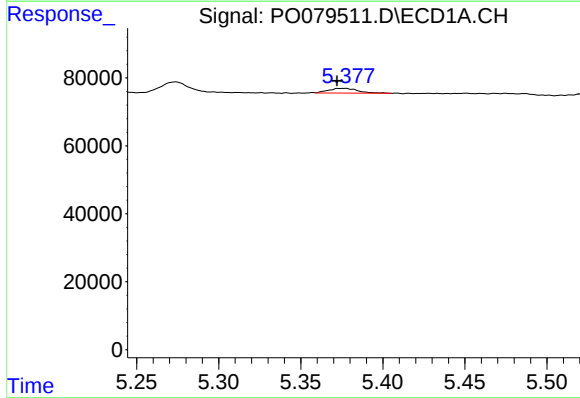


#9 AR-1221-2

R.T.: 5.378 min
Delta R.T.: 0.005 min
Response: 17455
Conc: 33.67 ng/ml

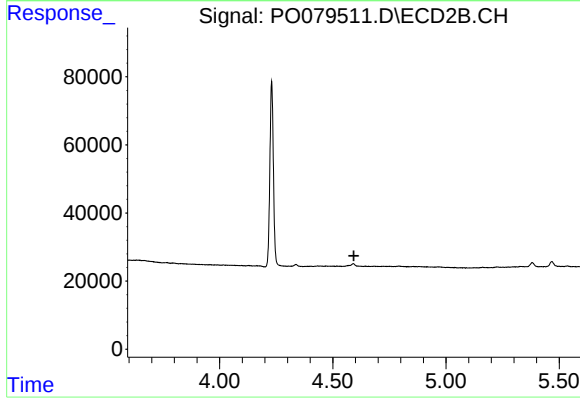

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.593 min
Response: 0
Conc: N.D.

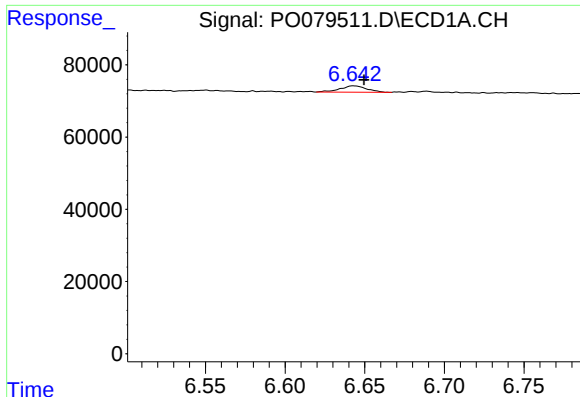

#15 AR-1232-5


R.T.: 6.643 min
Delta R.T.: -0.007 min
Response: 20754
Conc: 43.77 ng/ml

Instrument :
ECD_O
ClientSampleId :

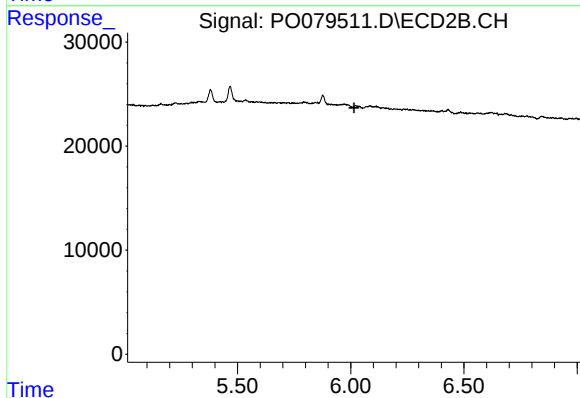


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 6.014 min
Response: 0
Conc: N.D.

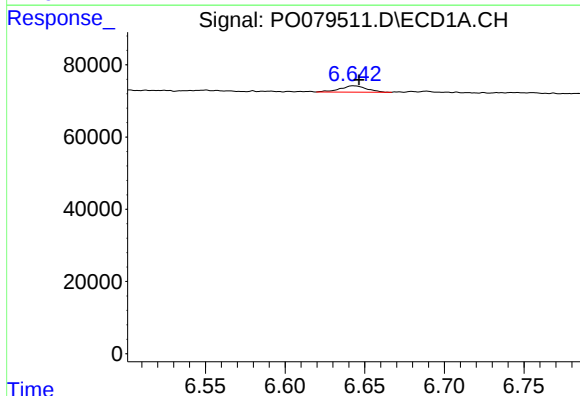


#22 AR-1248-2

R.T.: 6.643 min
Delta R.T.: -0.004 min
Response: 20754
Conc: 11.16 ng/ml

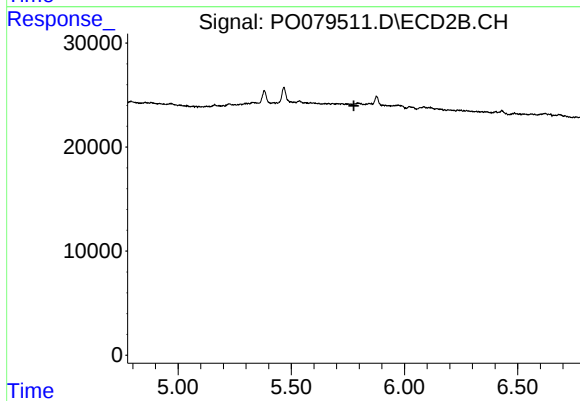

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T. : 5.776 min
Response: 0
Conc: N.D.

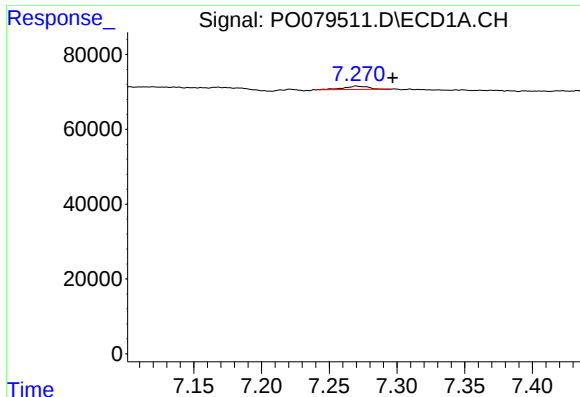

#24 AR-1248-4


R.T.: 7.270 min
Delta R.T.: -0.027 min
Response: 11847
Conc: 4.87 ng/ml

Instrument :
ECD_O
ClientSampleId :

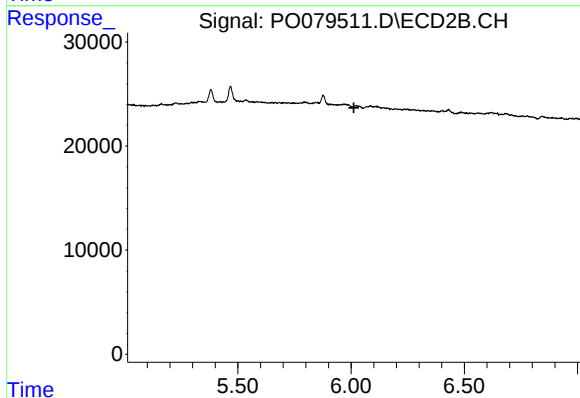


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 6.012 min
Response: 0
Conc: N.D.

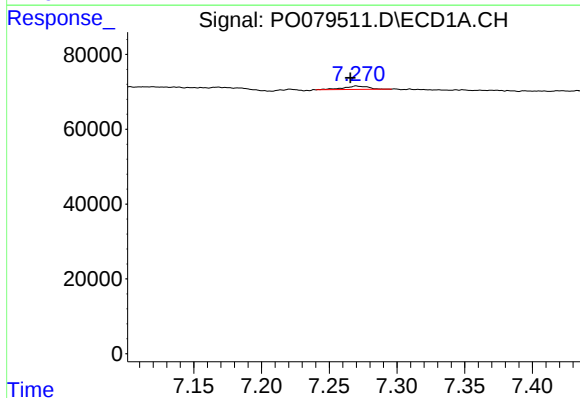


#26 AR-1254-1

R.T.: 7.270 min
Delta R.T.: 0.004 min
Response: 11847
Conc: 5.13 ng/ml

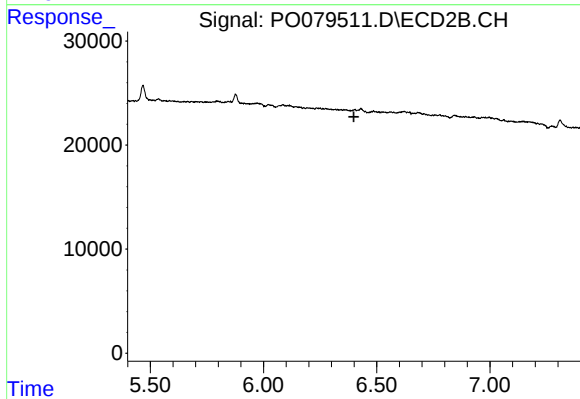

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.399 min
Response: 0
Conc: N.D.

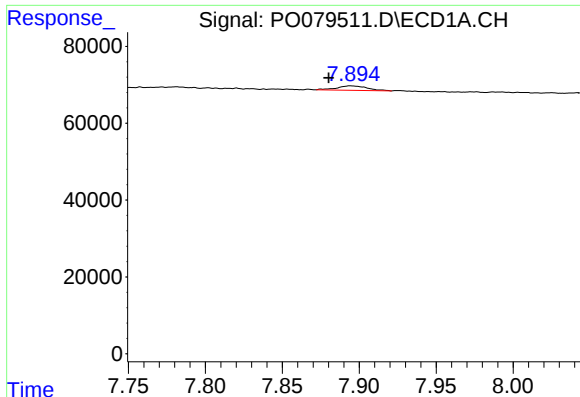

#28 AR-1254-3


R.T.: 7.894 min
Delta R.T.: 0.014 min
Response: 16018
Conc: 4.26 ng/ml

Instrument :
ECD_O
ClientSampleId :

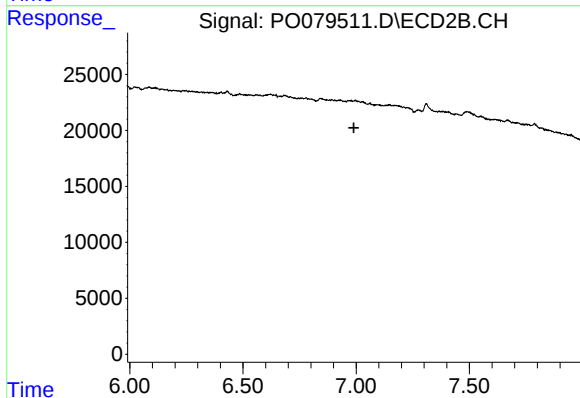


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.990 min
Response: 0
Conc: N.D.

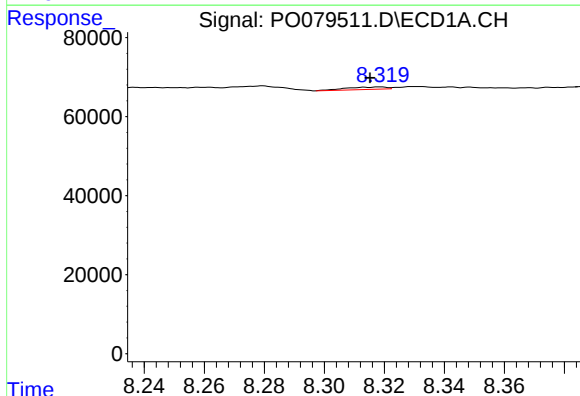

#32 AR-1260-2

R.T.: 8.319 min
Delta R.T.: 0.003 min
Response: 5789
Conc: 1.84 ng/ml

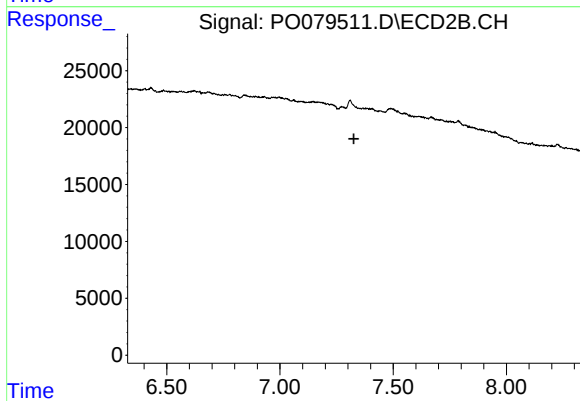

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.327 min
Response: 0
Conc: N.D.