

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071221\
 Data File : P0079506.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Jul 2021 17:01
 Operator : DD\AJ
 Sample : M3006-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CL-02-070921

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 07:03:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 10 00:52:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.019	4.228	1656407	649852	24.774	22.661
2) SA Decachlor...	11.142	9.675	1222361	563373	24.033	21.287

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071221\
Data File : P0079506.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jul 2021 17:01
Operator : DD\AJ
Sample : M3006-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CL-02-070921

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 07:03:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 10 00:52:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

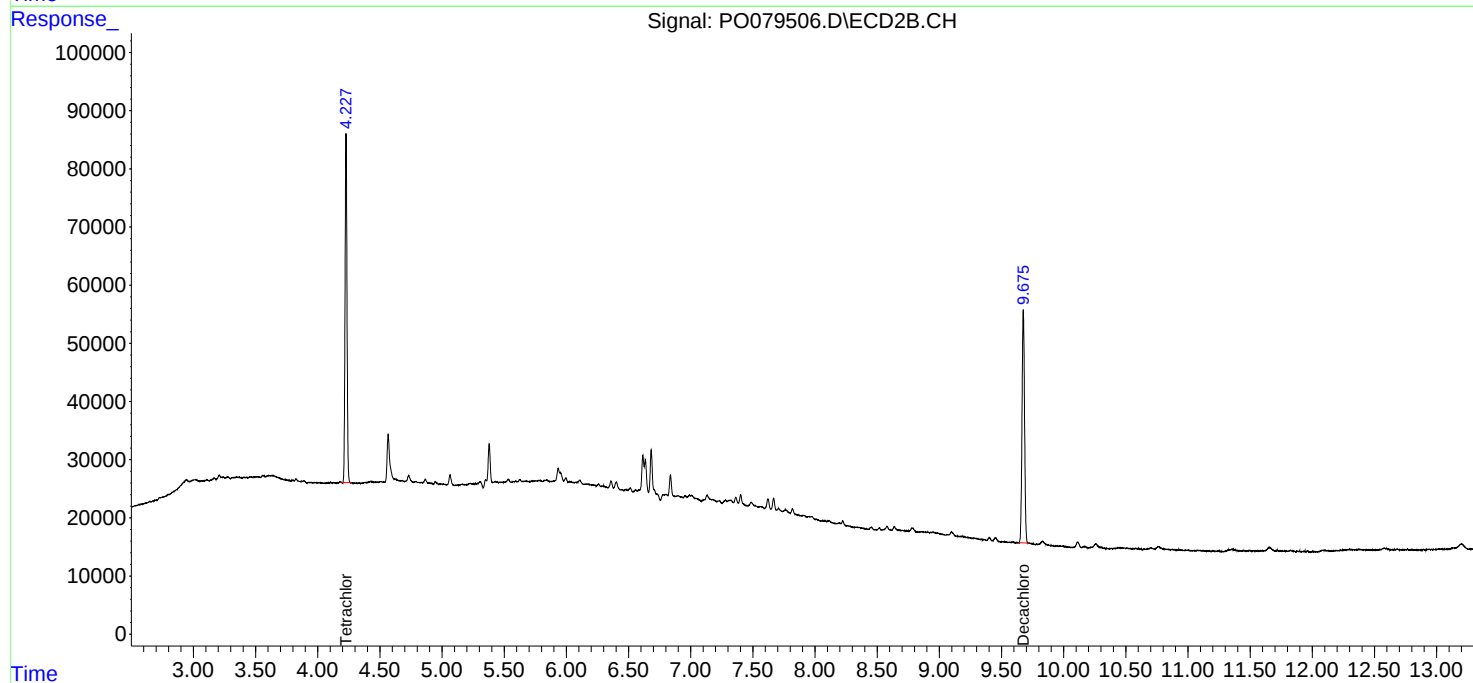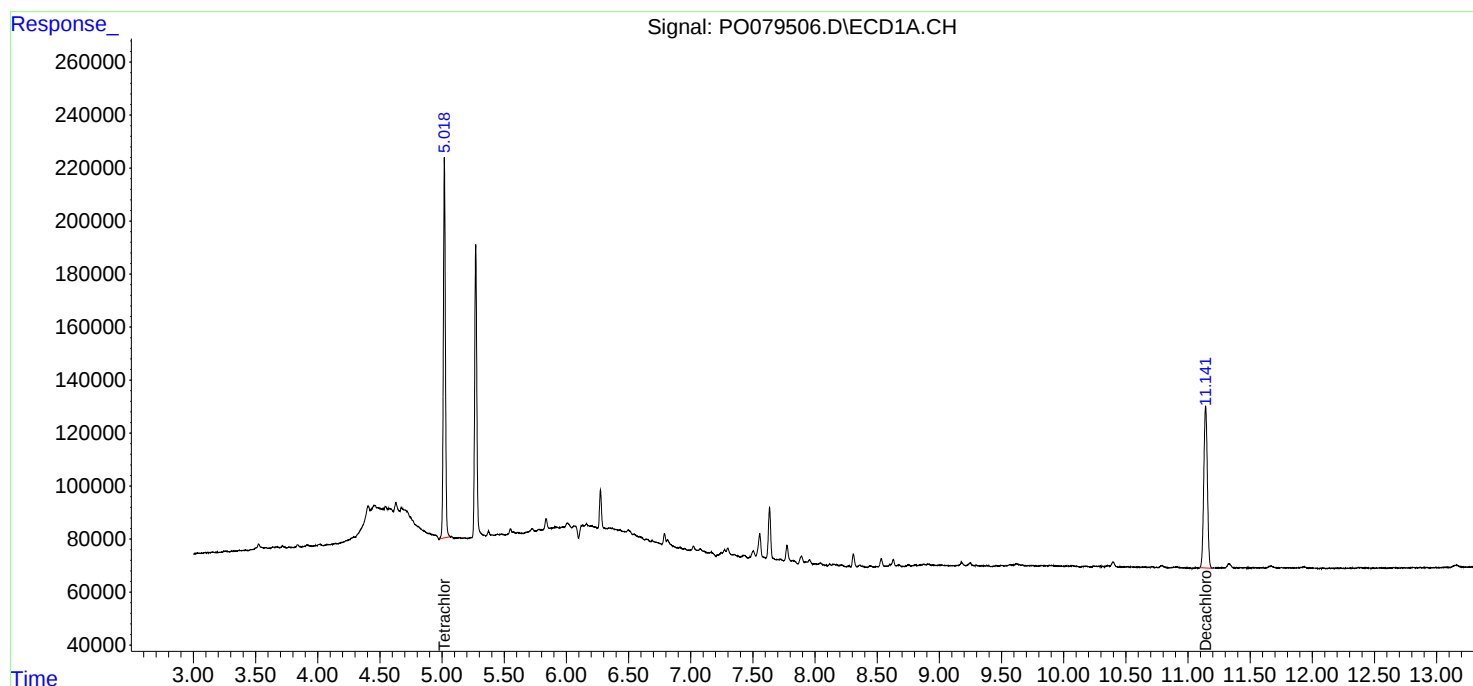


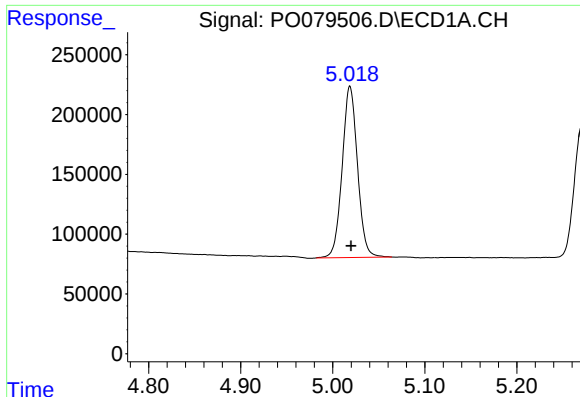

#1 Tetrachloro-m-xylene


R.T.: 5.019 min
Delta R.T.: -0.001 min
Response: 1656407
Conc: 24.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
CL-02-070921

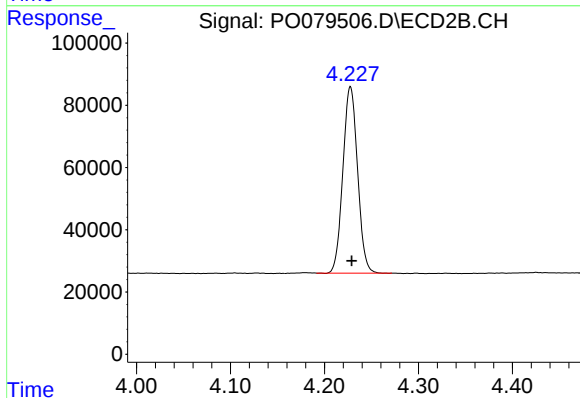


#1 Tetrachloro-m-xylene

R.T.: 4.228 min
Delta R.T.: -0.001 min
Response: 649852
Conc: 22.66 ng/ml

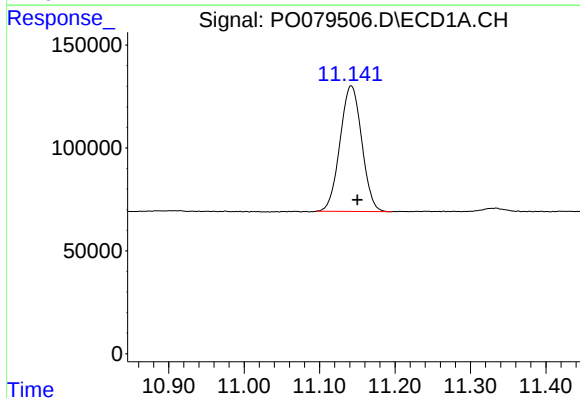

#2 Decachlorobiphenyl

R.T.: 11.142 min
Delta R.T.: -0.008 min
Response: 1222361
Conc: 24.03 ng/ml

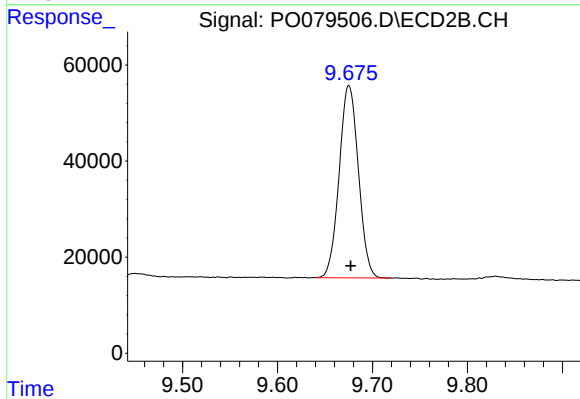

#2 Decachlorobiphenyl

R.T.: 9.675 min
Delta R.T.: -0.002 min
Response: 563373
Conc: 21.29 ng/ml