

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071222\
 Data File : P0087946.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2022 09:39
 Operator : YP/AJ
 Sample : N3650-13DL 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S5-05-SDL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/13/2022
 Supervised By :Ankita Jodhani 07/13/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 12 11:41:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 28 02:46:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.444	3.604	9472536	3163264	3.660	3.215
2) SA Decachlor...	10.297	8.610	7763057	3359023	3.800	4.144
Target Compounds						
26) L6 AR-1254-1	6.484	5.485	13894170	6559352	138.612	118.658
27) L6 AR-1254-2	6.701	5.633	31437125	8862800	206.006	181.164
28) L6 AR-1254-3	7.073	6.036	42066769	20341340	276.191	268.062
29) L6 AR-1254-4	7.358	6.265	24455810	9914622	222.174	218.387
30) L6 AR-1254-5	7.786	6.683	41525224	77710909	345.957m	1215.568 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO071222\
Data File : PO087946.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2022 09:39
Operator : YP/AJ
Sample : N3650-13DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S5-05-SDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/13/2022
Supervised By :Ankita Jodhani 07/13/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 11:41:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO062722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 28 02:46:21 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

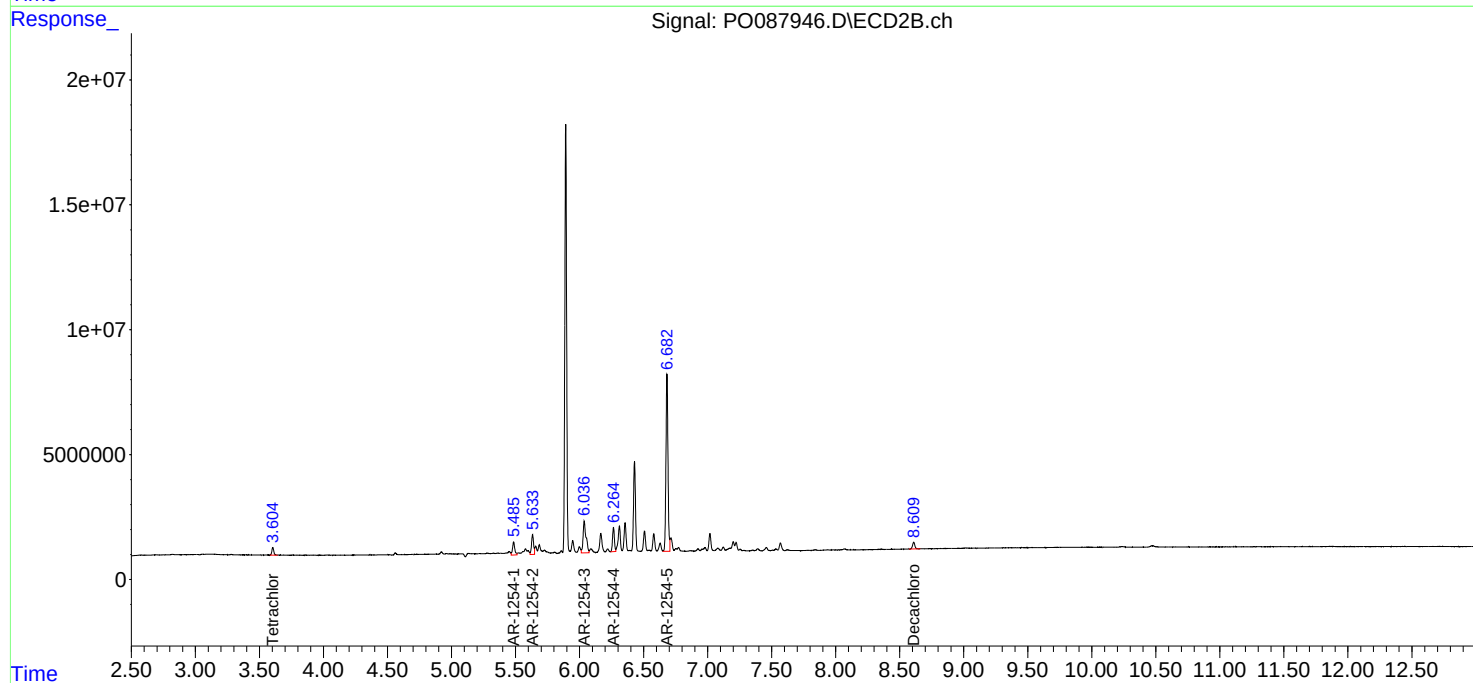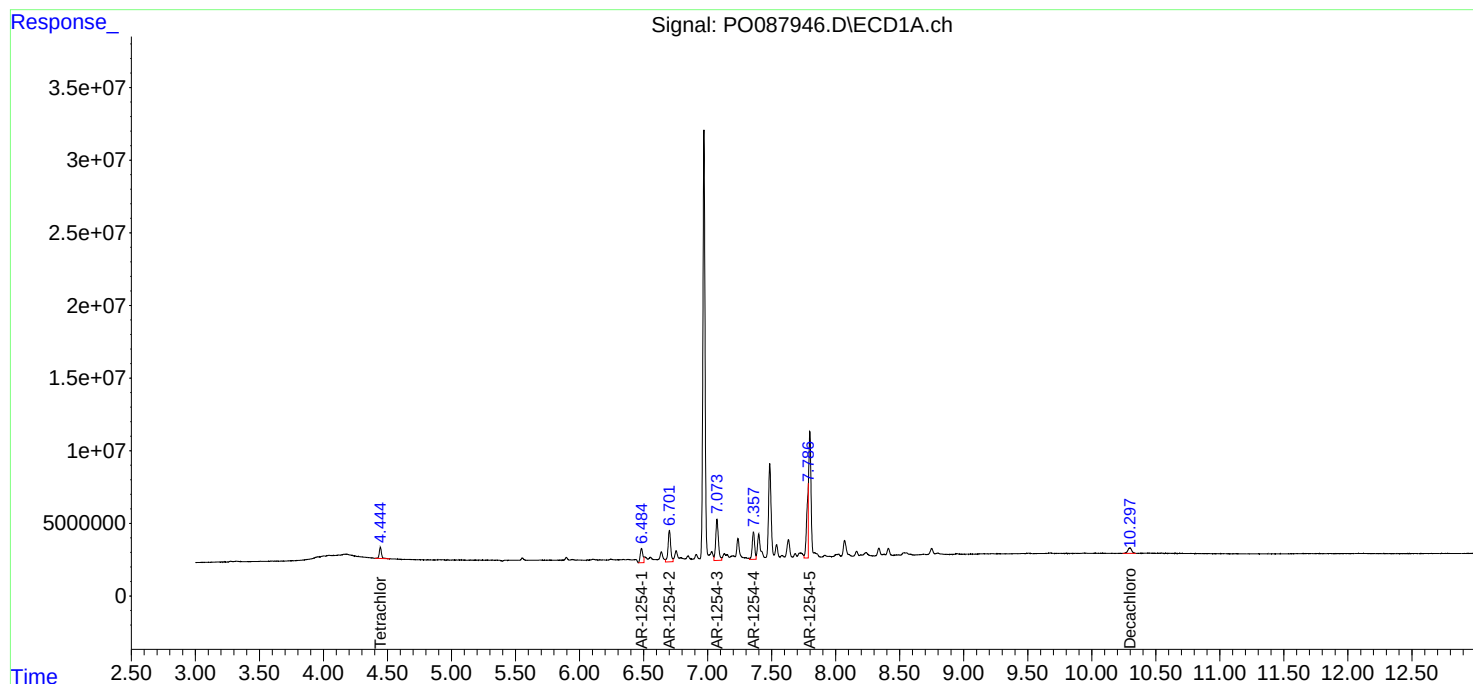

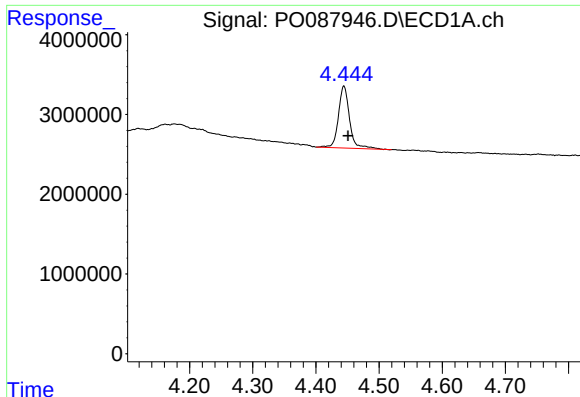


#1 Tetrachloro-m-xylene

R.T.: 4.444 min
Delta R.T.: -0.007 min
Response: 9472536
Conc: 3.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-05-SDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/13/2022
Supervised By :Ankita Jodhani 07/13/2022

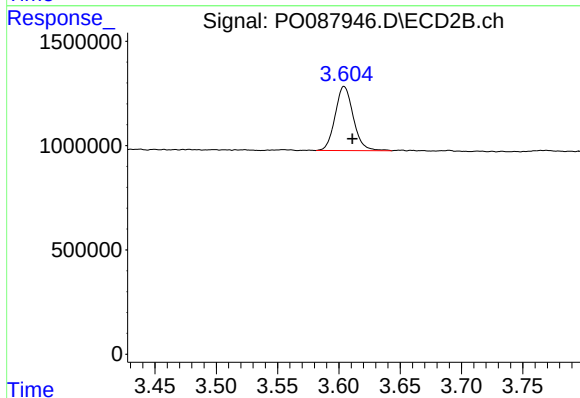


#1 Tetrachloro-m-xylene

R.T.: 3.604 min
Delta R.T.: -0.007 min
Response: 3163264
Conc: 3.21 ng/ml

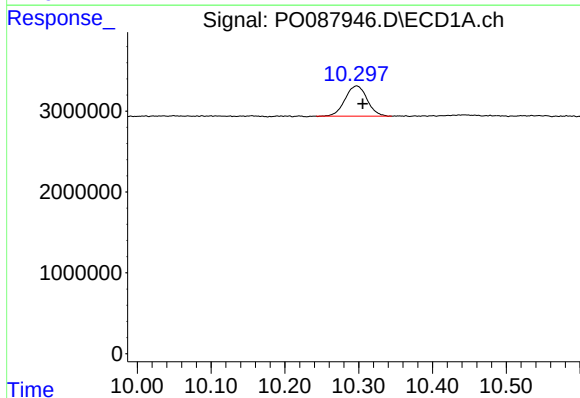


#2 Decachlorobiphenyl

R.T.: 10.297 min
Delta R.T.: -0.008 min
Response: 7763057
Conc: 3.80 ng/ml

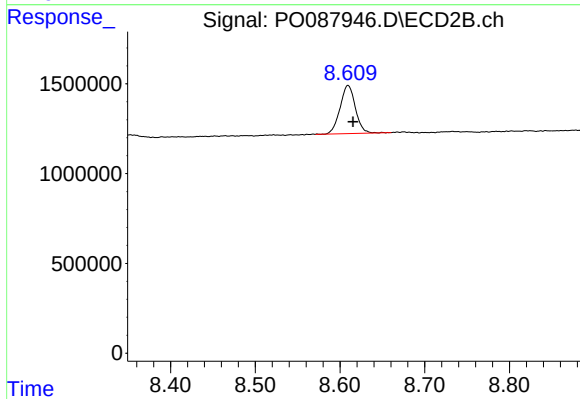

#2 Decachlorobiphenyl

R.T.: 8.610 min
Delta R.T.: -0.006 min
Response: 3359023
Conc: 4.14 ng/ml

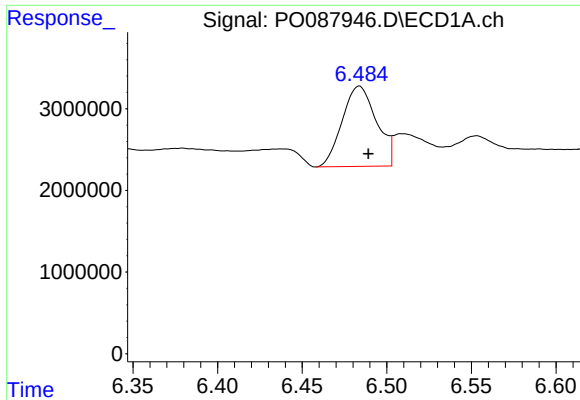


#26 AR-1254-1

R.T.: 6.484 min
Delta R.T.: -0.005 min
Response: 13894170
Conc: 138.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-05-SDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/13/2022
Supervised By :Ankita Jodhani 07/13/2022

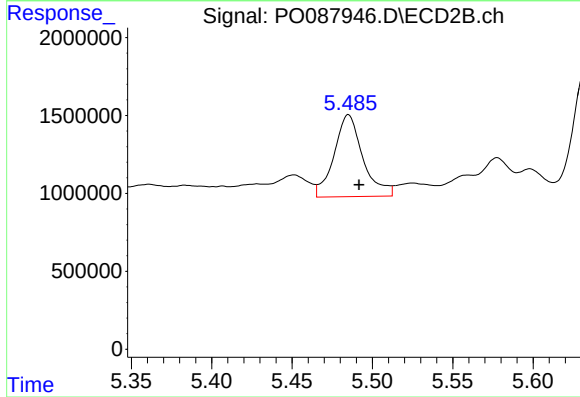


#26 AR-1254-1

R.T.: 5.485 min
Delta R.T.: -0.007 min
Response: 6559352
Conc: 118.66 ng/ml

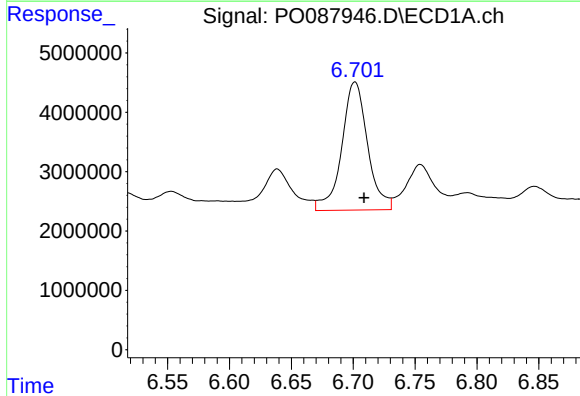


#27 AR-1254-2

R.T.: 6.701 min
Delta R.T.: -0.007 min
Response: 31437125
Conc: 206.01 ng/ml

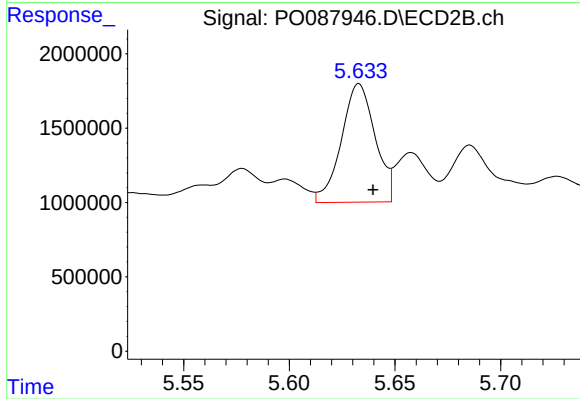

#27 AR-1254-2

R.T.: 5.633 min
Delta R.T.: -0.007 min
Response: 8862800
Conc: 181.16 ng/ml

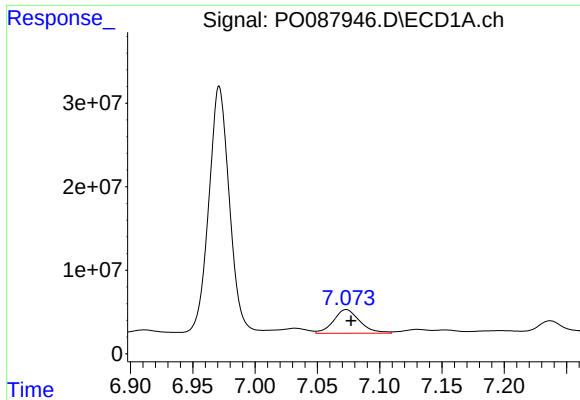


#28 AR-1254-3

R.T.: 7.073 min
Delta R.T.: -0.004 min
Response: 42066769
Conc: 276.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-05-SDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/13/2022
Supervised By :Ankita Jodhani 07/13/2022

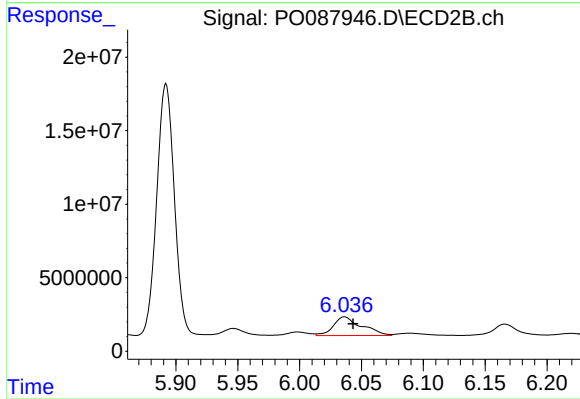


#28 AR-1254-3

R.T.: 6.036 min
Delta R.T.: -0.007 min
Response: 20341340
Conc: 268.06 ng/ml

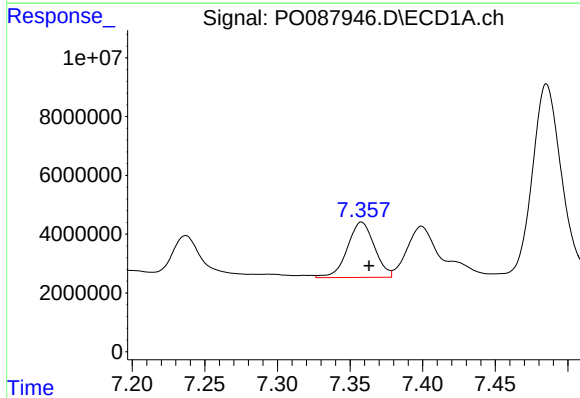


#29 AR-1254-4

R.T.: 7.358 min
Delta R.T.: -0.005 min
Response: 24455810
Conc: 222.17 ng/ml

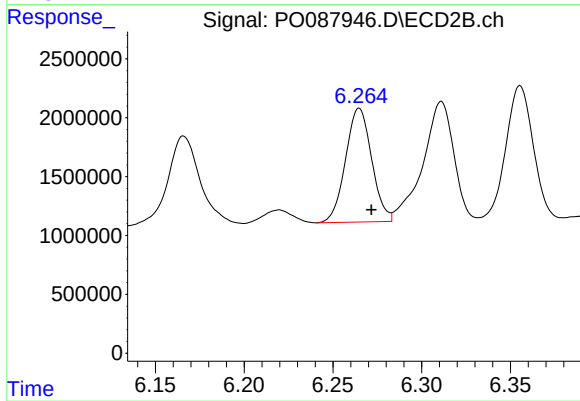

#29 AR-1254-4

R.T.: 6.265 min
Delta R.T.: -0.007 min
Response: 9914622
Conc: 218.39 ng/ml

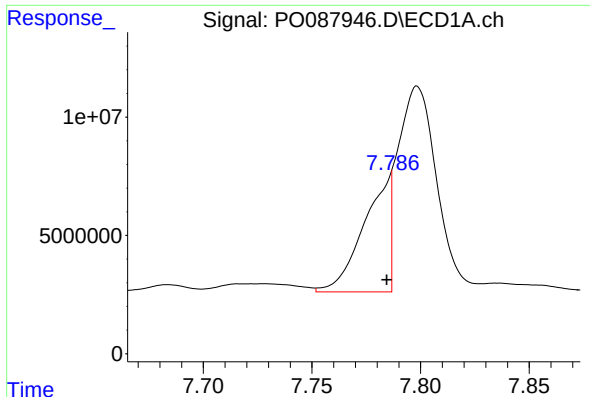


#30 AR-1254-5

R.T.: 7.786 min
Delta R.T.: 0.002 min
Response: 41525224
Conc: 345.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-05-SDL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/13/2022
Supervised By :Ankita Jodhani 07/13/2022

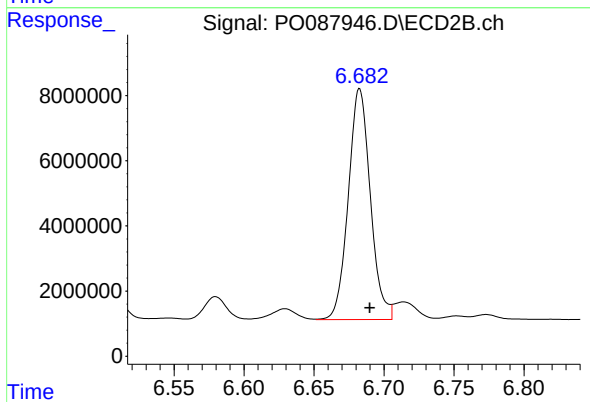

#30 AR-1254-5

R.T.: 6.683 min
Delta R.T.: -0.007 min
Response: 77710909
Conc: 1215.57 ng/ml