

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071224\
Data File : P0104768.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2024 17:29
Operator : YP/AJ
Sample : P3212-02 10x (Sig #1); P3212-02 (Sig #2)
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
407

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/15/2024
Supervised By :Ankita Jodhani 07/15/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 03:53:30 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070224.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 02 16:29:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.425	3.541	13856368	4819336	1.548	1.477
2) SA Decachlor...	10.206	8.438	5904639	3843288	0.963m	1.833m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071224\
Data File : PO104768.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2024 17:29
Operator : YP/AJ
Sample : P3212-02 10x (Sig #1); P3212-02 (Sig #2)
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
407


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/15/2024
Supervised By :Ankita Jodhani 07/15/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 03:53:30 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO070224.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 02 16:29:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

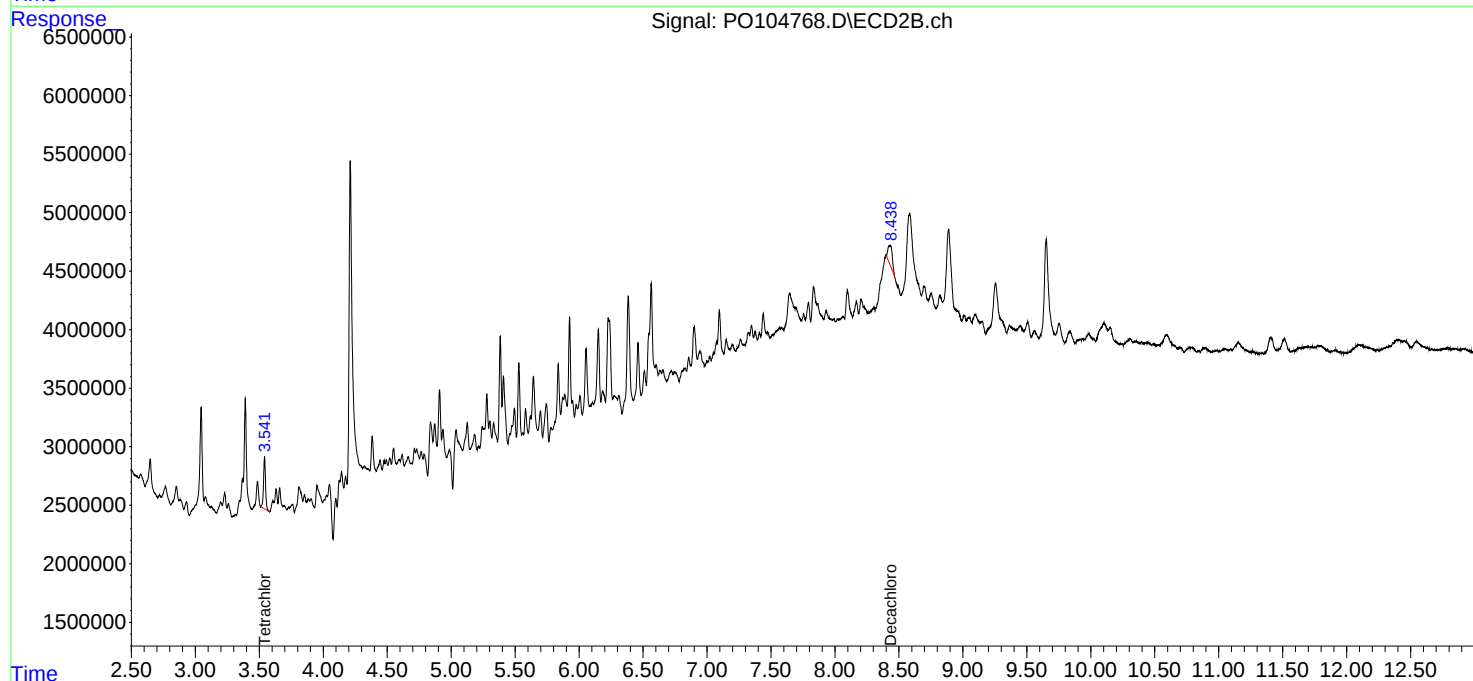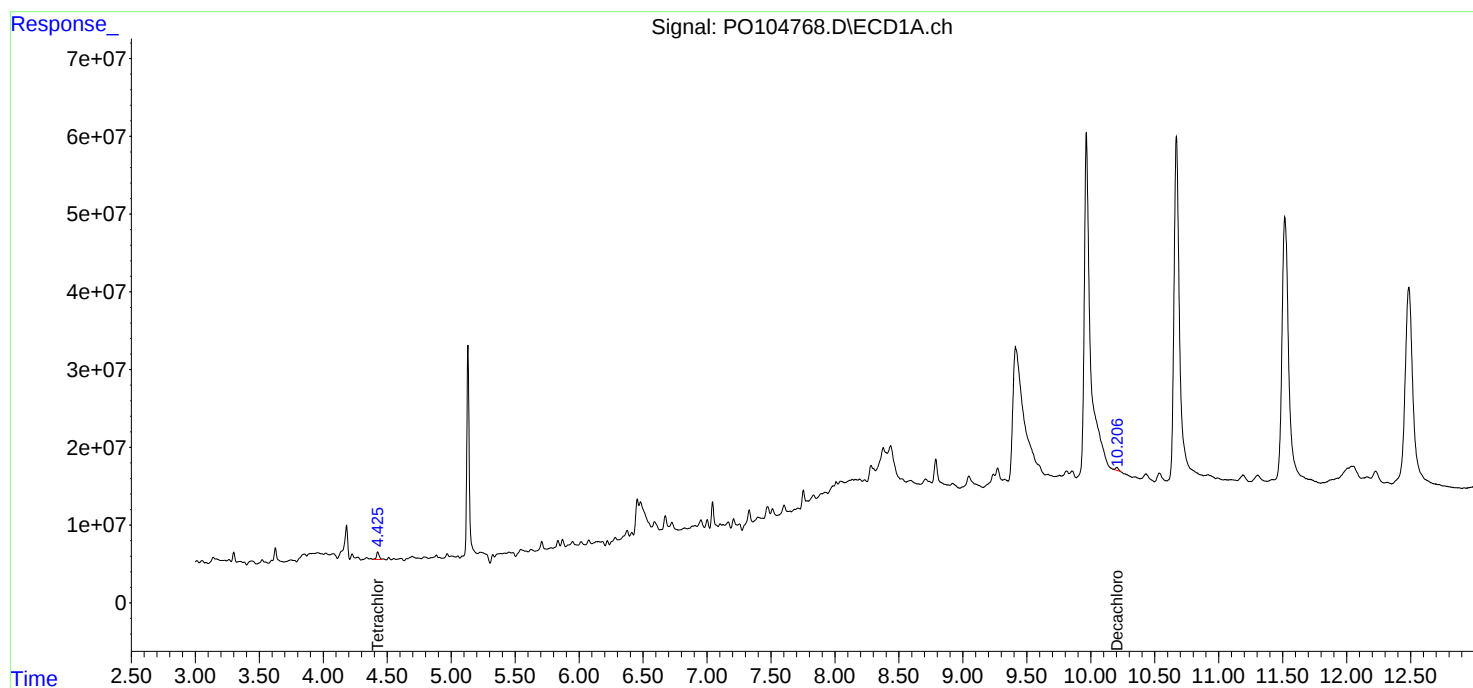

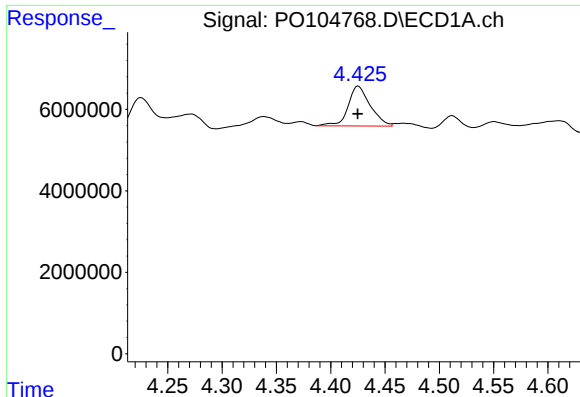


#1 Tetrachloro-m-xylene

R.T.: 4.425 min
Delta R.T.: 0.000 min
Response: 13856368
Conc: 1.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
407


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/15/2024
Supervised By :Ankita Jodhani 07/15/2024

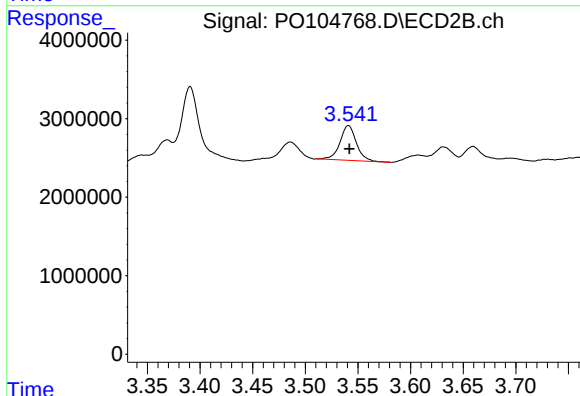


#1 Tetrachloro-m-xylene

R.T.: 3.541 min
Delta R.T.: 0.000 min
Response: 4819336
Conc: 1.48 ng/ml

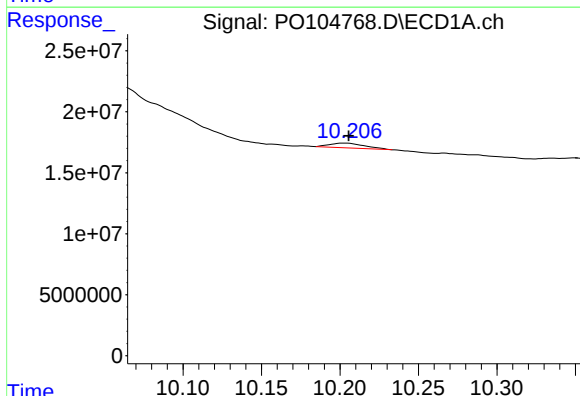

#2 Decachlorobiphenyl

R.T.: 10.206 min
Delta R.T.: 0.000 min
Response: 5904639
Conc: 0.96 ng/ml m

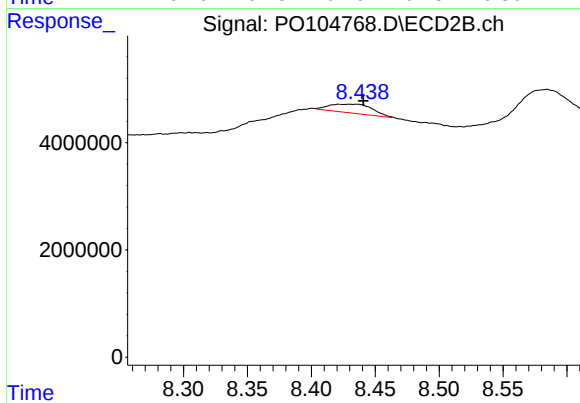

#2 Decachlorobiphenyl

R.T.: 8.438 min
Delta R.T.: -0.003 min
Response: 3843288
Conc: 1.83 ng/ml m