

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0071318\
Data File : P0046686.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jul 2018 14:42
Operator : SM/SJ
Sample : J3934-01RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TS-BASELINE-WATERRE

Manual Integrations
APPROVED

Sohil
7/16/2018 1:41:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 02:39:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.209	3.527	2475565	2904891	10.359m	13.676 #
2)	SA Decachlor...	9.735	8.459	1019796	1126722	5.350m	5.808

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0071318\
Data File : P0046686.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jul 2018 14:42
Operator : SM/SJ
Sample : J3934-01RE
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TS-BASELINE-WATERRE


Manual Integrations
APPROVED

Sohil
7/16/2018 1:41:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 02:39:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

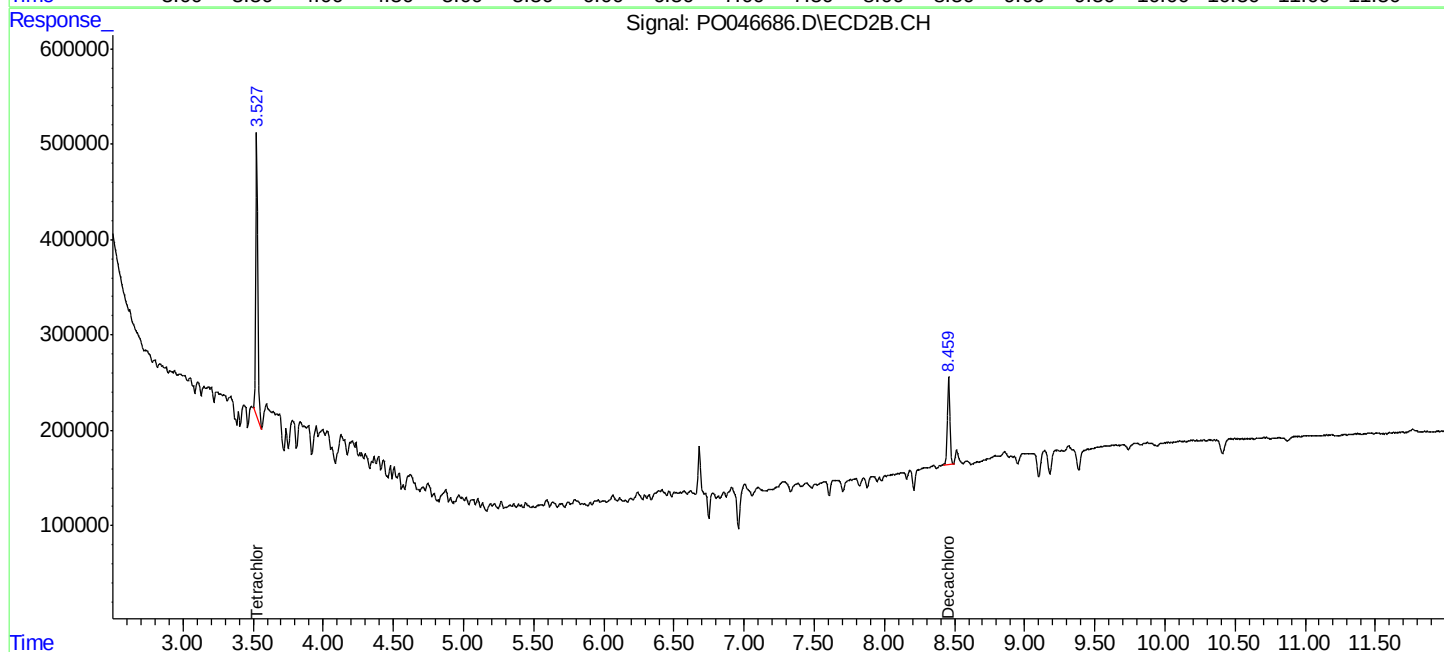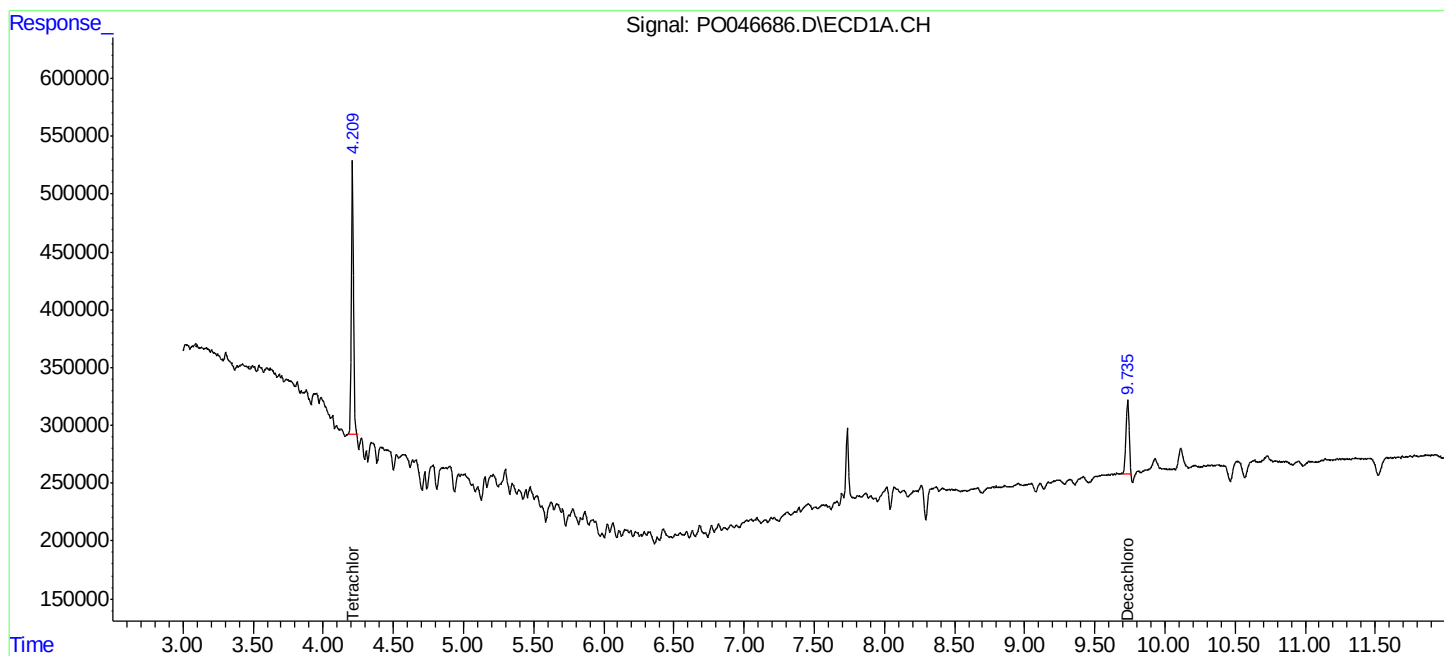

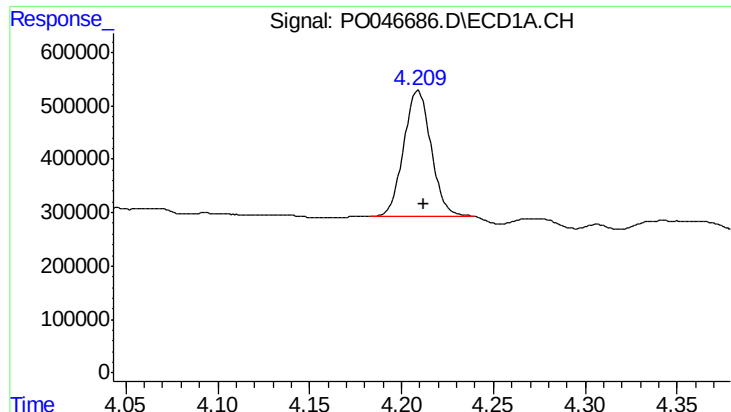


#1 Tetrachloro-m-xylene

R.T.: 4.209 min
Delta R.T.: -0.004 min
Response: 2475565
Conc: 10.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
TS-BASELINE-WATERRE


Manual Integrations
APPROVED

Sohil
7/16/2018 1:41:52 PM

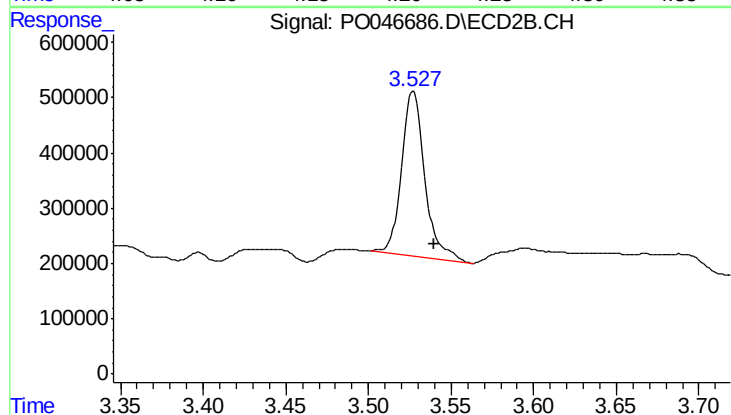


#1 Tetrachloro-m-xylene

R.T.: 3.527 min
Delta R.T.: -0.013 min
Response: 2904891
Conc: 13.68 ng/ml

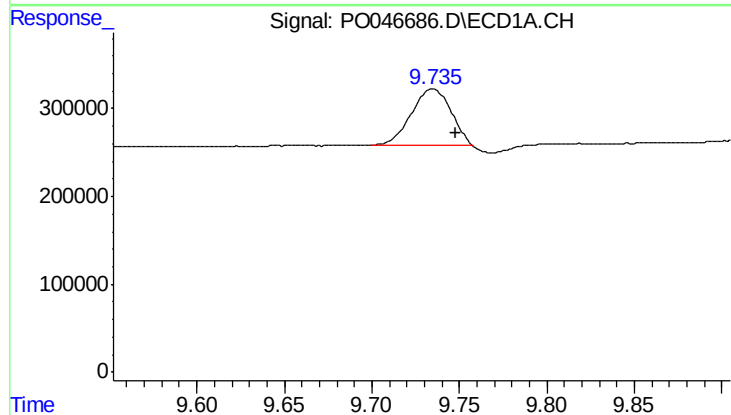

#2 Decachlorobiphenyl

R.T.: 9.735 min
Delta R.T.: -0.013 min
Response: 1019796
Conc: 5.35 ng/ml m

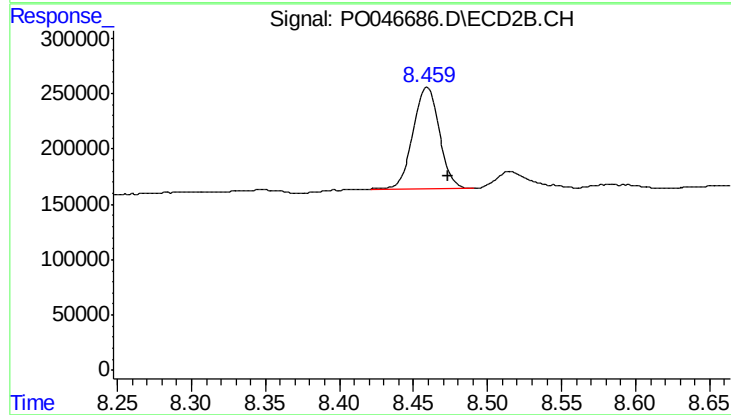

#2 Decachlorobiphenyl

R.T.: 8.459 min
Delta R.T.: -0.014 min
Response: 1126722
Conc: 5.81 ng/ml