

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071322\
 Data File : P0088000.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jul 2022 17:00
 Operator : YP/AJ
 Sample : N3687-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ETGI-346

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/14/2022
 Supervised By :Ankita Jodhani 07/14/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 11:59:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 28 02:46:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.448	3.607	60501143	22564656	23.375	22.932
2) SA Decachlor...	10.294	8.608	39854457	20034264	19.511	24.713 #
Target Compounds						
31) L7 AR-1260-1	7.237	6.169	6171877	3231998	55.055	57.249
32) L7 AR-1260-2	7.489	6.359	28322500	6998549	207.832	103.443m#
33) L7 AR-1260-3	7.856	6.509	4891833	2900534	52.225	45.917
34) L7 AR-1260-4	8.078	6.983	9872007	2838110	94.371	61.029 #
35) L7 AR-1260-5	8.412	7.223	7018349	3937756	35.578	36.530

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071322\
Data File : P0088000.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jul 2022 17:00
Operator : YP/AJ
Sample : N3687-03
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ETGI-346


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/14/2022
Supervised By :Ankita Jodhani 07/14/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 11:59:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 28 02:46:21 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

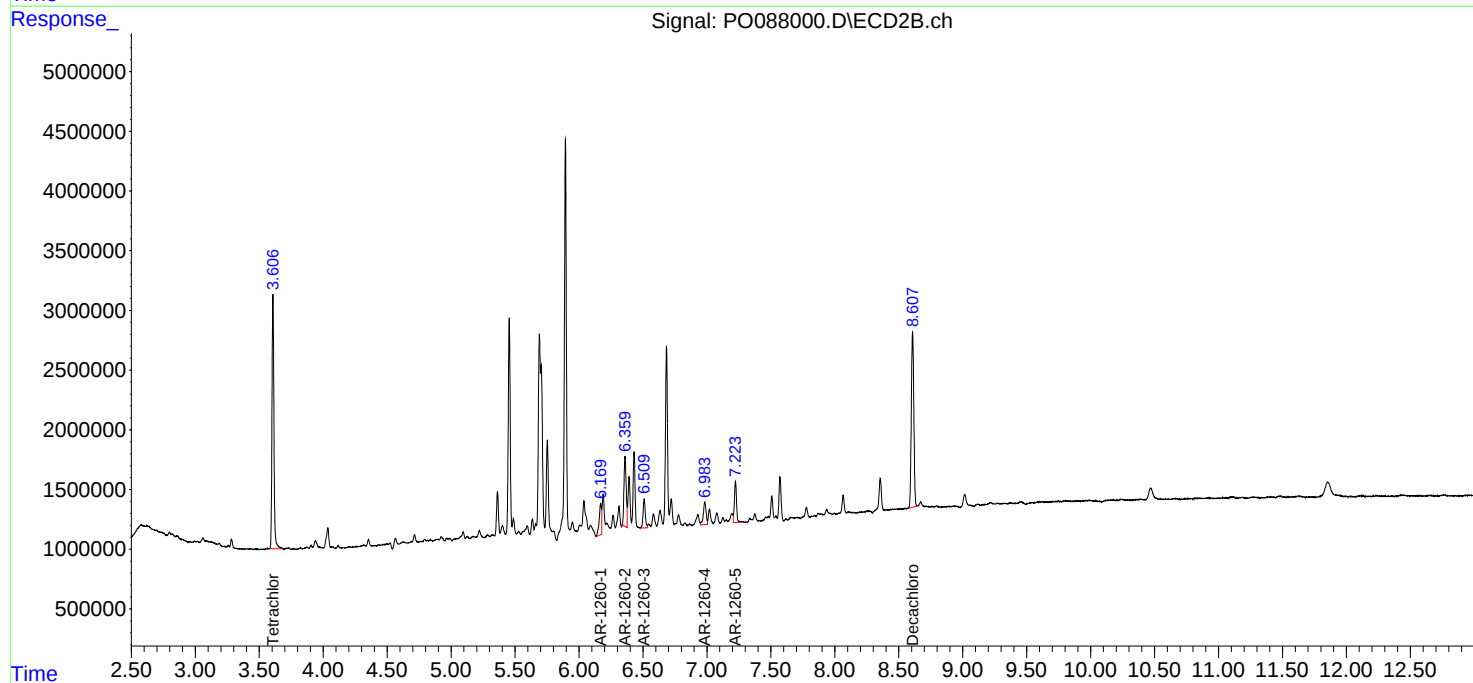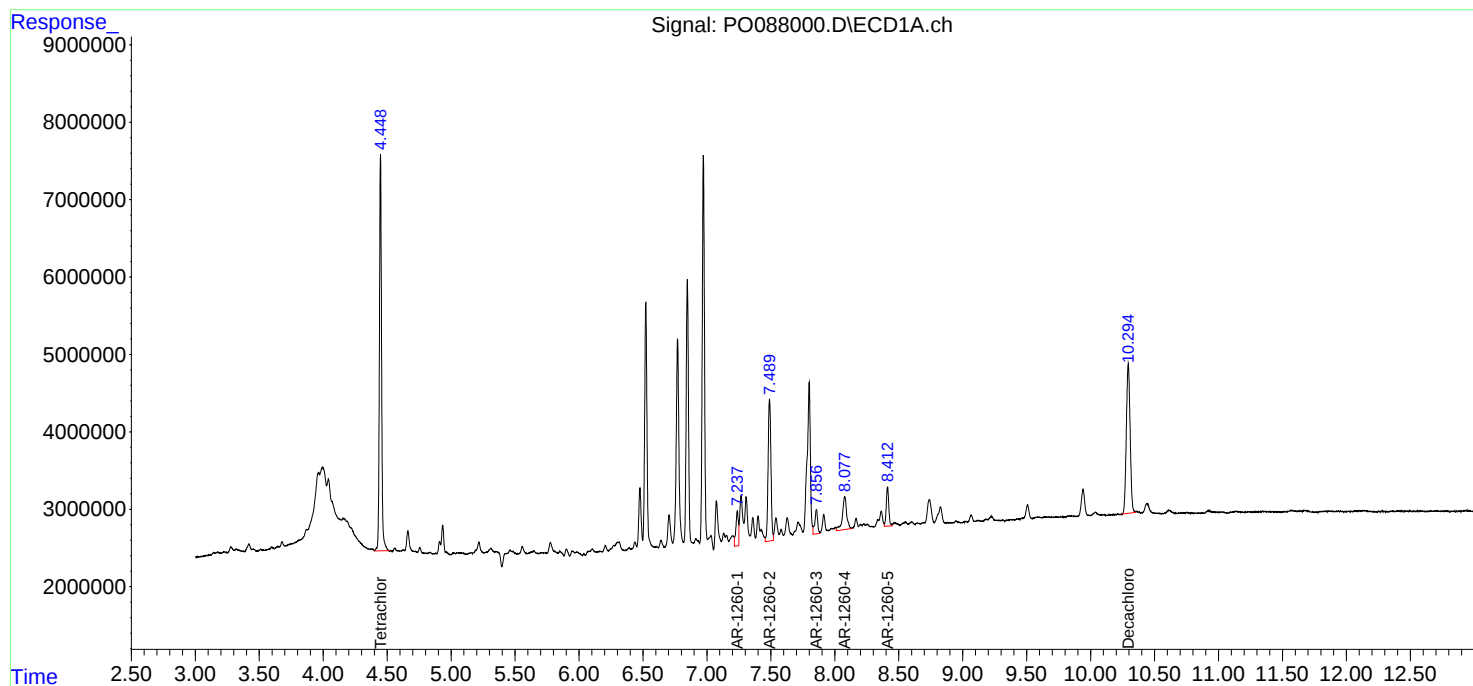

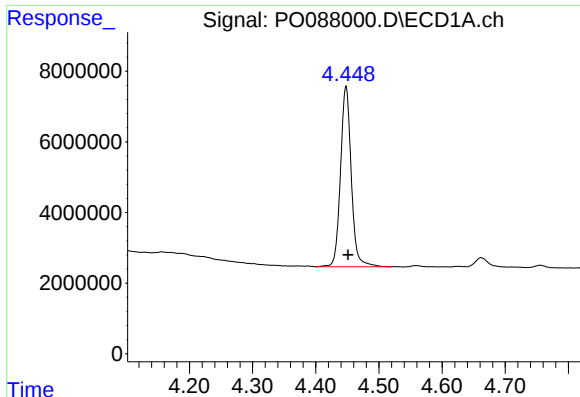


#1 Tetrachloro-m-xylene

R.T.: 4.448 min
Delta R.T.: -0.003 min
Response: 60501143
Conc: 23.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
ETGI-346


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/14/2022
Supervised By :Ankita Jodhani 07/14/2022

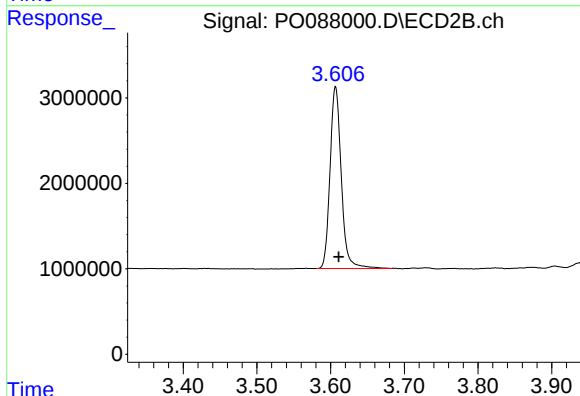


#1 Tetrachloro-m-xylene

R.T.: 3.607 min
Delta R.T.: -0.004 min
Response: 22564656
Conc: 22.93 ng/ml

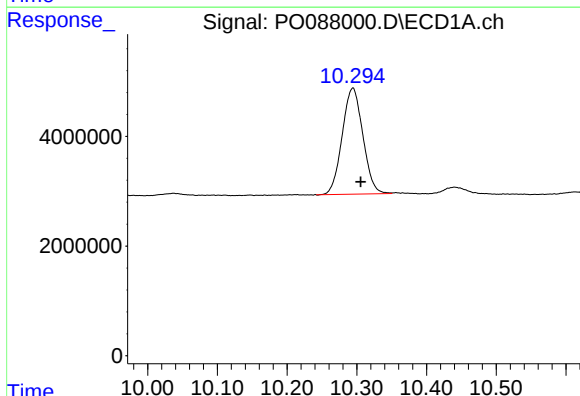


#2 Decachlorobiphenyl

R.T.: 10.294 min
Delta R.T.: -0.011 min
Response: 39854457
Conc: 19.51 ng/ml

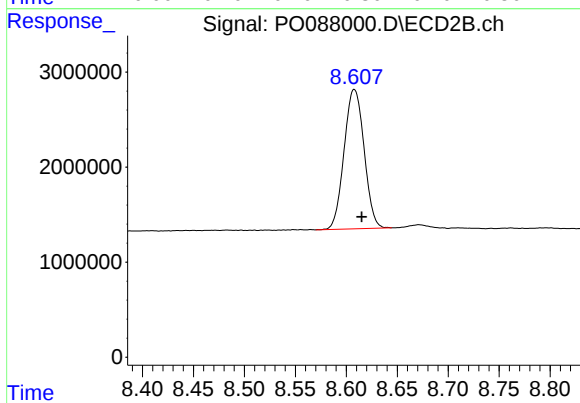

#2 Decachlorobiphenyl

R.T.: 8.608 min
Delta R.T.: -0.007 min
Response: 20034264
Conc: 24.71 ng/ml

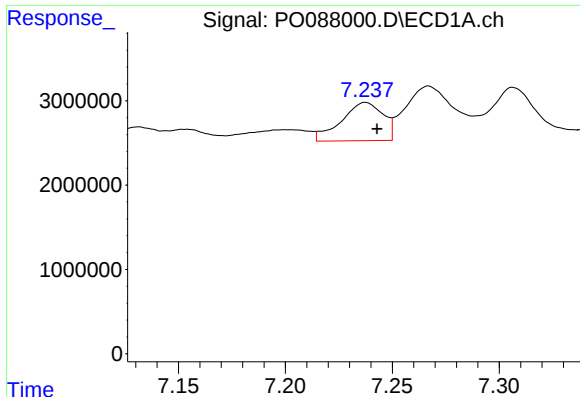


#31 AR-1260-1

R.T.: 7.237 min
Delta R.T.: -0.005 min
Response: 6171877
Conc: 55.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
ETGI-346


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/14/2022
Supervised By :Ankita Jodhani 07/14/2022

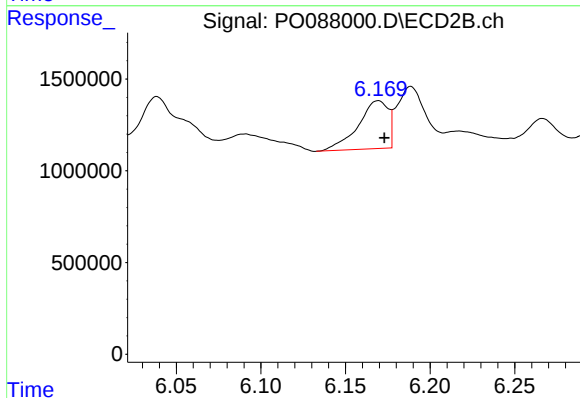


#31 AR-1260-1

R.T.: 6.169 min
Delta R.T.: -0.004 min
Response: 3231998
Conc: 57.25 ng/ml

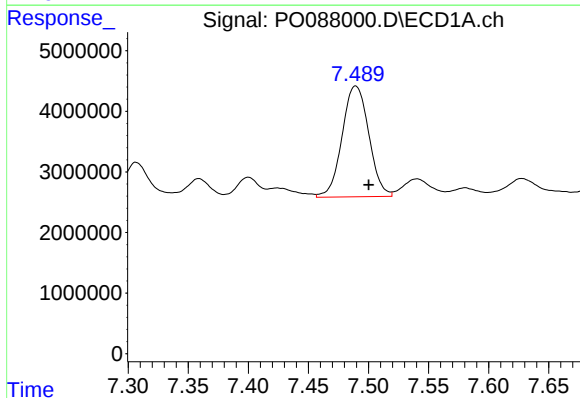


#32 AR-1260-2

R.T.: 7.489 min
Delta R.T.: -0.011 min
Response: 28322500
Conc: 207.83 ng/ml

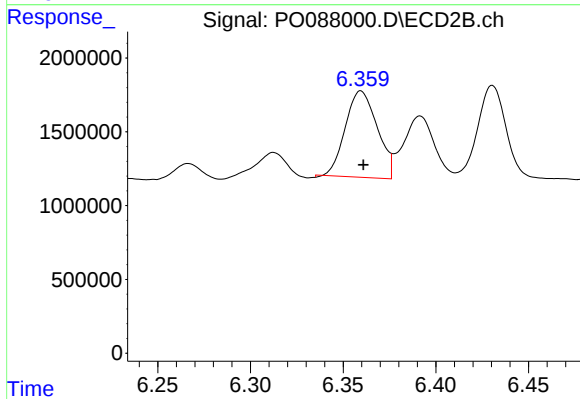

#32 AR-1260-2

R.T.: 6.359 min
Delta R.T.: -0.002 min
Response: 6998549
Conc: 103.44 ng/ml m

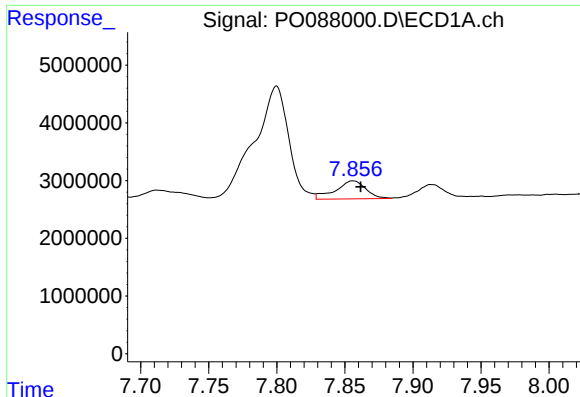


#33 AR-1260-3

R.T.: 7.856 min
Delta R.T.: -0.006 min
Response: 4891833
Conc: 52.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
ETGI-346


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/14/2022
Supervised By :Ankita Jodhani 07/14/2022

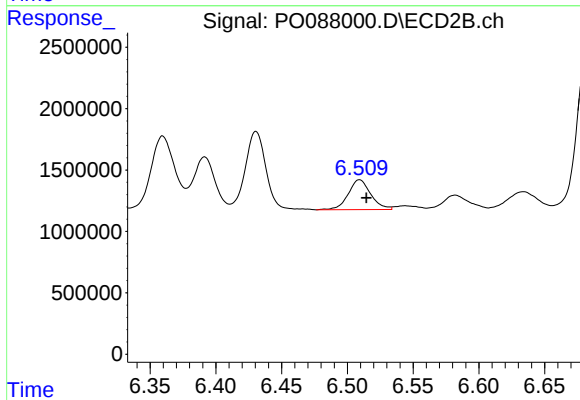


#33 AR-1260-3

R.T.: 6.509 min
Delta R.T.: -0.005 min
Response: 2900534
Conc: 45.92 ng/ml

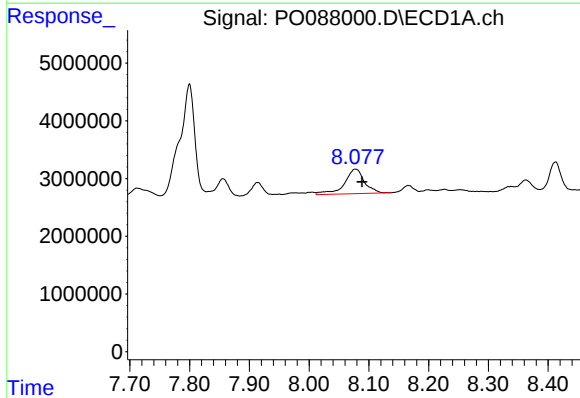


#34 AR-1260-4

R.T.: 8.078 min
Delta R.T.: -0.011 min
Response: 9872007
Conc: 94.37 ng/ml

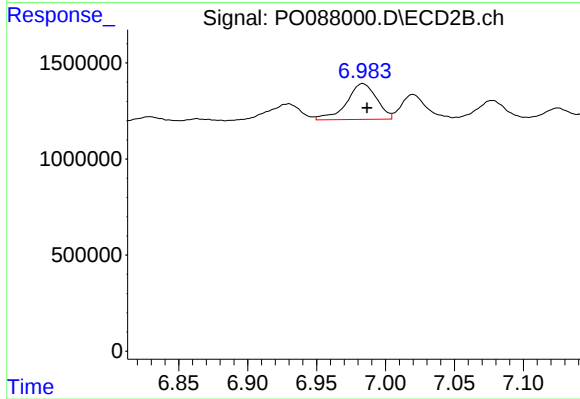

#34 AR-1260-4

R.T.: 6.983 min
Delta R.T.: -0.003 min
Response: 2838110
Conc: 61.03 ng/ml

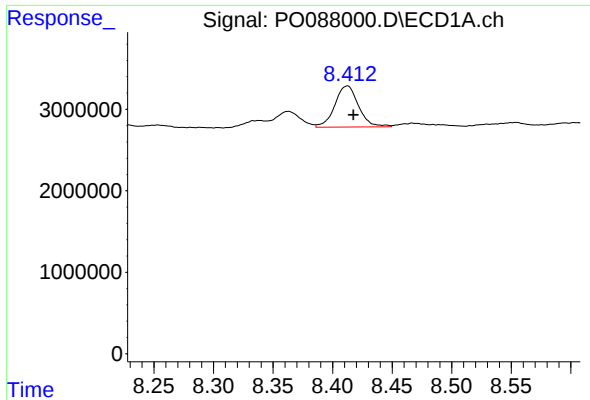


#35 AR-1260-5

R.T.: 8.412 min
Delta R.T.: -0.005 min
Response: 7018349
Conc: 35.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
ETGI-346

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/14/2022
Supervised By :Ankita Jodhani 07/14/2022

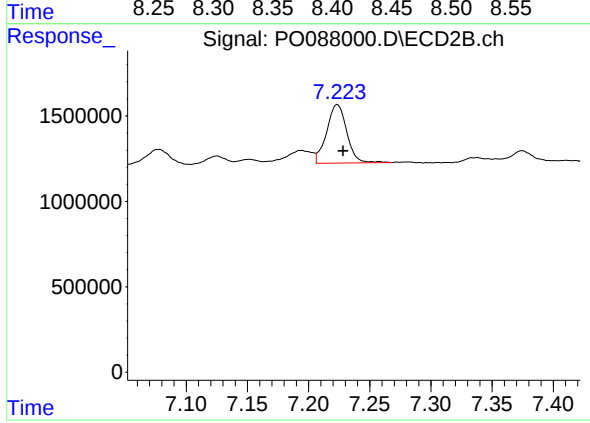

#35 AR-1260-5

R.T.: 7.223 min
Delta R.T.: -0.005 min
Response: 3937756
Conc: 36.53 ng/ml