

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071322\
 Data File : P0088036.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jul 2022 05:23
 Operator : YP/AJ
 Sample : N3684-01 10X
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 JEC5015-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/14/2022
 Supervised By :Ankita Jodhani 07/14/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 07:38:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 28 02:46:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.446	3.606	4283630	1730532	1.655	1.759
2) SA Decachlor...	10.290	8.605	3986557	1990101	1.952m	2.455 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071322\
Data File : PO088036.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jul 2022 05:23
Operator : YP/AJ
Sample : N3684-01 10X
Misc :
ALS Vial : 43 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
JEC5015-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/14/2022
Supervised By :Ankita Jodhani 07/14/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 07:38:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 28 02:46:21 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

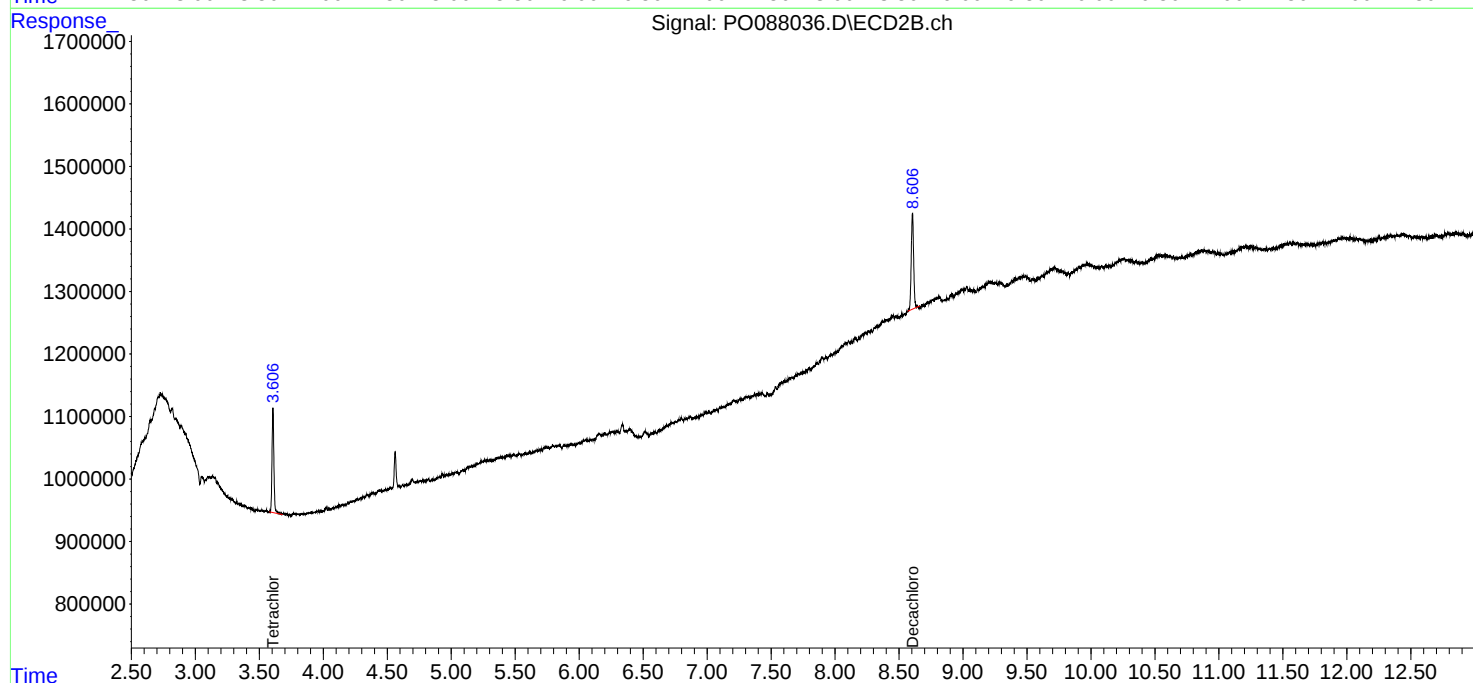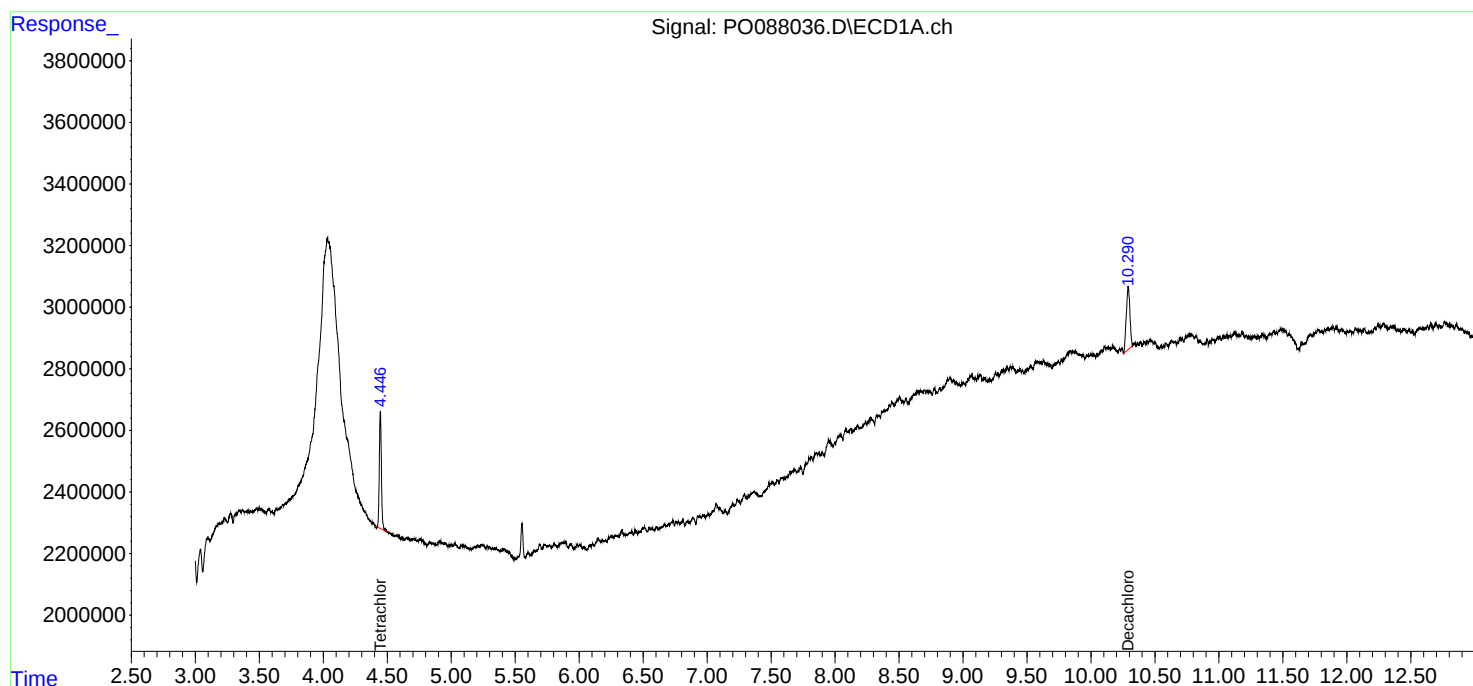

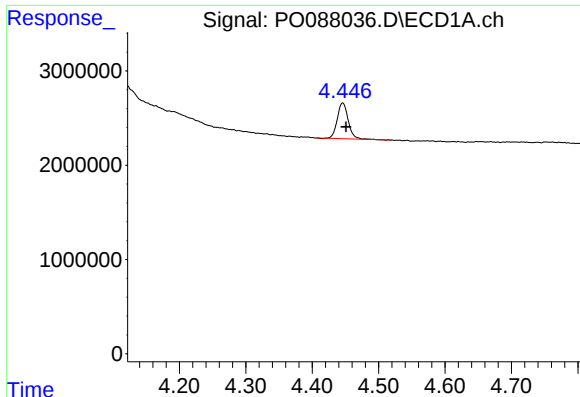

#1 Tetrachloro-m-xylene

R.T.: 4.446 min
Delta R.T.: -0.005 min
Response: 4283630
Conc: 1.65 ng/ml


Instrument :
ECD_O
ClientSampleId :
JEC5015-1-1

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/14/2022
Supervised By :Ankita Jodhani 07/14/2022

#1 Tetrachloro-m-xylene

R.T.: 3.606 min
Delta R.T.: -0.005 min
Response: 1730532
Conc: 1.76 ng/ml

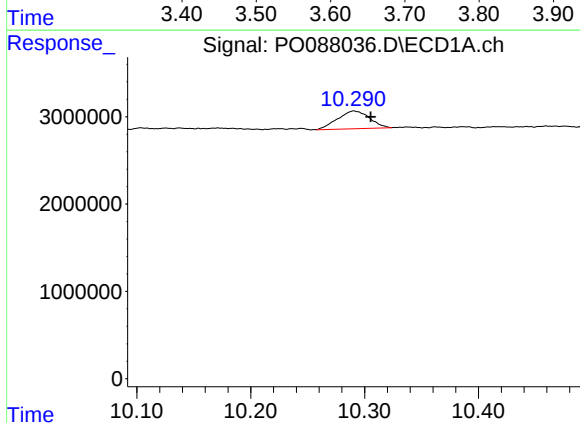

#2 Decachlorobiphenyl

R.T.: 10.290 min
Delta R.T.: -0.015 min
Response: 3986557
Conc: 1.95 ng/ml m

#2 Decachlorobiphenyl

R.T.: 8.605 min
Delta R.T.: -0.010 min
Response: 1990101
Conc: 2.45 ng/ml