

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0071418\
 Data File : P0046726.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Jul 2018 7:50
 Operator : SM/SJ
 Sample : J3948-05
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 2018-NYSEG-CLARK-ST-PH4-AREA

Manual Integrations
 APPROVED

Sohil
 7/17/2018 3:36:01 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 10:05:06 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 09 15:27:34 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.196	3.523	2464648	3067993	10.313m	14.444 #
2) SA Decachlor...	9.719	8.450	2202070	1961277	11.553m	10.111

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0071418\
Data File : P0046726.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Jul 2018 7:50
Operator : SM/SJ
Sample : J3948-05
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-ST-PH4-AREA


Manual Integrations
APPROVED

Sohil
7/17/2018 3:36:01 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 10:05:06 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

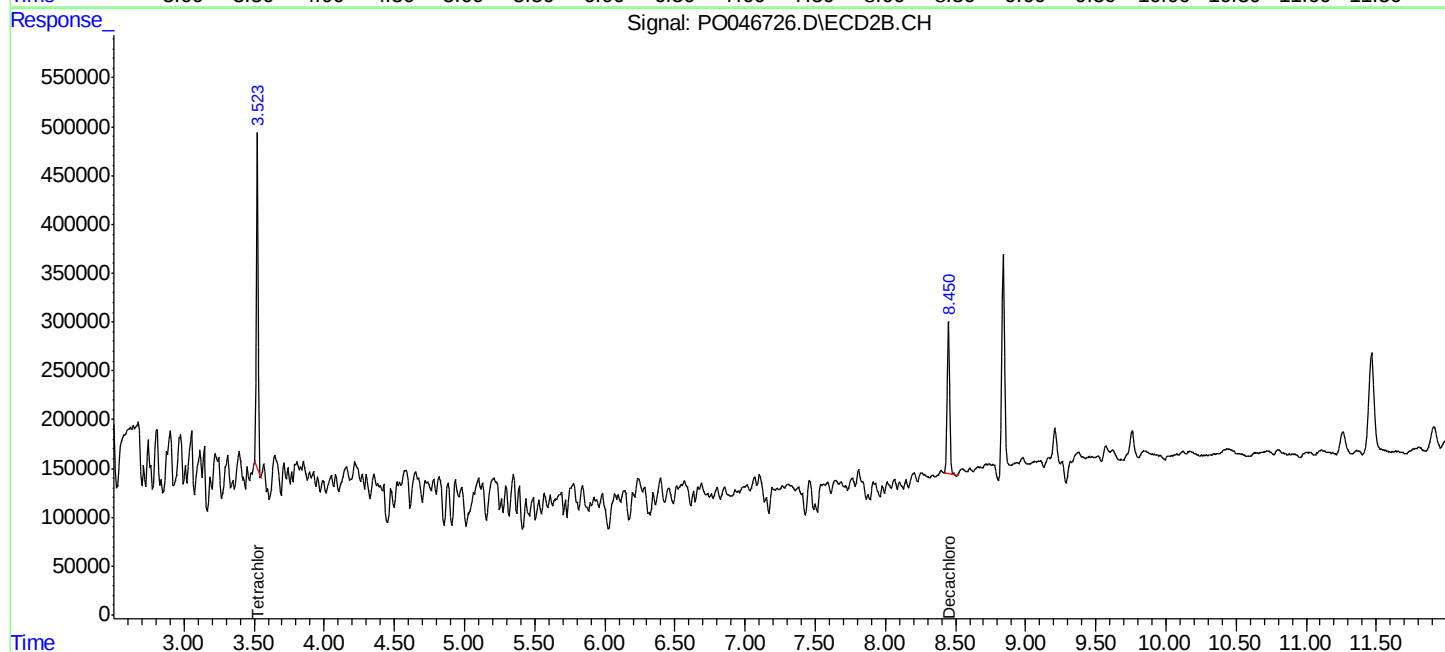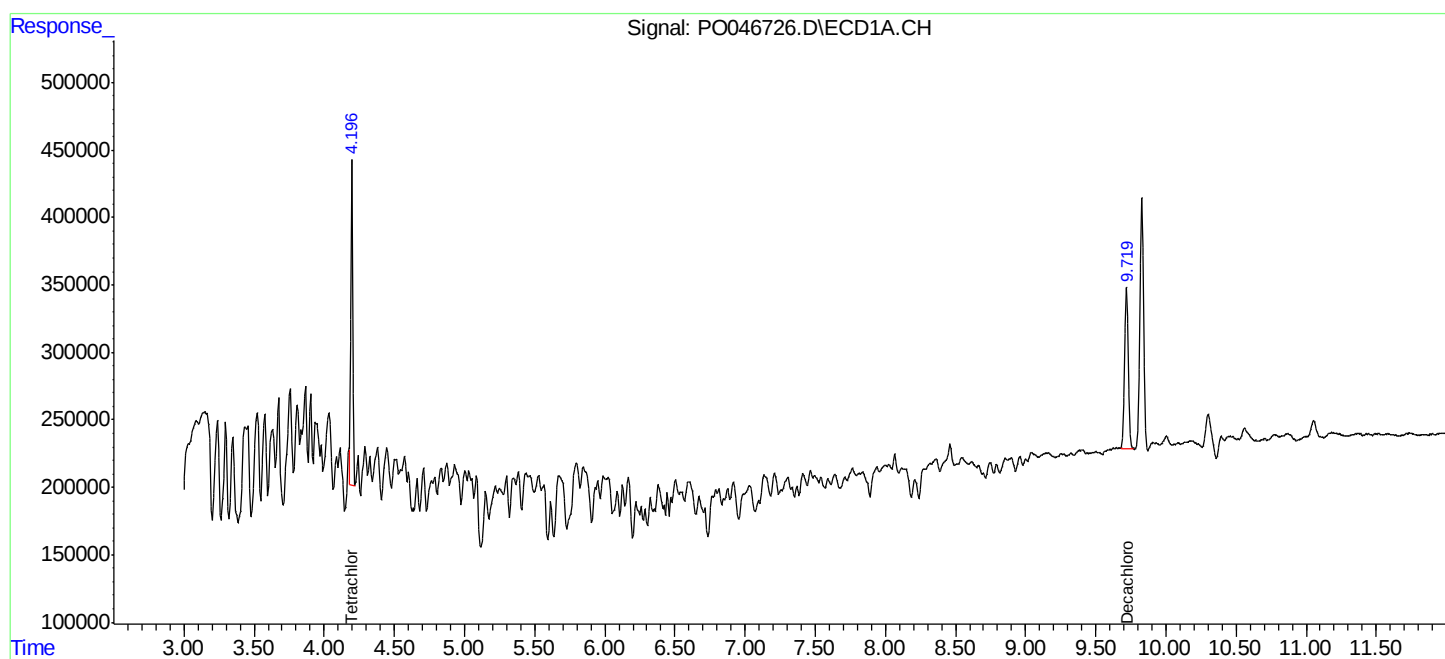

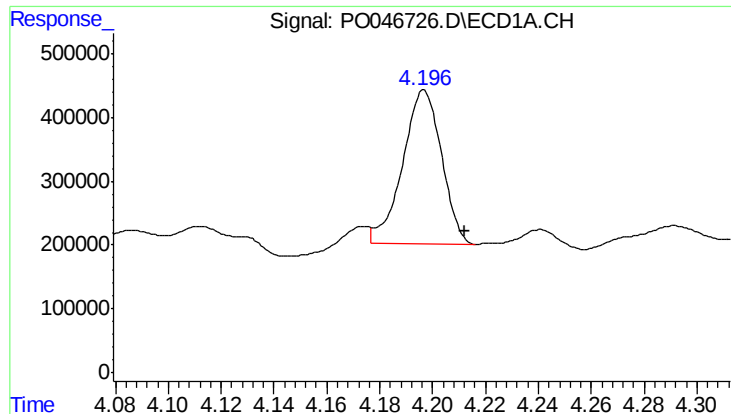


#1 Tetrachloro-m-xylene

R.T.: 4.196 min
Delta R.T.: -0.016 min
Response: 2464648
Conc: 10.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-ST-PH4-AREA


Manual Integrations
APPROVED

Sohil
7/17/2018 3:36:01 PM

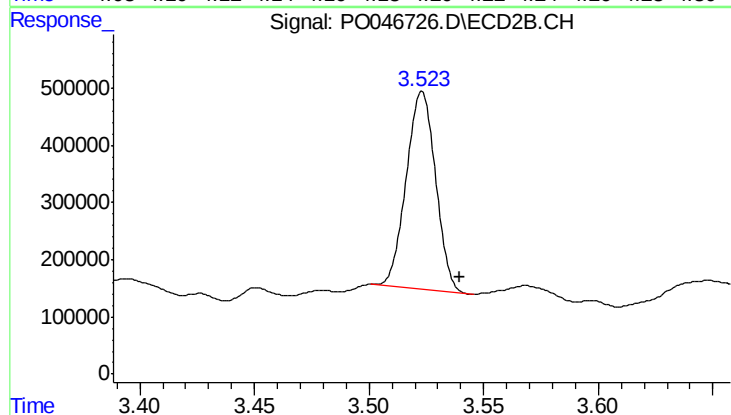


#1 Tetrachloro-m-xylene

R.T.: 3.523 min
Delta R.T.: -0.016 min
Response: 3067993
Conc: 14.44 ng/ml

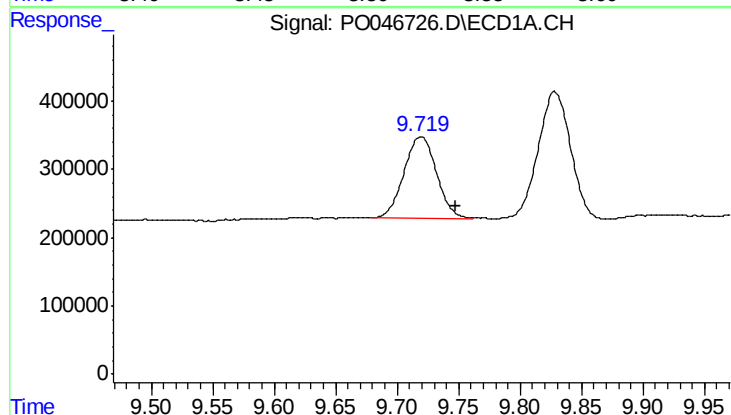

#2 Decachlorobiphenyl

R.T.: 9.719 min
Delta R.T.: -0.029 min
Response: 2202070
Conc: 11.55 ng/ml m

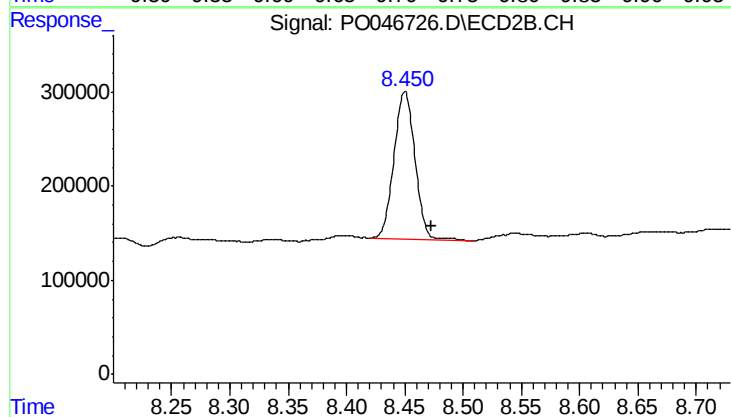

#2 Decachlorobiphenyl

R.T.: 8.450 min
Delta R.T.: -0.023 min
Response: 1961277
Conc: 10.11 ng/ml