

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0071418\
Data File : P0046727.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Jul 2018 8:06
Operator : SM/SJ
Sample : J3956-01
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CONTINGENCY-DUCK-BANK-CON

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 10:05:47 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.198	3.522	5404794	5758385	22.616	27.110
2) SA Decachlor...	9.720	8.449	3869061	3657132	20.299	18.853

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0071418\
Data File : P0046727.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Jul 2018 8:06
Operator : SM/SJ
Sample : J3956-01
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CONTINGENCY-DUCK-BANK-CON

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 10:05:47 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

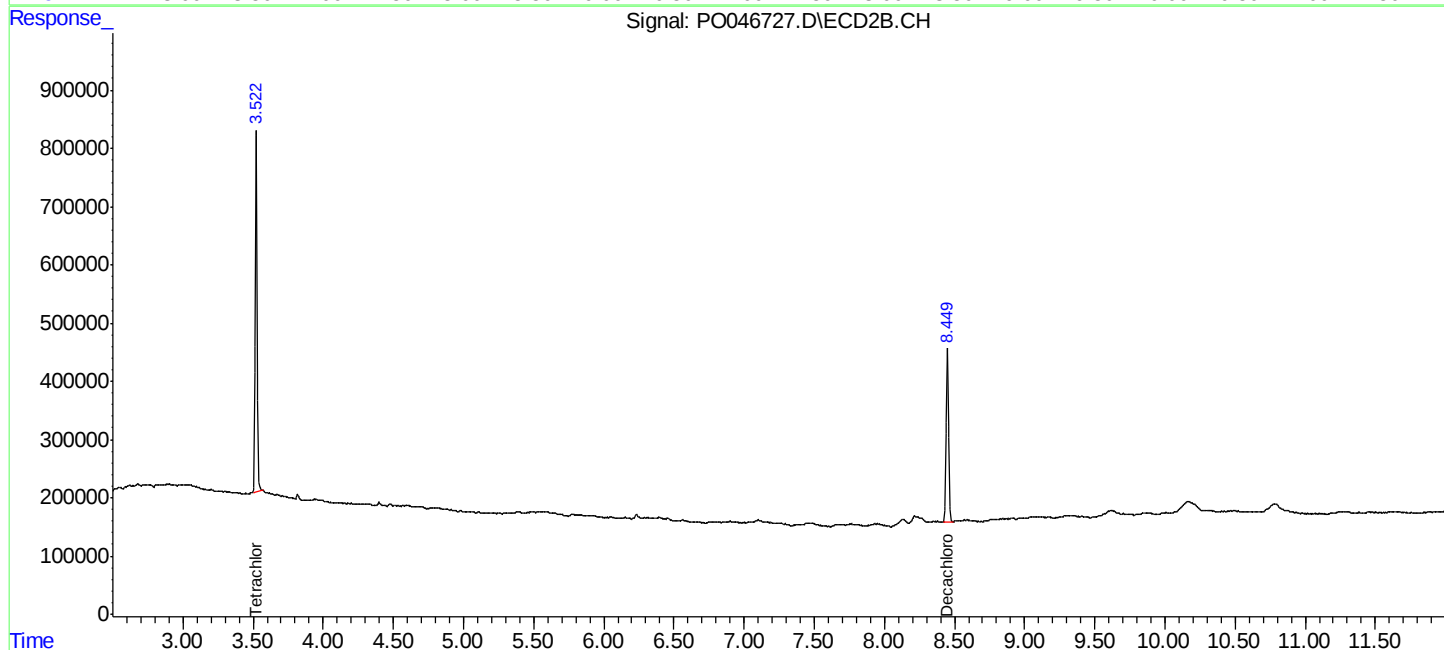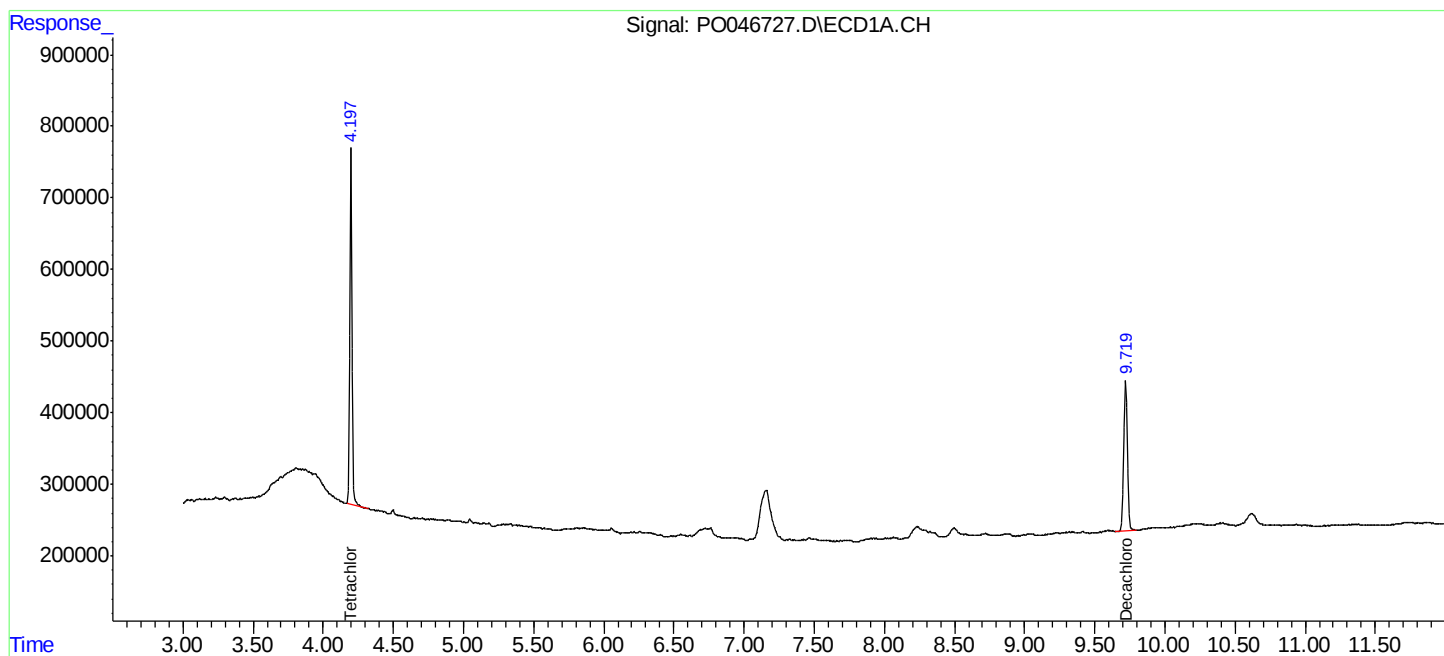


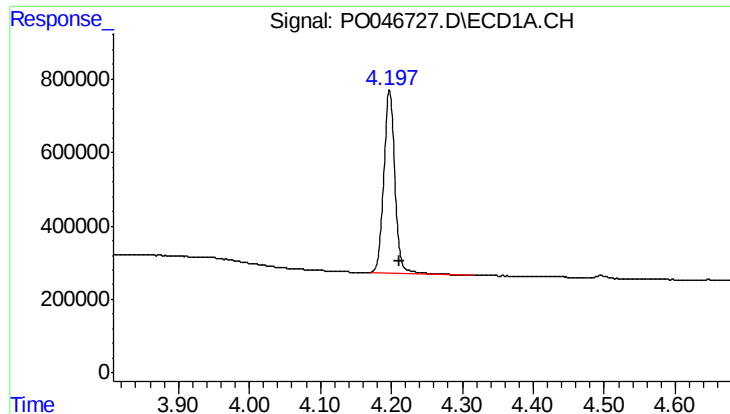

#1 Tetrachloro-m-xylene


R.T.: 4.198 min
Delta R.T.: -0.015 min
Response: 5404794
Conc: 22.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTINGENCY-DUCK-BANK-CON

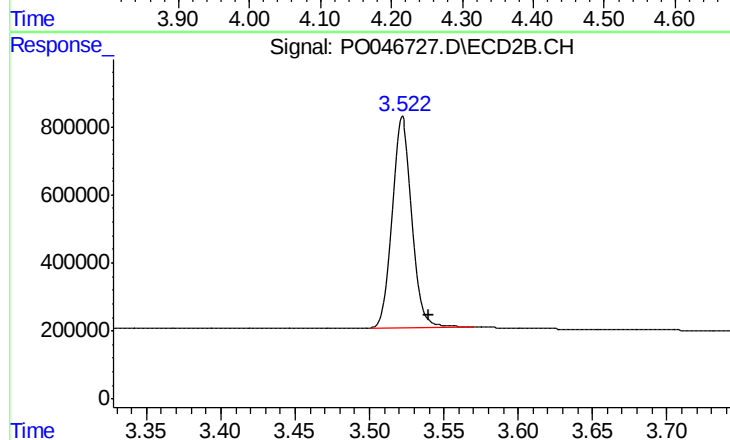


#1 Tetrachloro-m-xylene

R.T.: 3.522 min
Delta R.T.: -0.018 min
Response: 5758385
Conc: 27.11 ng/ml

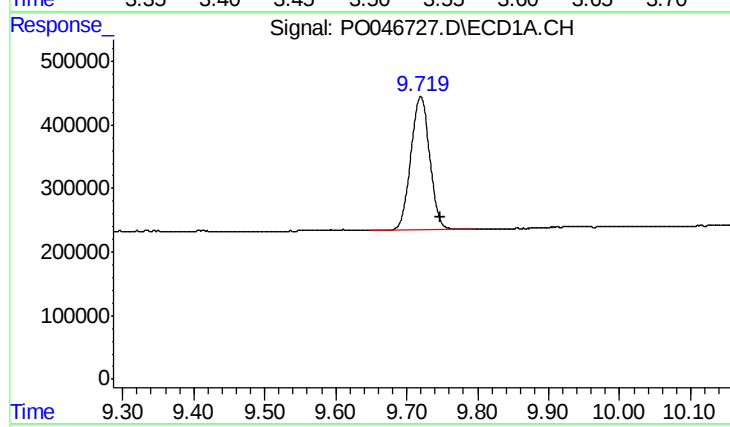

#2 Decachlorobiphenyl

R.T.: 9.720 min
Delta R.T.: -0.028 min
Response: 3869061
Conc: 20.30 ng/ml

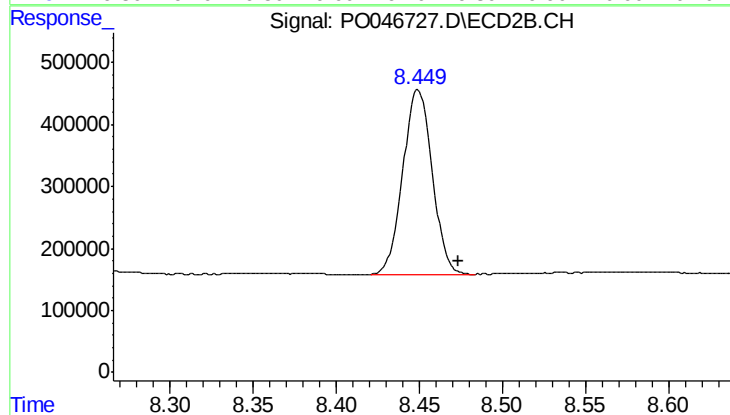

#2 Decachlorobiphenyl

R.T.: 8.449 min
Delta R.T.: -0.024 min
Response: 3657132
Conc: 18.85 ng/ml