

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0071418\
 Data File : P0046731.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Jul 2018 9:10
 Operator : SM/SJ
 Sample : J3961-01
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1-6-30-GAL-55-GAL-1-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 10:02:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 09 15:27:34 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

	System Monitoring Compounds						
1)	SA Tetrachlo...	4.200	3.526	5014785	4857294	20.984	22.868
2)	SA Decachlor...	9.725	8.454	3850767	3664707	20.203	18.892

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0071418\
Data File : P0046731.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Jul 2018 9:10
Operator : SM/SJ
Sample : J3961-01
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
1-6-30-GAL-55-GAL-1-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 10:02:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

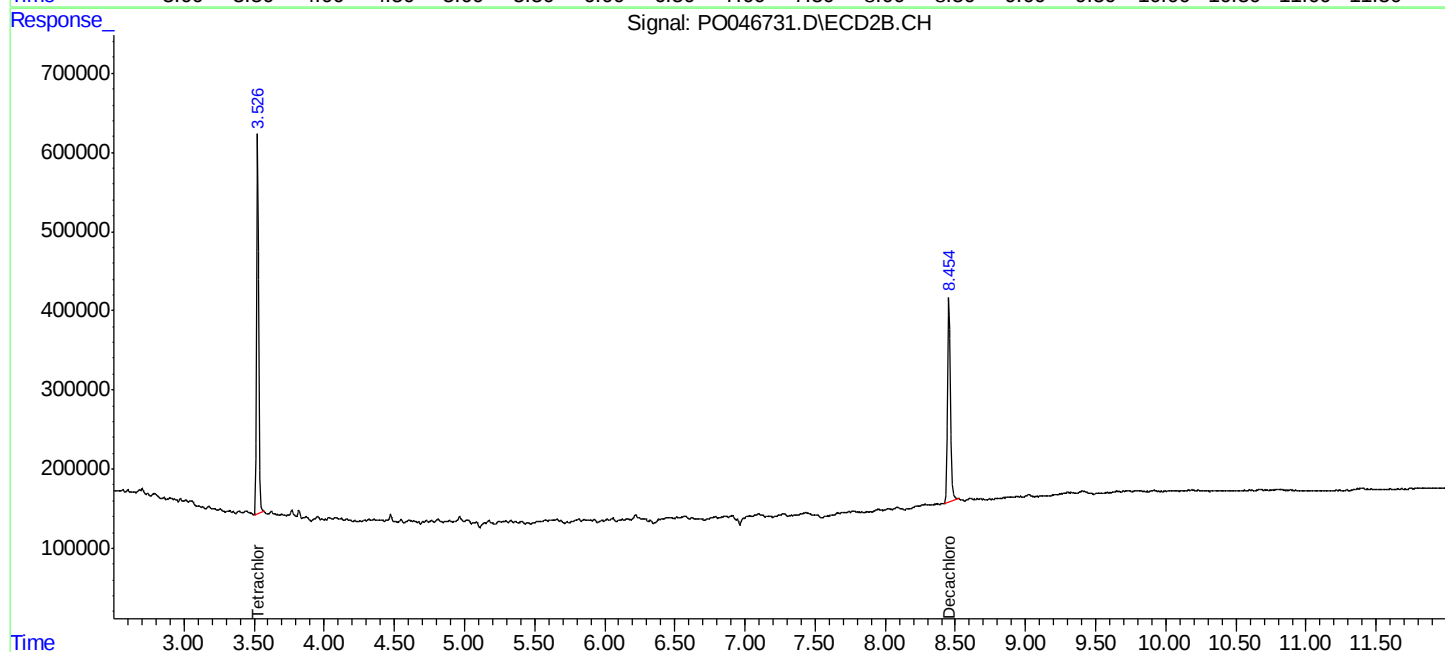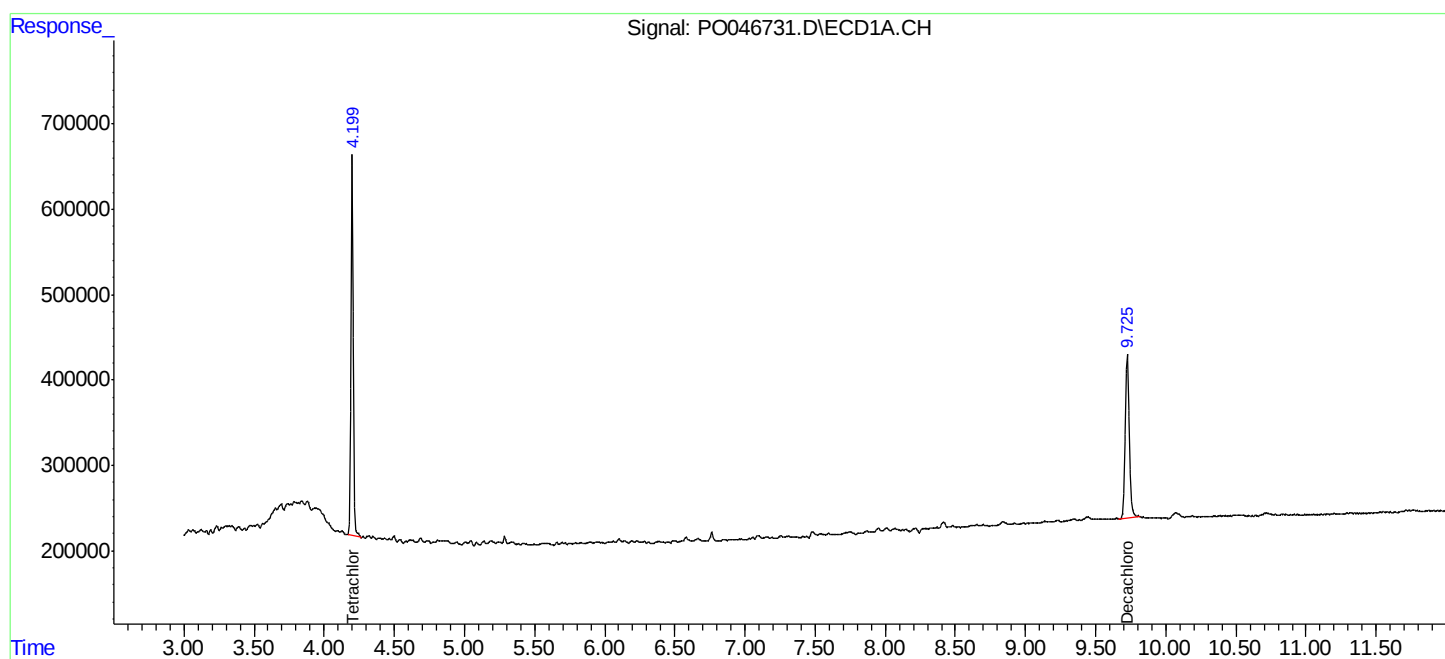


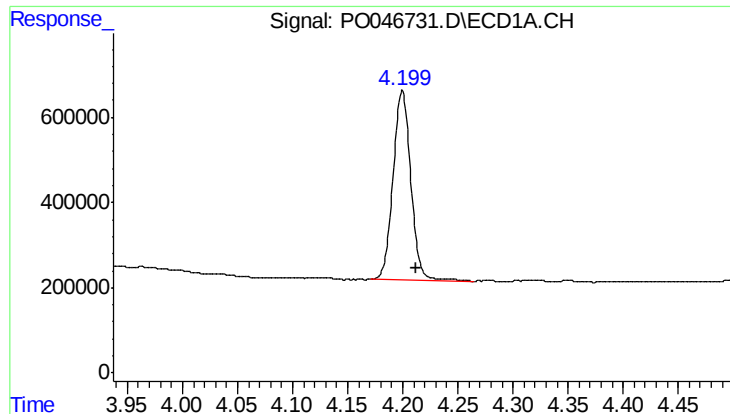

#1 Tetrachloro-m-xylene


R.T.: 4.200 min
Delta R.T.: -0.013 min
Response: 5014785
Conc: 20.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
1-6-30-GAL-55-GAL-1-6

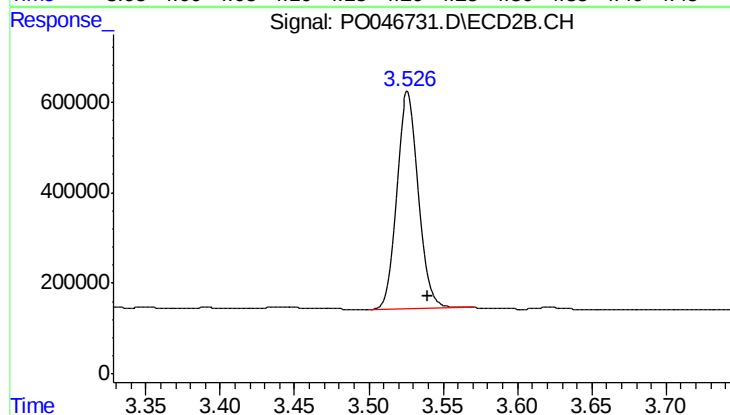


#1 Tetrachloro-m-xylene

R.T.: 3.526 min
Delta R.T.: -0.013 min
Response: 4857294
Conc: 22.87 ng/ml

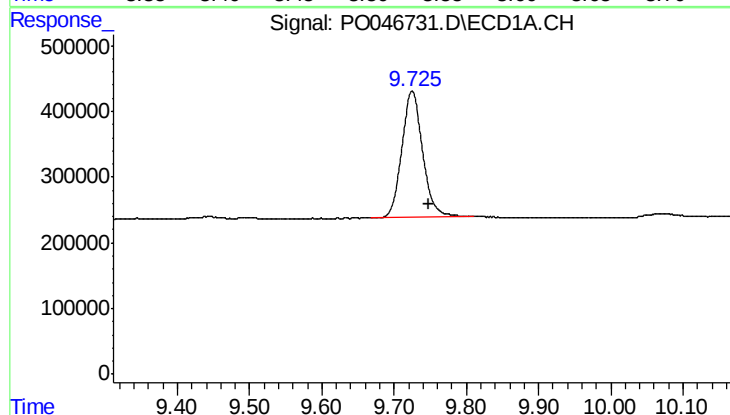

#2 Decachlorobiphenyl

R.T.: 9.725 min
Delta R.T.: -0.023 min
Response: 3850767
Conc: 20.20 ng/ml

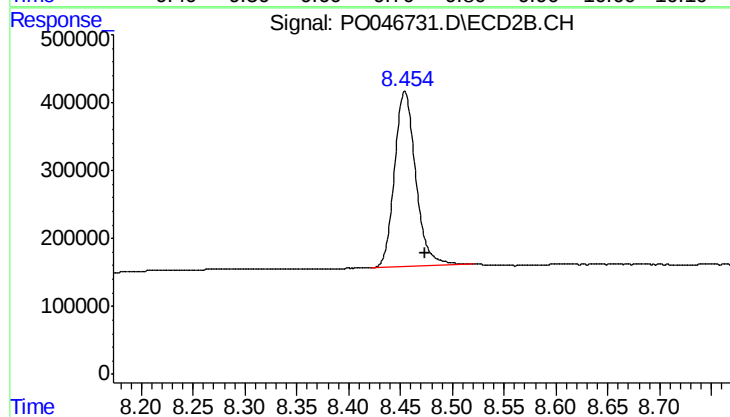

#2 Decachlorobiphenyl

R.T.: 8.454 min
Delta R.T.: -0.019 min
Response: 3664707
Conc: 18.89 ng/ml