

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0071418\
Data File : P0046734.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Jul 2018 9:58
Operator : SM/SJ
Sample : J3948-01
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-ST-PH4-AREA

Manual Integrations
APPROVED

Sohil
7/17/2018 3:36:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 10:06:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.198	3.526	5336017	6596575	22.328m	31.056 #
2)	SA Decachlor...	9.722	8.452	4662095	4049135	24.459	20.874

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0071418\
Data File : P0046734.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Jul 2018 9:58
Operator : SM/SJ
Sample : J3948-01
Misc :
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-ST-PH4-AREA


Manual Integrations
APPROVED

Sohil
7/17/2018 3:36:04 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 10:06:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

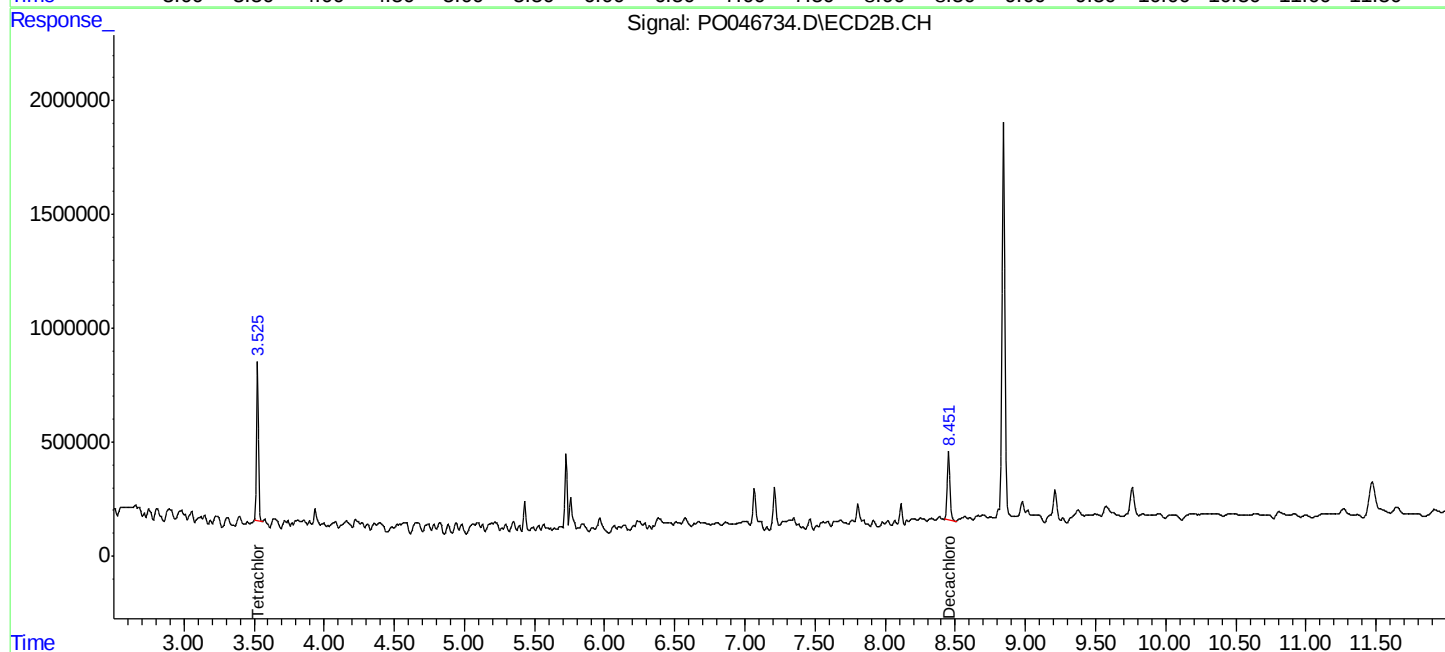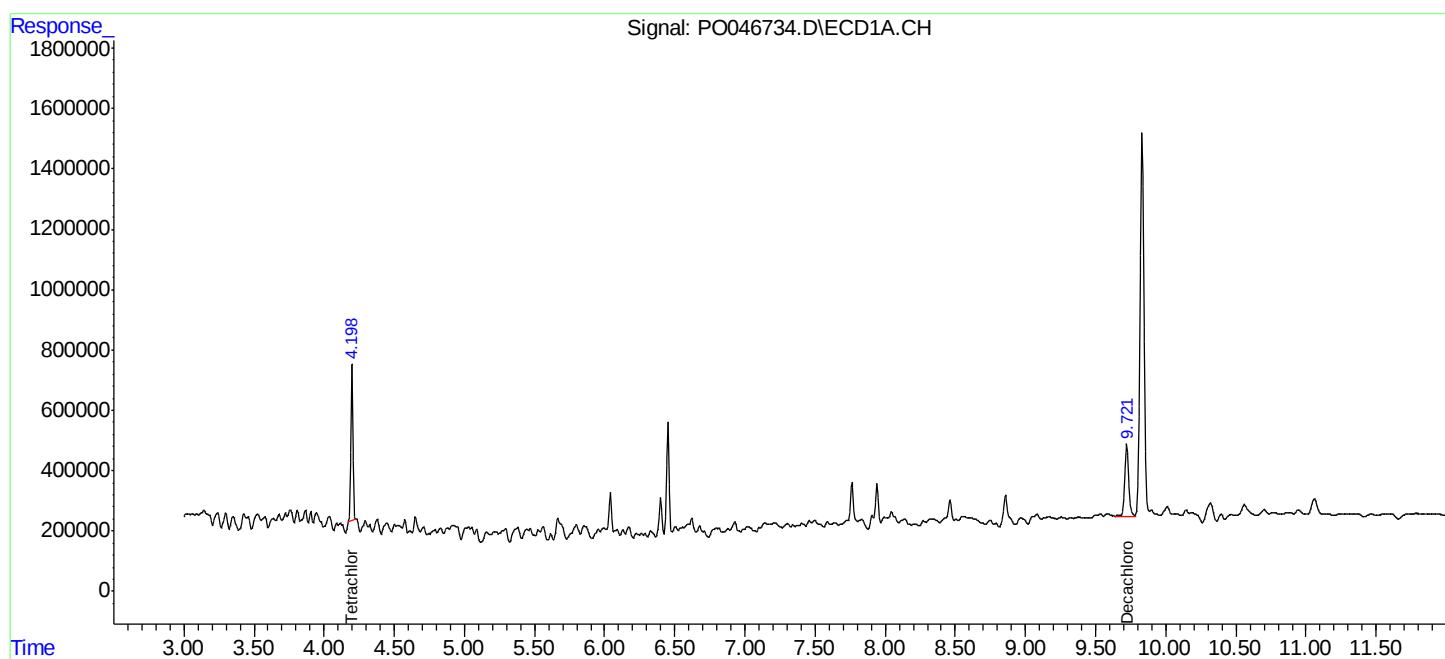

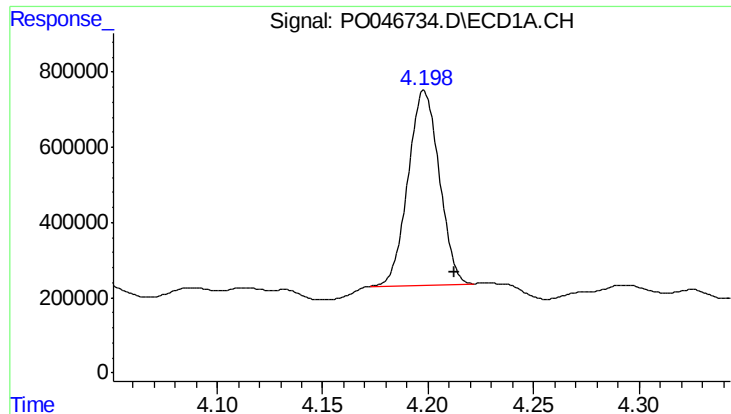


#1 Tetrachloro-m-xylene

R.T.: 4.198 min
Delta R.T.: -0.015 min
Response: 5336017
Conc: 22.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-ST-PH4-AREA


Manual Integrations
APPROVED

Sohil
7/17/2018 3:36:04 PM

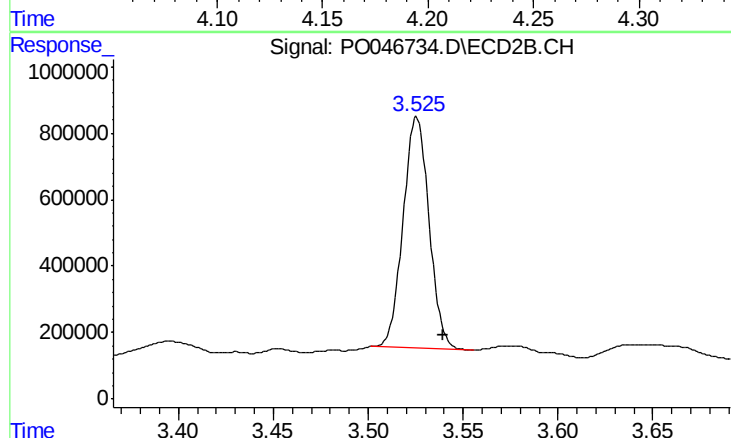


#1 Tetrachloro-m-xylene

R.T.: 3.526 min
Delta R.T.: -0.014 min
Response: 6596575
Conc: 31.06 ng/ml

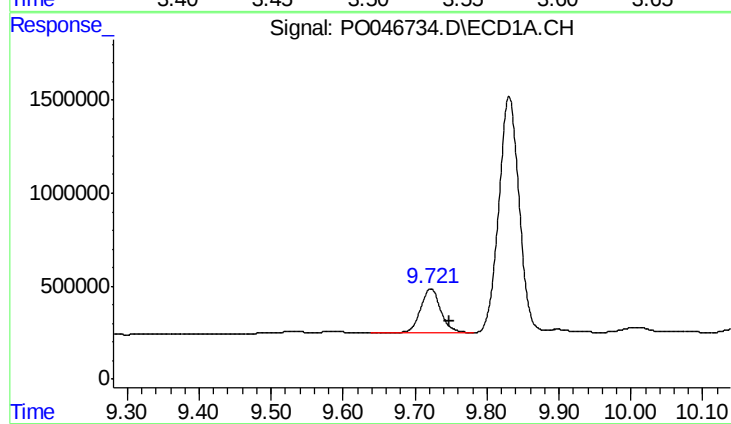

#2 Decachlorobiphenyl

R.T.: 9.722 min
Delta R.T.: -0.026 min
Response: 4662095
Conc: 24.46 ng/ml

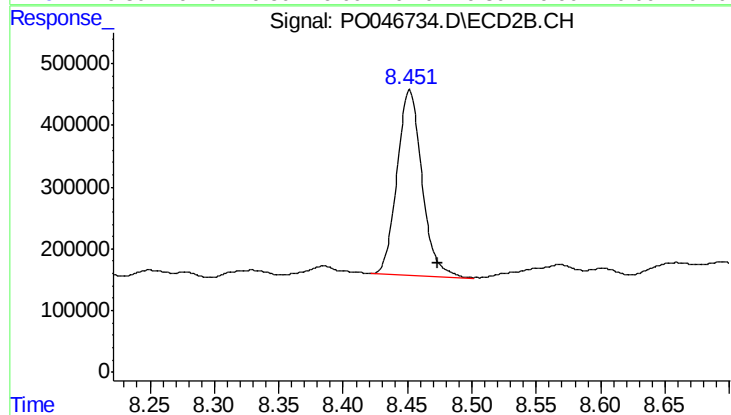

#2 Decachlorobiphenyl

R.T.: 8.452 min
Delta R.T.: -0.022 min
Response: 4049135
Conc: 20.87 ng/ml