

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0071418\
Data File : P0046735.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Jul 2018 10:14
Operator : SM/SJ
Sample : J3948-03
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-ST-PH4-AREA

Manual Integrations
APPROVED

Sohil
7/17/2018 3:36:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 10:07:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.198	3.525	4851492	6015561	20.300m	28.321 #
2) SA Decachlor...	9.720	8.451	3038642	2786834	15.942m	14.367

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0071418\
Data File : P0046735.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Jul 2018 10:14
Operator : SM/SJ
Sample : J3948-03
Misc :
ALS Vial : 46 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-ST-PH4-AREA


Manual Integrations
APPROVED

Sohil
7/17/2018 3:36:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 10:07:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

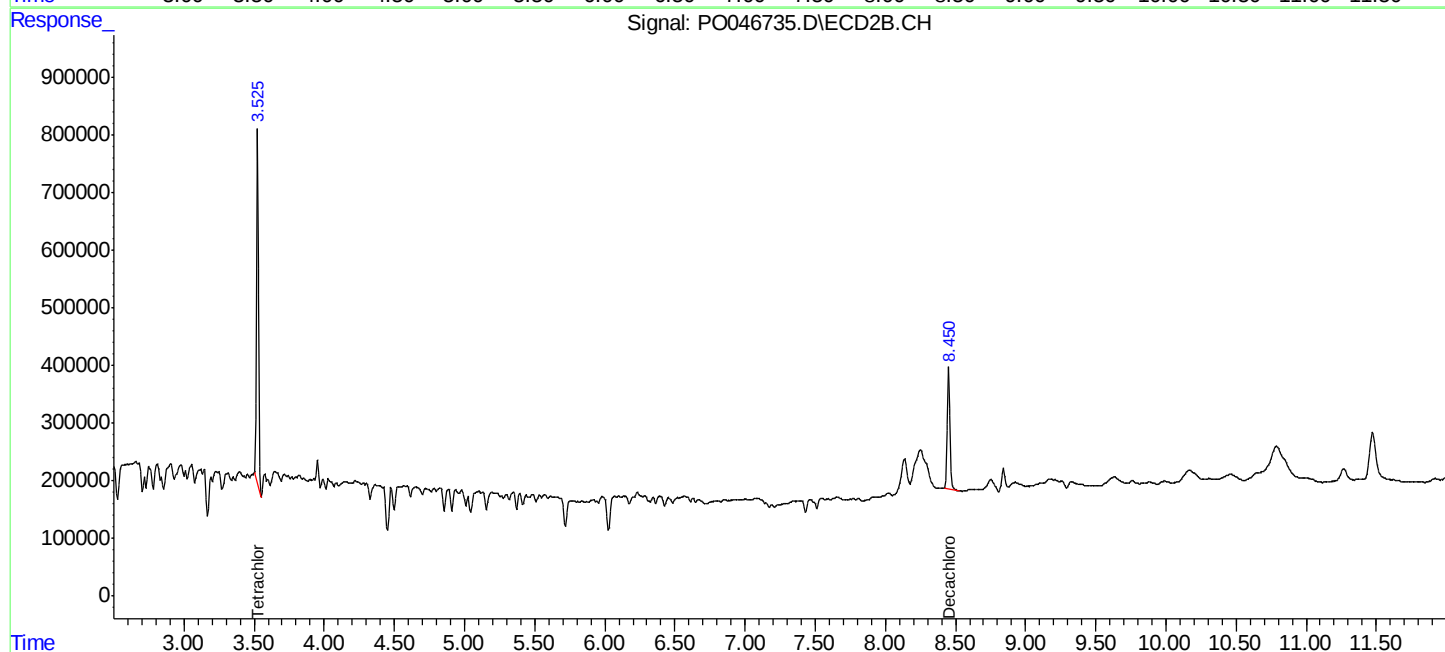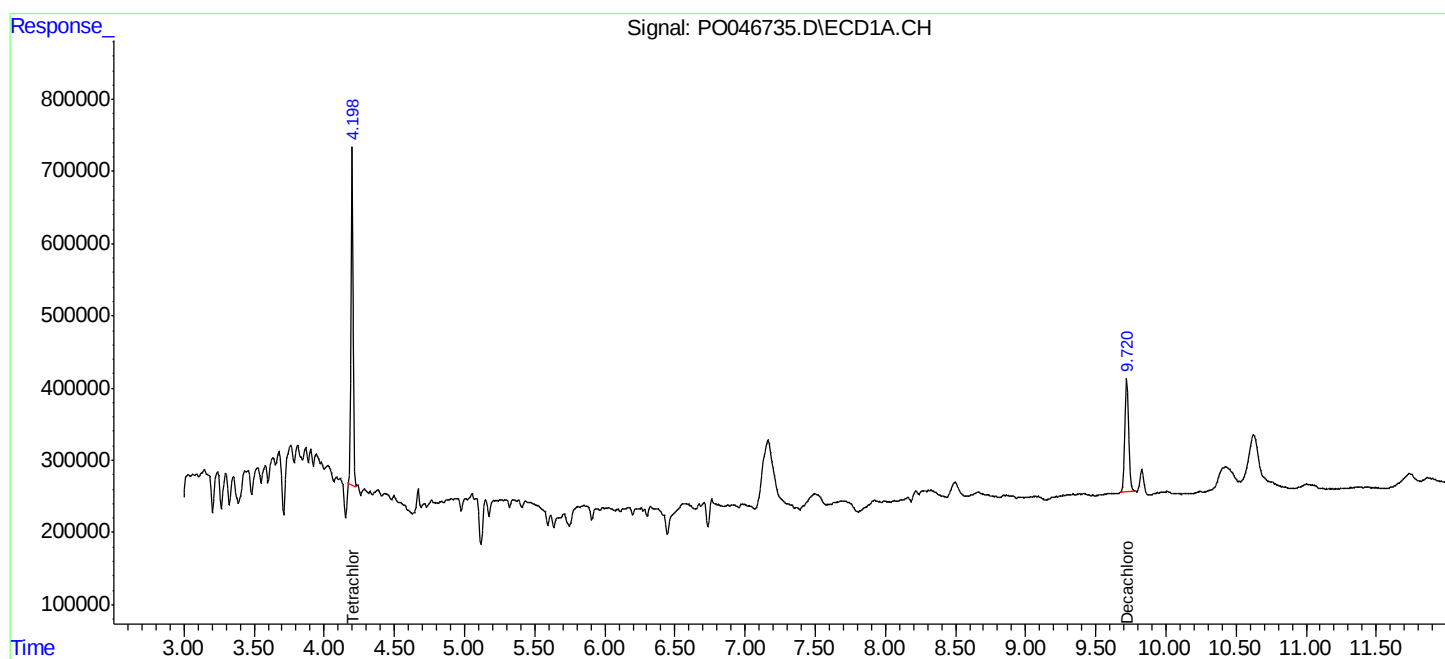

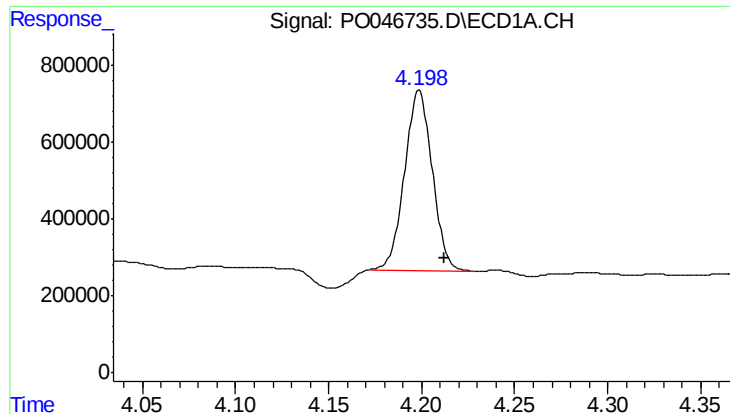


#1 Tetrachloro-m-xylene

R.T.: 4.198 min
Delta R.T.: -0.014 min
Response: 4851492
Conc: 20.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-ST-PH4-AREA


Manual Integrations
APPROVED

Sohil
7/17/2018 3:36:05 PM

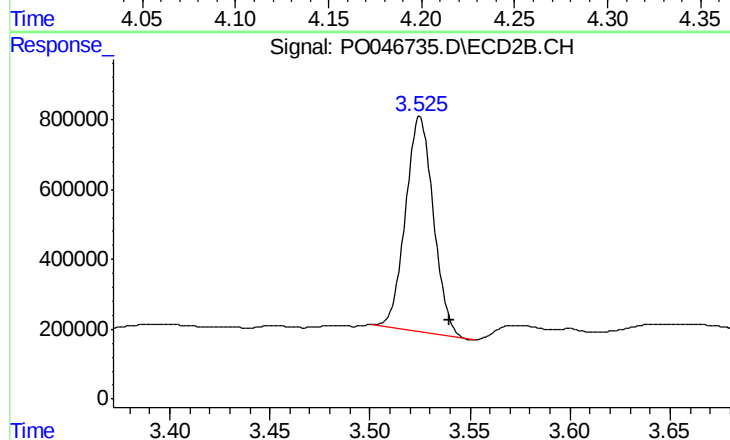


#1 Tetrachloro-m-xylene

R.T.: 3.525 min
Delta R.T.: -0.015 min
Response: 6015561
Conc: 28.32 ng/ml

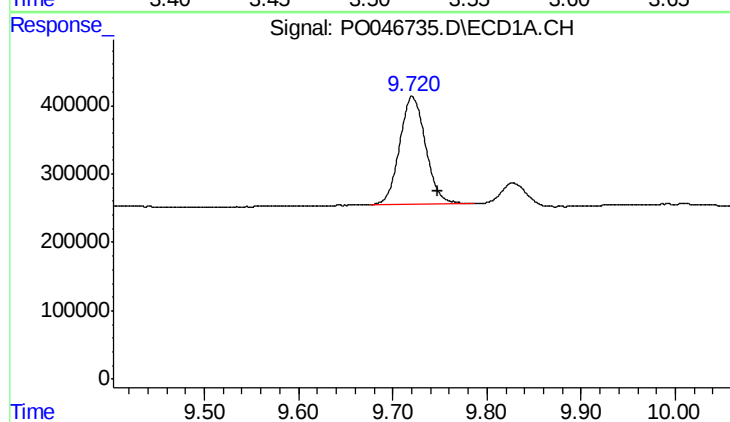

#2 Decachlorobiphenyl

R.T.: 9.720 min
Delta R.T.: -0.028 min
Response: 3038642
Conc: 15.94 ng/ml m

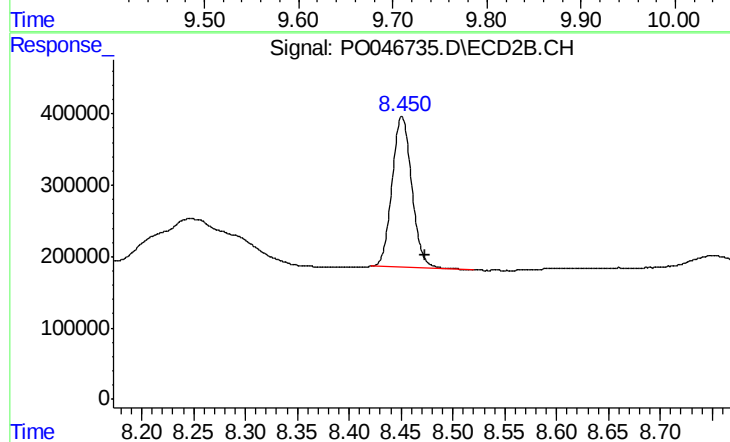

#2 Decachlorobiphenyl

R.T.: 8.451 min
Delta R.T.: -0.022 min
Response: 2786834
Conc: 14.37 ng/ml