

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071419\
 Data File : P0057935.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jul 2019 10:36
 Operator : SM/AJ
 Sample : K3801-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S12-14-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 01:27:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.204	3.542	826981	757202	21.053	21.534
2) SA Decachlor...	9.727	8.449	307986	703658	5.477	18.811 #
Target Compounds						
12) L3 AR-1232-2	5.184	0.000	58325	0	120.361	N.D. #
27) L6 AR-1254-2	6.476	0.000	41170	0	13.209	N.D. #
29) L6 AR-1254-4	0.000	6.205	0	26613	N.D.	14.784 #
30) L6 AR-1254-5	7.508	6.574	97343	81183	34.816	29.967
32) L7 AR-1260-2	7.200	6.205	64588	26613	17.520	9.700 #
36) L8 AR-1262-1	0.000	6.574	0	81183	N.D.	21.688 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071419\
Data File : PO057935.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jul 2019 10:36
Operator : SM/AJ
Sample : K3801-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
S12-14-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 01:27:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

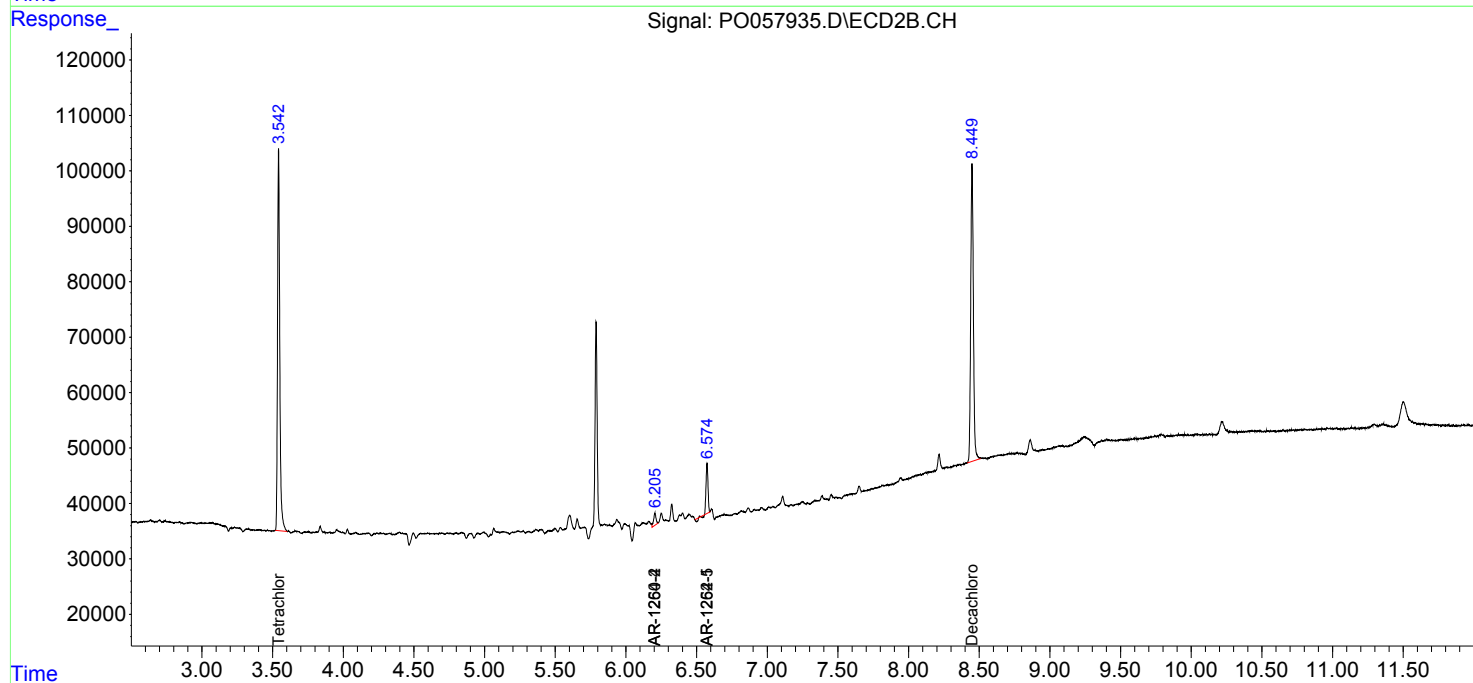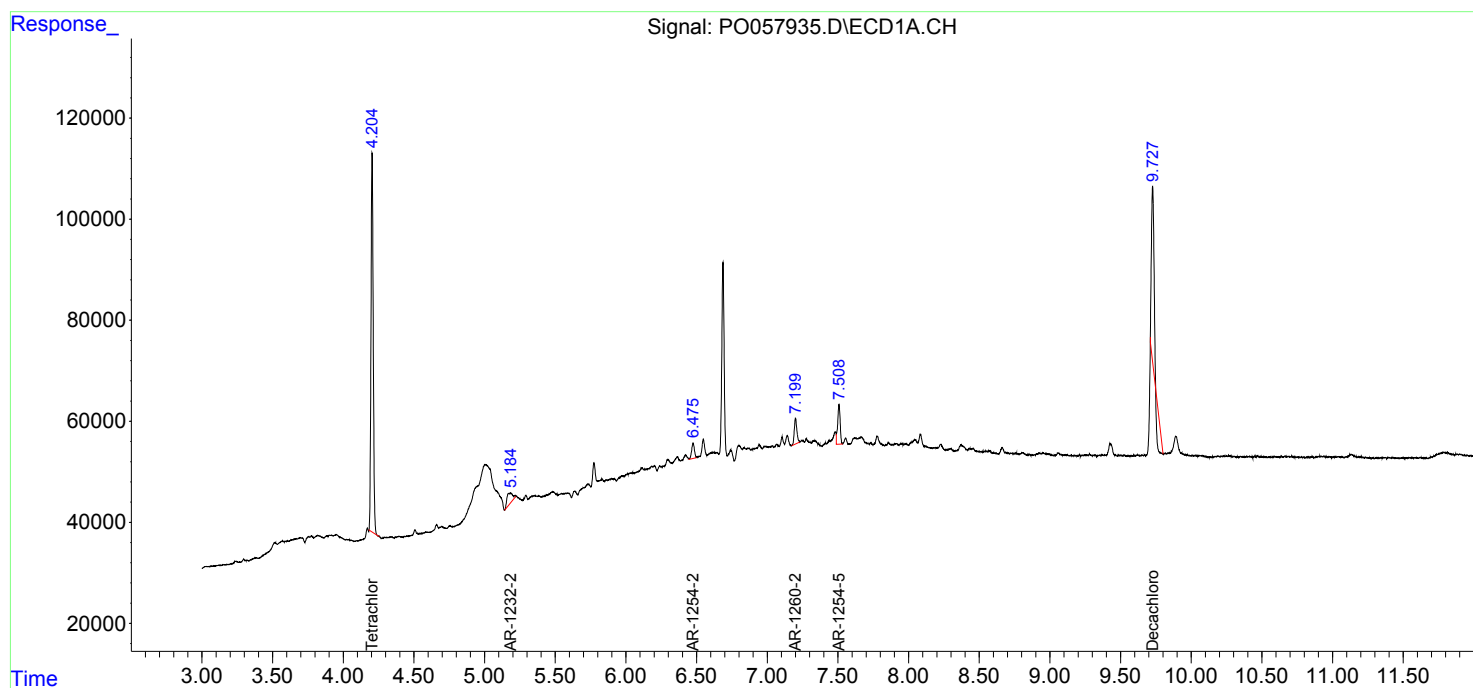


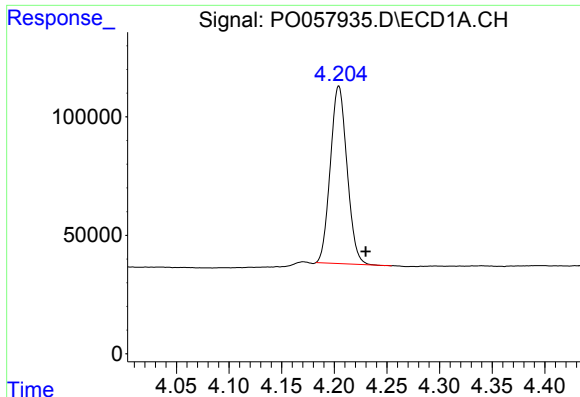

#1 Tetrachloro-m-xylene


R.T.: 4.204 min
Delta R.T.: -0.026 min
Response: 826981
Conc: 21.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
S12-14-B

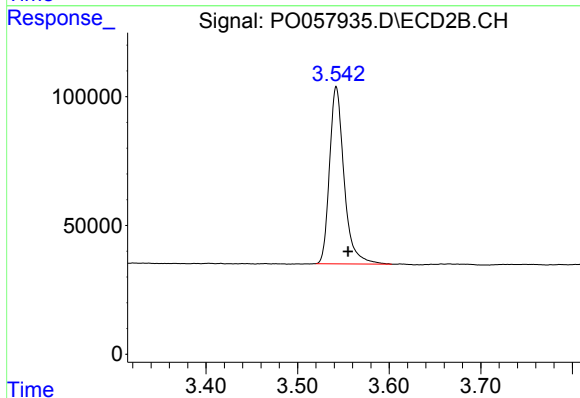


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: -0.013 min
Response: 757202
Conc: 21.53 ng/ml

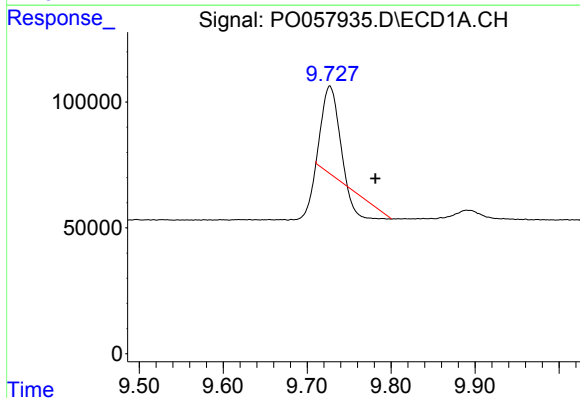


#2 Decachlorobiphenyl

R.T.: 9.727 min
Delta R.T.: -0.054 min
Response: 307986
Conc: 5.48 ng/ml

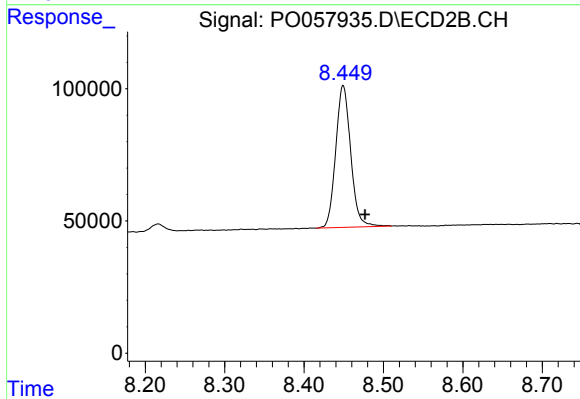

#2 Decachlorobiphenyl


R.T.: 8.449 min
Delta R.T.: -0.028 min
Response: 703658
Conc: 18.81 ng/ml

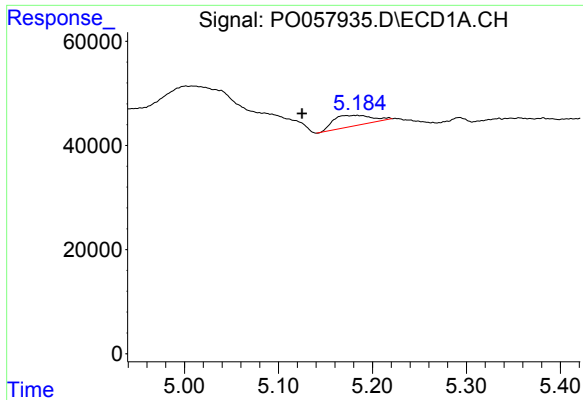

#12 AR-1232-2


R.T.: 5.184 min
Delta R.T.: 0.058 min
Response: 58325
Conc: 120.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
S12-14-B

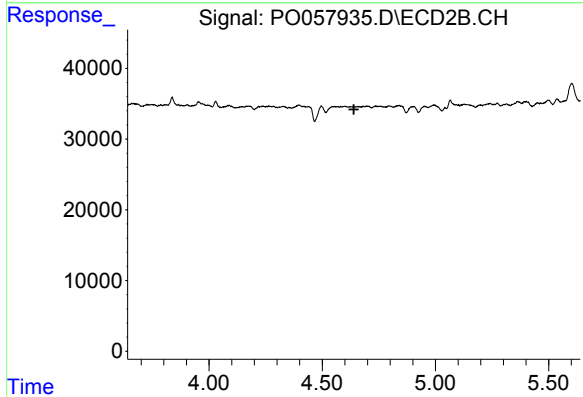


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 4.640 min
Response: 0
Conc: N.D.

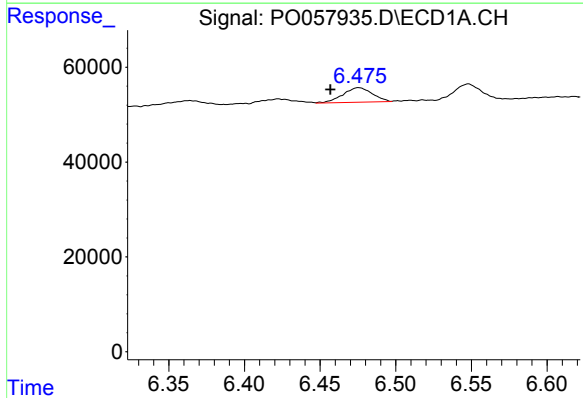


#27 AR-1254-2

R.T.: 6.476 min
Delta R.T.: 0.019 min
Response: 41170
Conc: 13.21 ng/ml

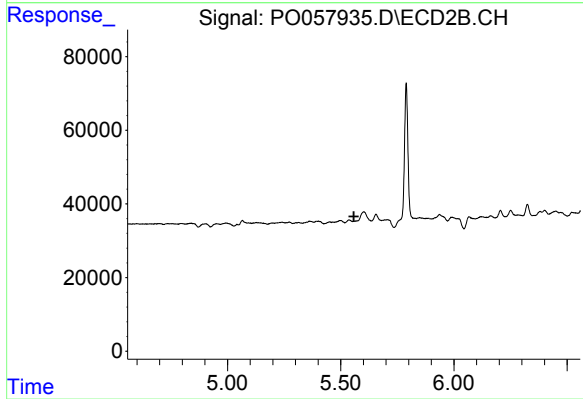

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T. : 5.558 min
Response: 0
Conc: N.D.

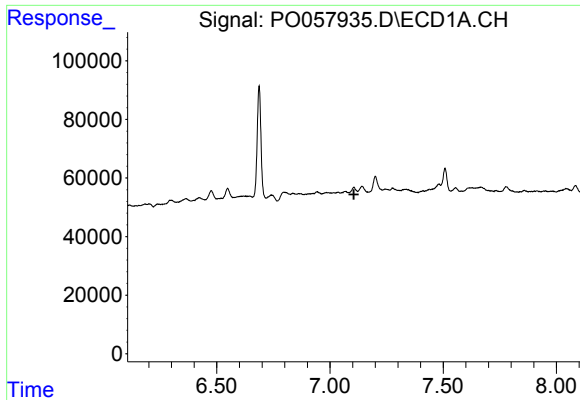

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.106 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
S12-14-B

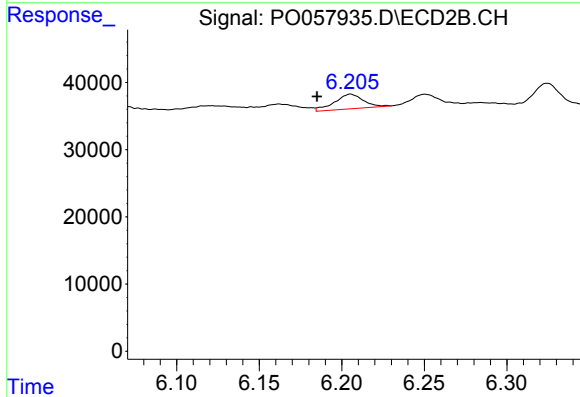


#29 AR-1254-4

R.T.: 6.205 min
Delta R.T.: 0.020 min
Response: 26613
Conc: 14.78 ng/ml

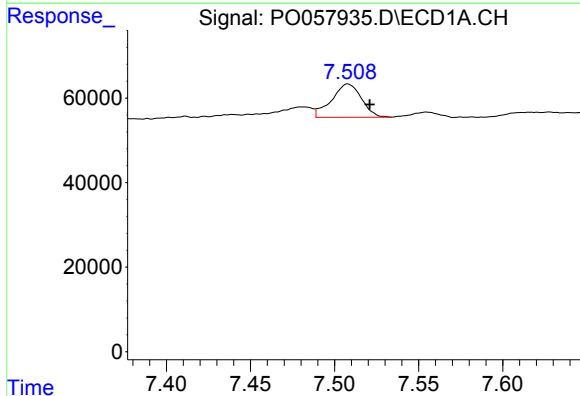


#30 AR-1254-5

R.T.: 7.508 min
Delta R.T.: -0.013 min
Response: 97343
Conc: 34.82 ng/ml

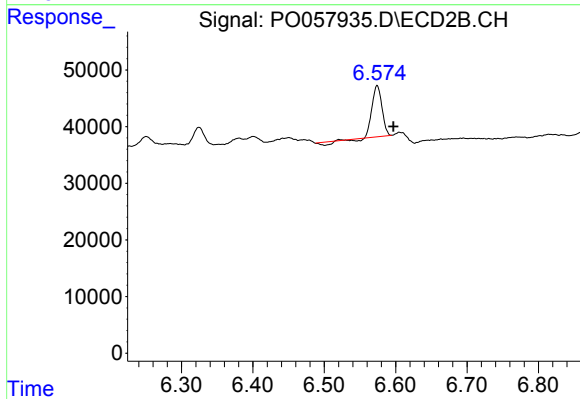

#30 AR-1254-5


R.T.: 6.574 min
Delta R.T.: -0.023 min
Response: 81183
Conc: 29.97 ng/ml

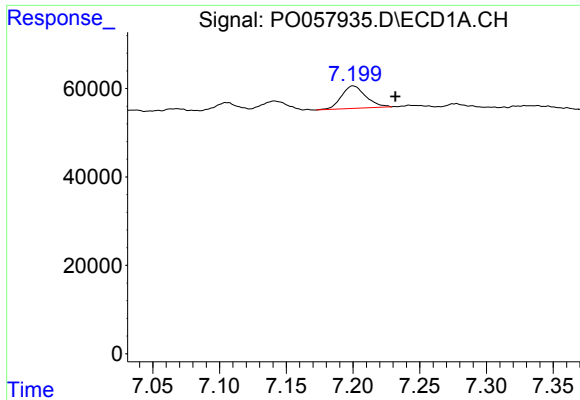

#32 AR-1260-2


R.T.: 7.200 min
Delta R.T.: -0.032 min
Response: 64588
Conc: 17.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
S12-14-B

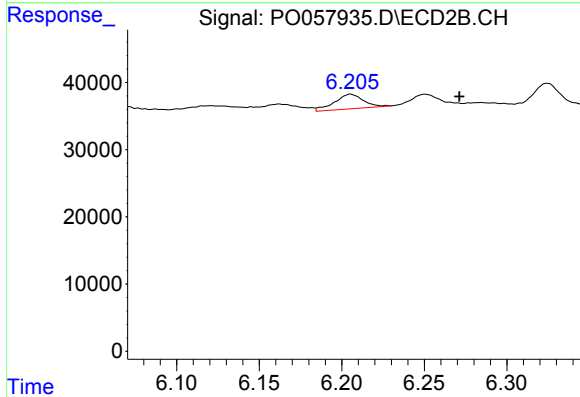


#32 AR-1260-2

R.T.: 6.205 min
Delta R.T.: -0.066 min
Response: 26613
Conc: 9.70 ng/ml

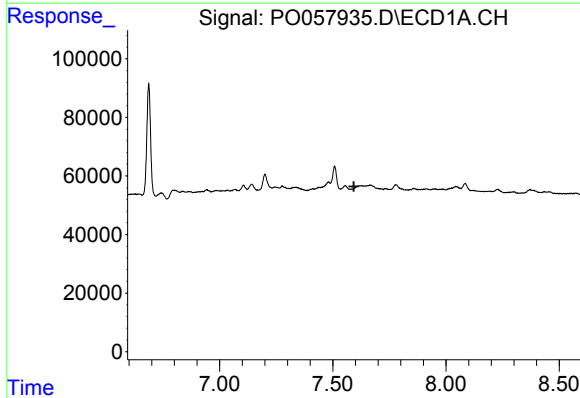

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.593 min
Response: 0
Conc: N.D.

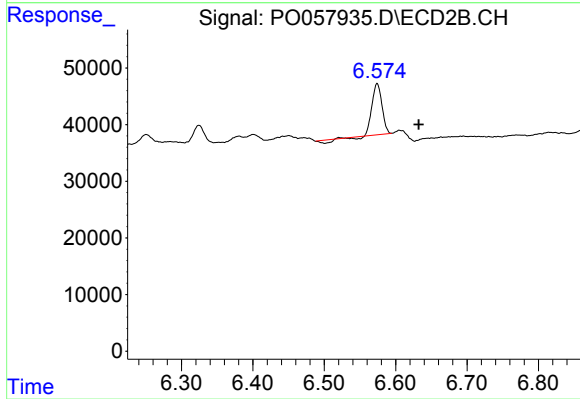

#36 AR-1262-1

R.T.: 6.574 min
Delta R.T.: -0.058 min
Response: 81183
Conc: 21.69 ng/ml