

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071419\
 Data File : P0057933.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jul 2019 10:02
 Operator : SM/AJ
 Sample : K3801-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S12-13-B

Manual Integrations
 APPROVED

Ankita
 7/16/2019 10:18:38 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 02:05:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.204	3.542	951017	826755	24.210	23.512
2) SA Decachlor...	9.726	8.450	1020052	717911	18.140m	19.192

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071419\
Data File : PO057933.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jul 2019 10:02
Operator : SM/AJ
Sample : K3801-05
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S12-13-B


Manual Integrations
APPROVED

Ankita
7/16/2019 10:18:38 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 02:05:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

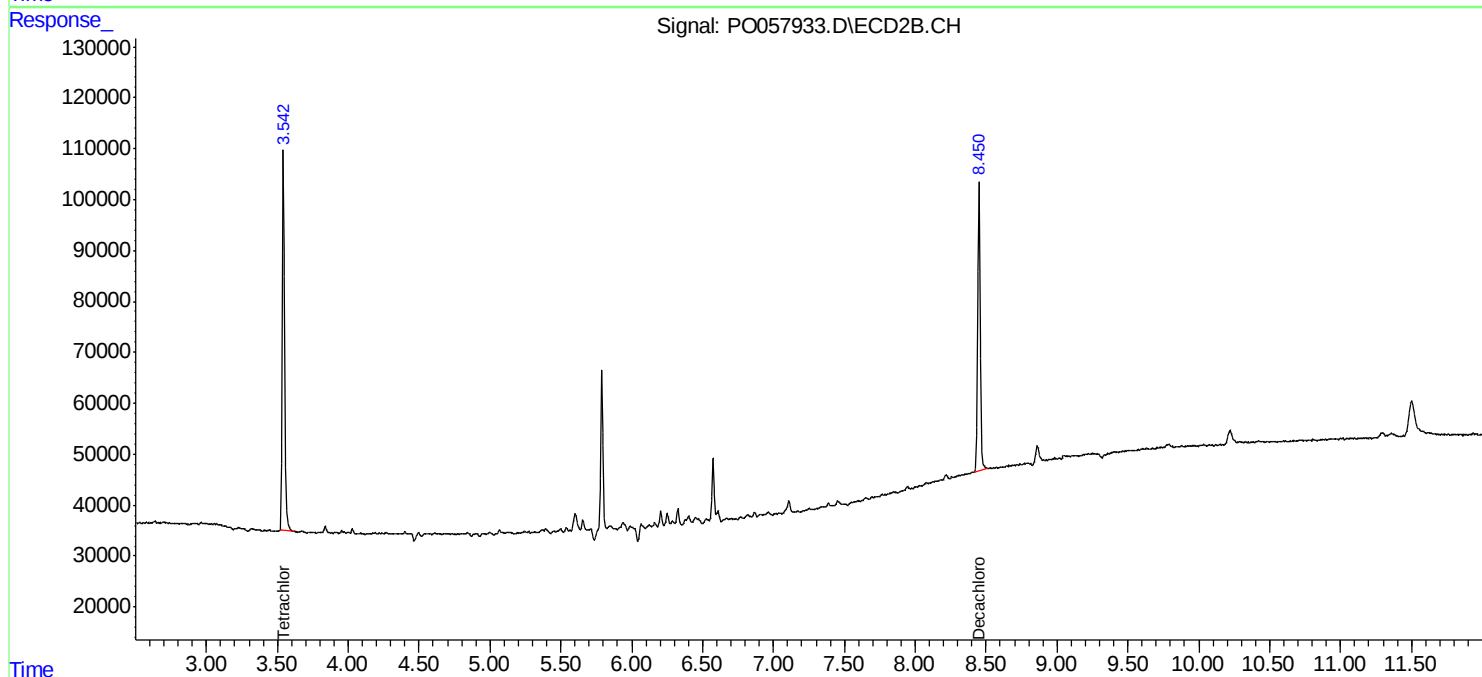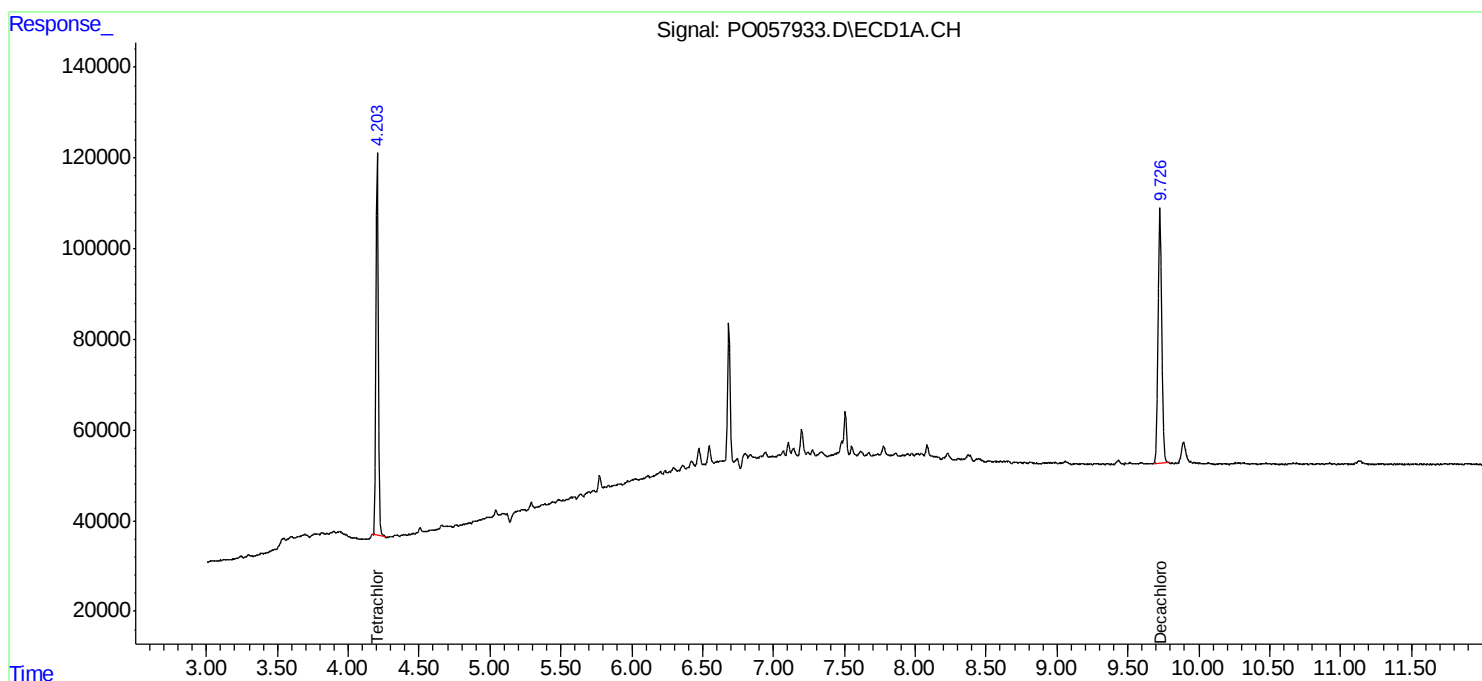

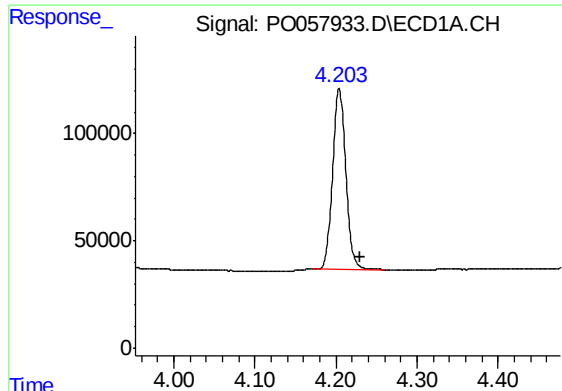


#1 Tetrachloro-m-xylene

R.T.: 4.204 min
Delta R.T.: -0.026 min
Response: 951017
Conc: 24.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
S12-13-B


Manual Integrations
APPROVED

Ankita
7/16/2019 10:18:38 AM

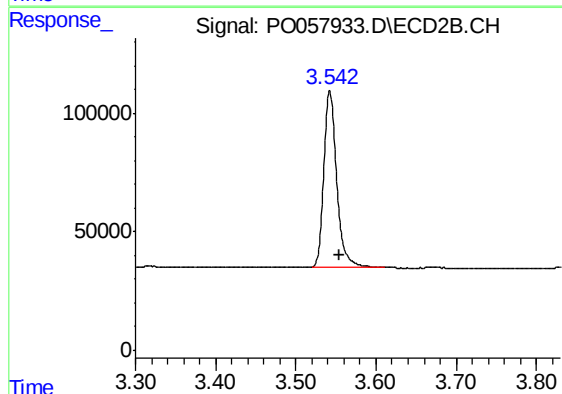


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: -0.013 min
Response: 826755
Conc: 23.51 ng/ml

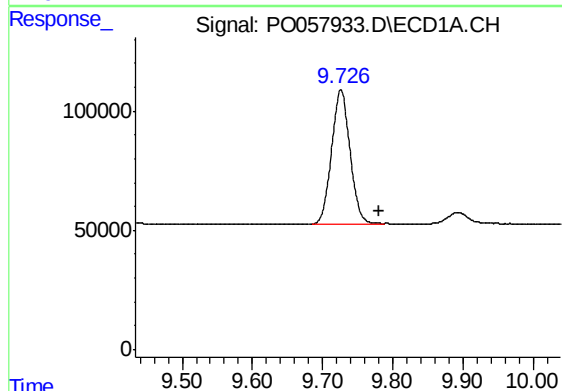

#2 Decachlorobiphenyl

R.T.: 9.726 min
Delta R.T.: -0.056 min
Response: 1020052
Conc: 18.14 ng/ml m

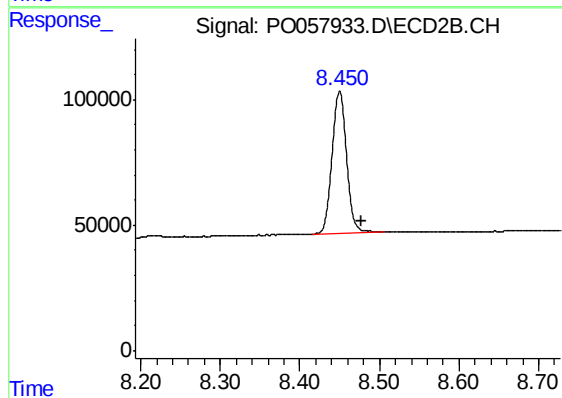

#2 Decachlorobiphenyl

R.T.: 8.450 min
Delta R.T.: -0.027 min
Response: 717911
Conc: 19.19 ng/ml