

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071420\
 Data File : P0069622.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jul 2020 15:21
 Operator : DD\AJ
 Sample : L3282-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ST-JOES-AVE-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 17:49:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 08 16:12:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.391	3.564	1107151	1178592	29.654	29.616
2)	SA Decachlor...	10.051	8.771	1262939	1124004	20.991	19.805
Target Compounds							
27)	L6 AR-1254-2	6.822	0.000	280124	0	87.260	N.D. #
28)	L6 AR-1254-3	7.200	6.226	351554	203723	100.098	54.246 #
29)	L6 AR-1254-4	7.495	6.467	137505	39350	45.944	15.571 #
30)	L6 AR-1254-5	7.918	6.890	102212	125046	33.971	34.842
31)	L7 AR-1260-1	7.363	6.363	213103	132047	81.046	50.064 #
32)	L7 AR-1260-2	7.632	6.563	69296	101991	19.534	31.160 #
33)	L7 AR-1260-3	0.000	6.709	0	68275	N.D.	22.425 #
34)	L7 AR-1260-4	8.215	0.000	60817	0	20.533	N.D. #
35)	L7 AR-1260-5	8.532	7.442	100379	82812	14.835	12.922
36)	L8 AR-1262-1	0.000	6.890	0	125046	N.D.	64.757 #
37)	L8 AR-1262-2	8.532	7.442	100379	82812	13.907	12.683
38)	L8 AR-1262-3	8.823f	0.000	56766	0	11.855	N.D. #
39)	L8 AR-1262-4	0.000	7.783	0	83230	N.D.	16.716 #
41)	L9 AR-1268-1	8.823f	0.000	56766	0	6.193	N.D. #
42)	L9 AR-1268-2	0.000	7.783	0	83230	N.D.	11.652 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071420\
Data File : P0069622.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jul 2020 15:21
Operator : DD\AJ
Sample : L3282-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
ST-JOES-AVE-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 17:49:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 08 16:12:41 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

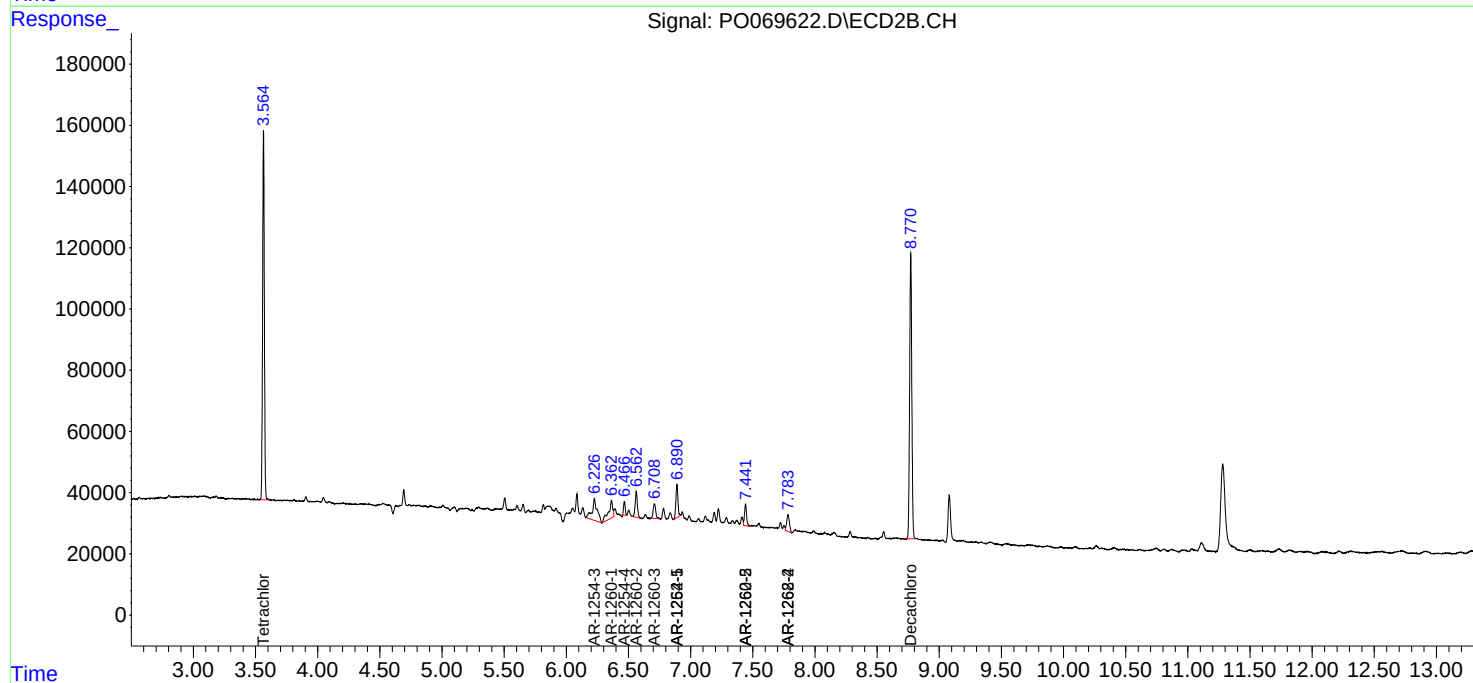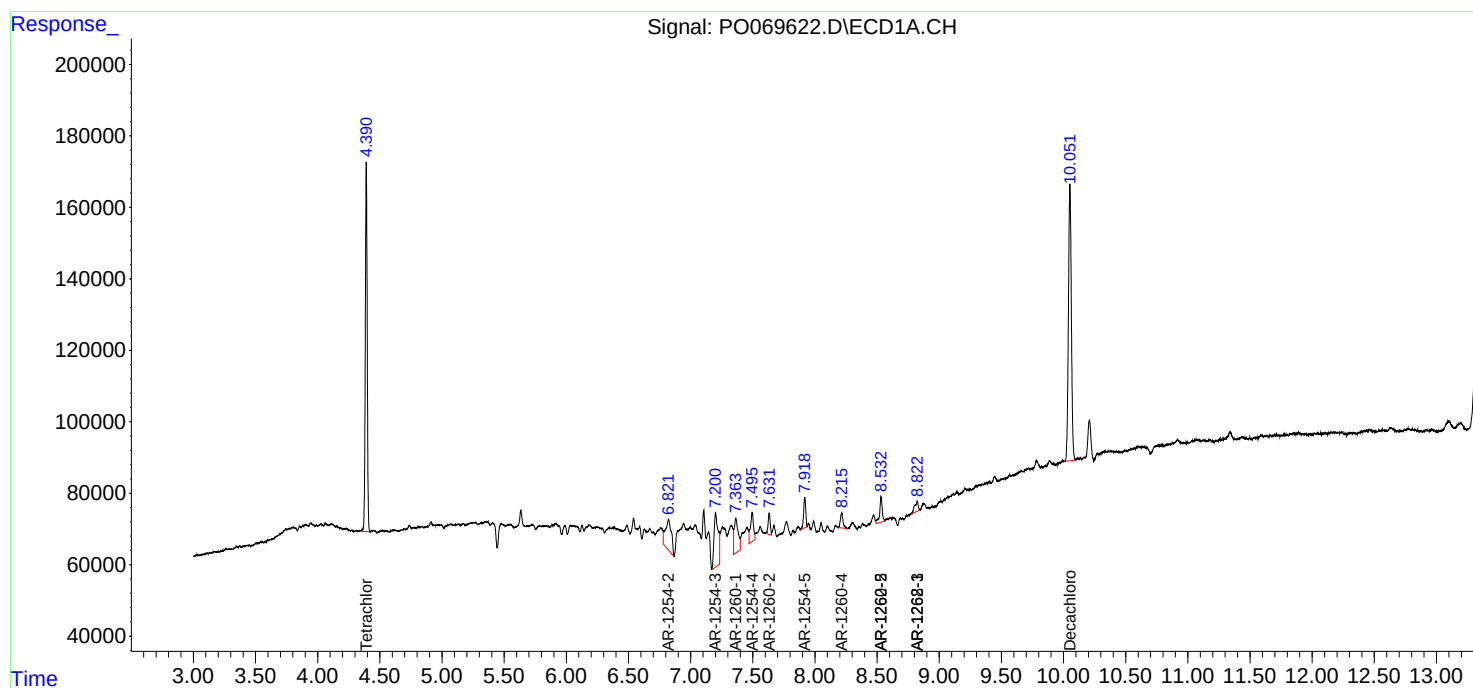


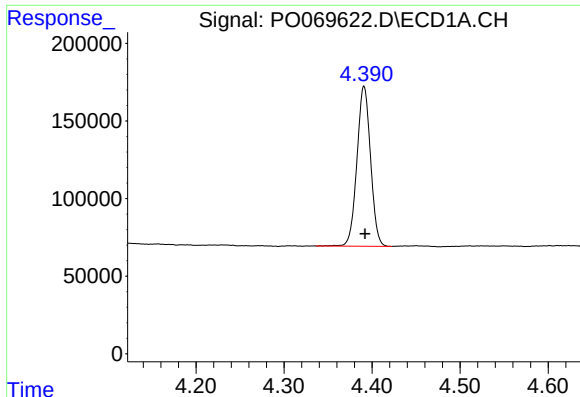

#1 Tetrachloro-m-xylene


R.T.: 4.391 min
Delta R.T.: -0.001 min
Response: 1107151
Conc: 29.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
ST-JOES-AVE-2

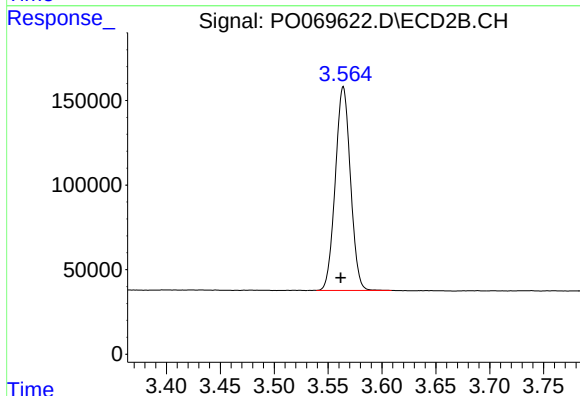


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: 0.002 min
Response: 1178592
Conc: 29.62 ng/ml

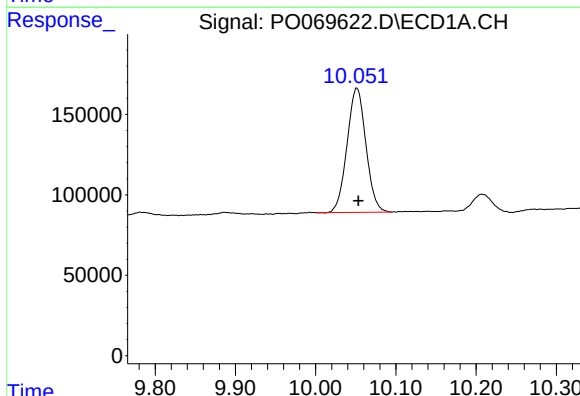


#2 Decachlorobiphenyl

R.T.: 10.051 min
Delta R.T.: -0.002 min
Response: 1262939
Conc: 20.99 ng/ml

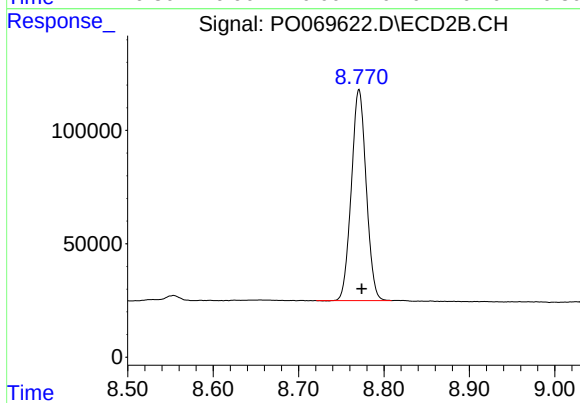

#2 Decachlorobiphenyl


R.T.: 8.771 min
Delta R.T.: -0.003 min
Response: 1124004
Conc: 19.80 ng/ml

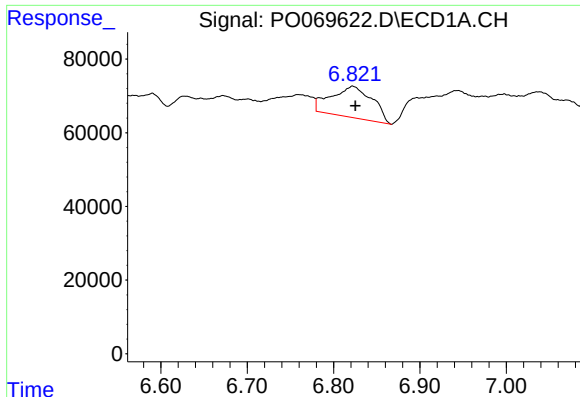

#27 AR-1254-2


R.T.: 6.822 min
Delta R.T.: -0.003 min
Response: 280124
Conc: 87.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
ST-JOES-AVE-2

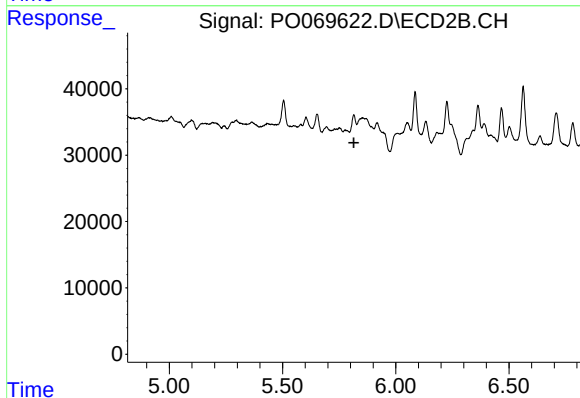


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 5.815 min
Response: 0
Conc: N.D.

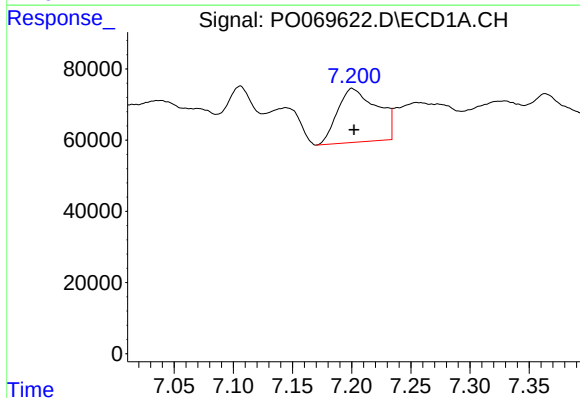


#28 AR-1254-3

R.T.: 7.200 min
Delta R.T.: -0.002 min
Response: 351554
Conc: 100.10 ng/ml

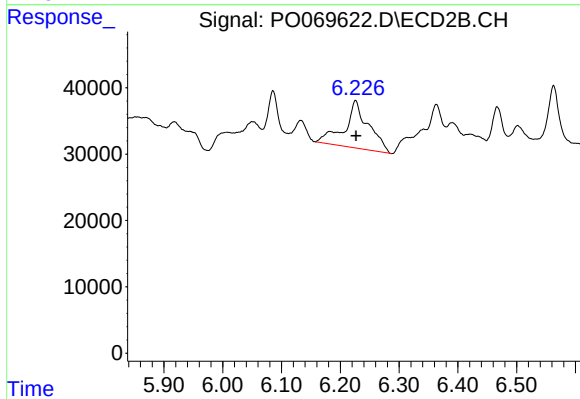

#28 AR-1254-3


R.T.: 6.226 min
Delta R.T.: 0.000 min
Response: 203723
Conc: 54.25 ng/ml

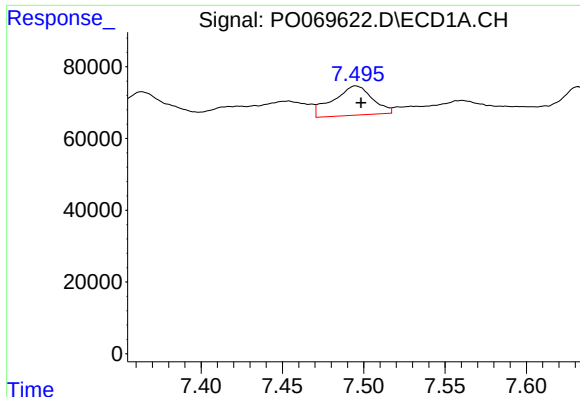

#29 AR-1254-4


R.T.: 7.495 min
Delta R.T.: -0.003 min
Response: 137505
Conc: 45.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
ST-JOES-AVE-2

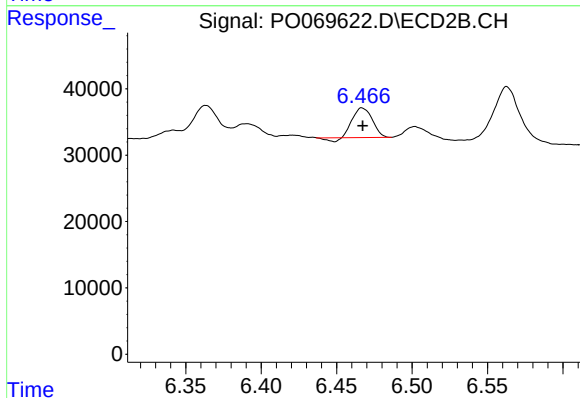


#29 AR-1254-4

R.T.: 6.467 min
Delta R.T.: 0.000 min
Response: 39350
Conc: 15.57 ng/ml

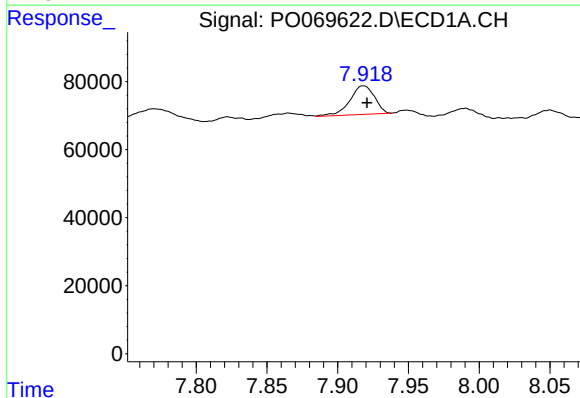


#30 AR-1254-5

R.T.: 7.918 min
Delta R.T.: -0.002 min
Response: 102212
Conc: 33.97 ng/ml

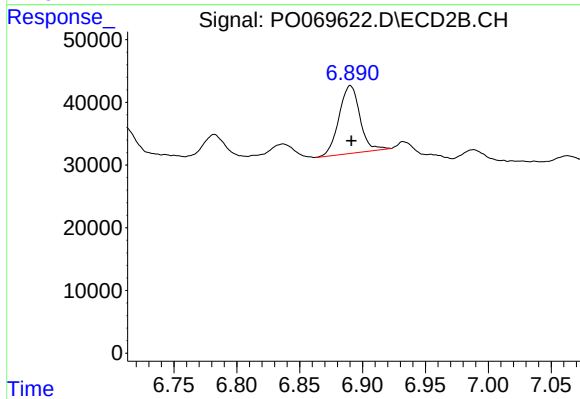

#30 AR-1254-5


R.T.: 6.890 min
Delta R.T.: 0.000 min
Response: 125046
Conc: 34.84 ng/ml

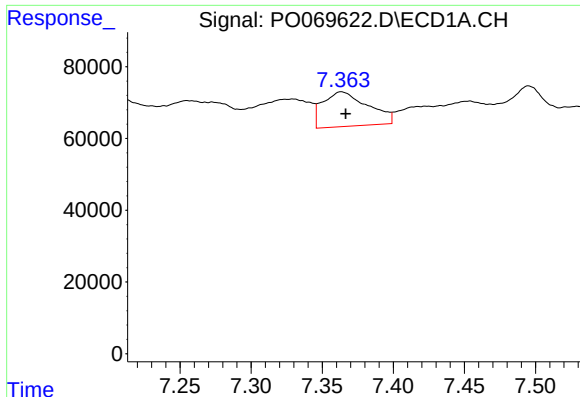

#31 AR-1260-1


R.T.: 7.363 min
Delta R.T.: -0.003 min
Response: 213103
Conc: 81.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
ST-JOES-AVE-2

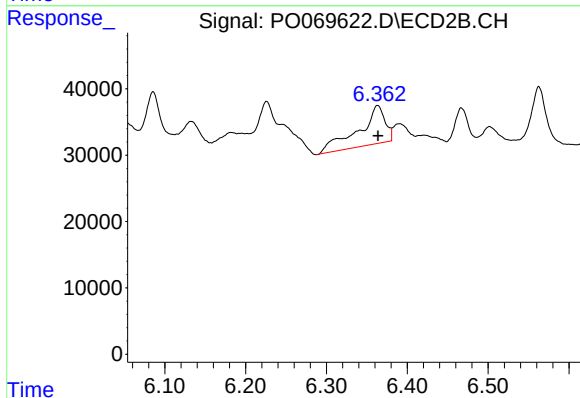


#31 AR-1260-1

R.T.: 6.363 min
Delta R.T.: 0.000 min
Response: 132047
Conc: 50.06 ng/ml

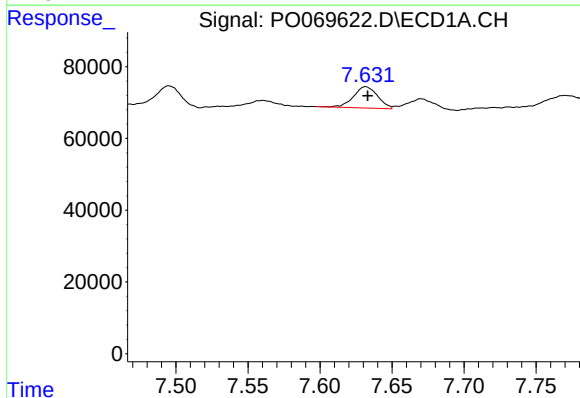


#32 AR-1260-2

R.T.: 7.632 min
Delta R.T.: -0.001 min
Response: 69296
Conc: 19.53 ng/ml

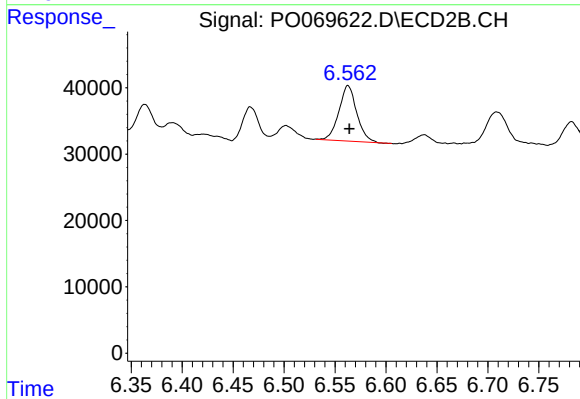

#32 AR-1260-2


R.T.: 6.563 min
Delta R.T.: -0.001 min
Response: 101991
Conc: 31.16 ng/ml

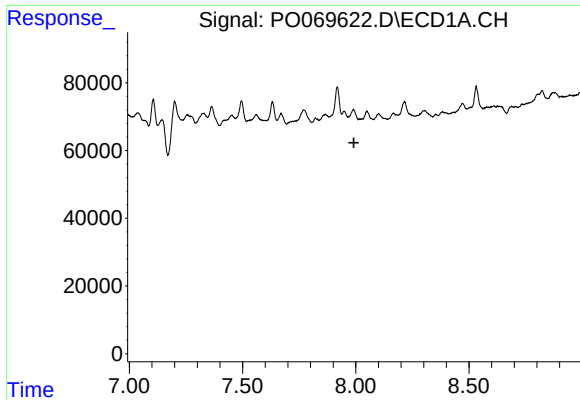

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.992 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
ST-JOES-AVE-2

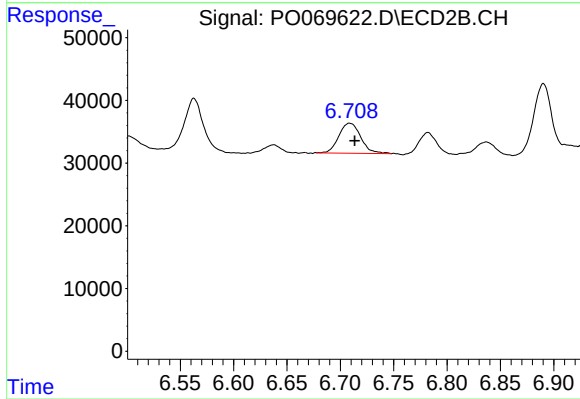


#33 AR-1260-3

R.T.: 6.709 min
Delta R.T.: -0.005 min
Response: 68275
Conc: 22.42 ng/ml

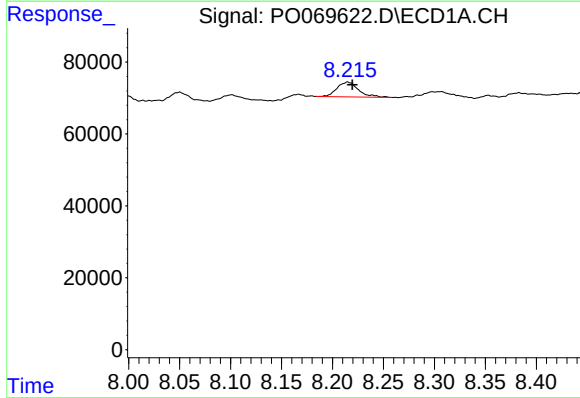


#34 AR-1260-4

R.T.: 8.215 min
Delta R.T.: -0.004 min
Response: 60817
Conc: 20.53 ng/ml

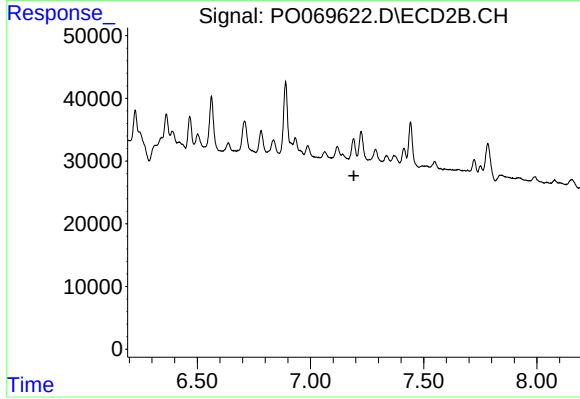

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T.: 7.191 min
Response: 0
Conc: N.D.

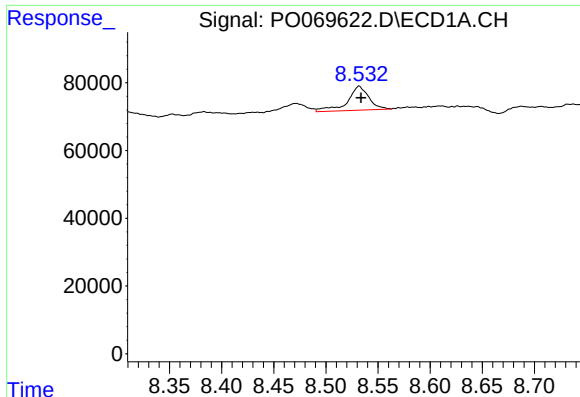

#35 AR-1260-5


R.T.: 8.532 min
Delta R.T.: -0.002 min
Response: 100379
Conc: 14.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
ST-JOES-AVE-2

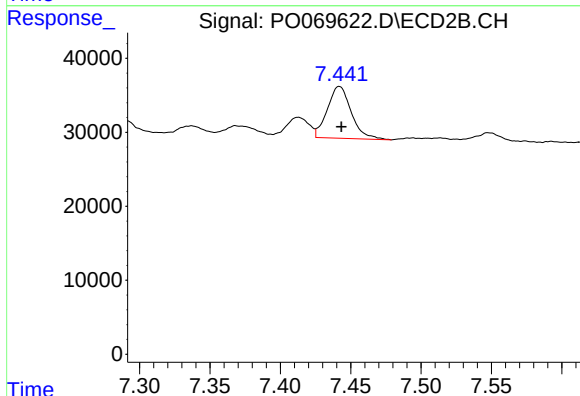


#35 AR-1260-5

R.T.: 7.442 min
Delta R.T.: -0.001 min
Response: 82812
Conc: 12.92 ng/ml

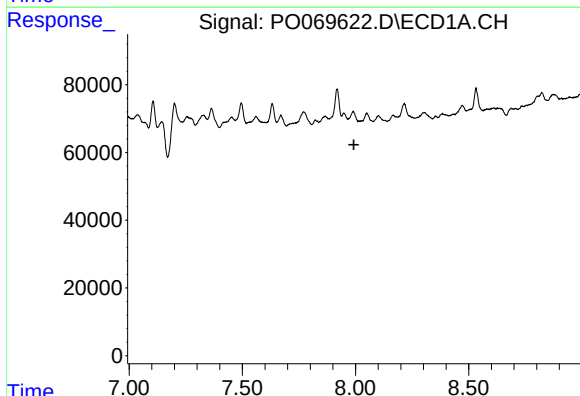


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.993 min
Response: 0
Conc: N.D.

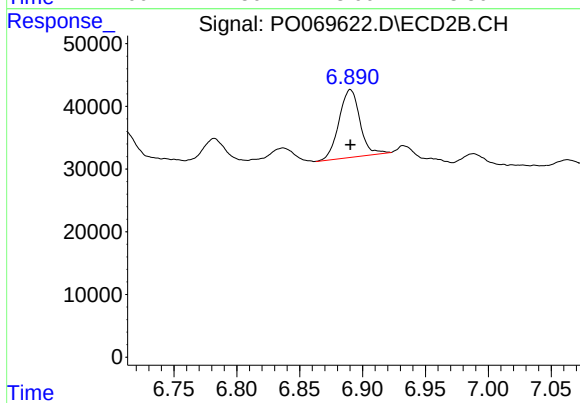

#36 AR-1262-1


R.T.: 6.890 min
Delta R.T.: 0.000 min
Response: 125046
Conc: 64.76 ng/ml

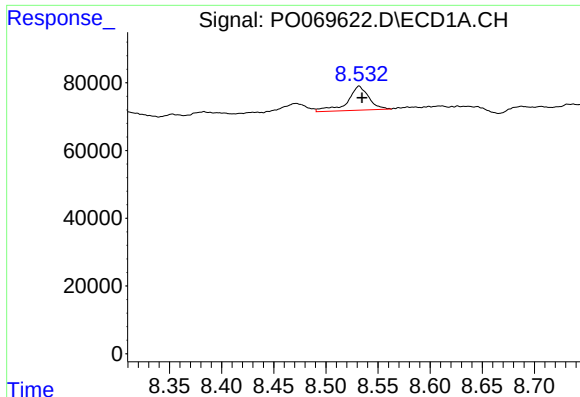

#37 AR-1262-2


R.T.: 8.532 min
Delta R.T.: -0.003 min
Response: 100379
Conc: 13.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
ST-JOES-AVE-2

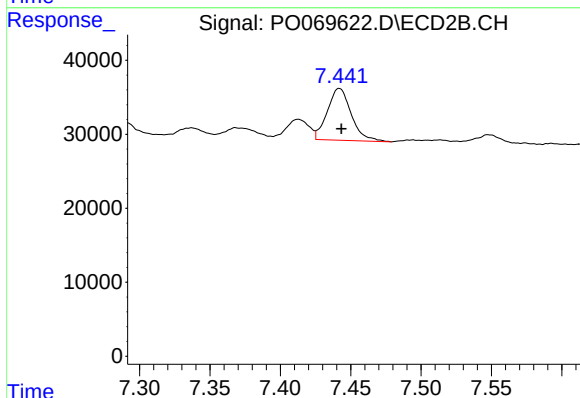


#37 AR-1262-2

R.T.: 7.442 min
Delta R.T.: -0.001 min
Response: 82812
Conc: 12.68 ng/ml

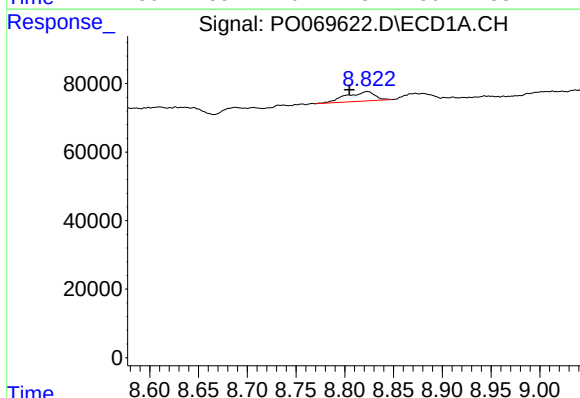


#38 AR-1262-3

R.T.: 8.823 min
Delta R.T.: 0.018 min
Response: 56766
Conc: 11.86 ng/ml

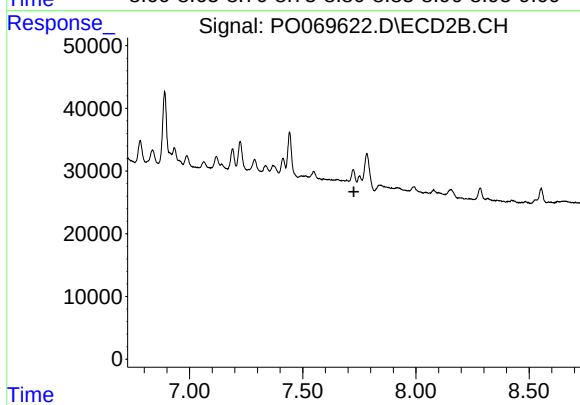

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

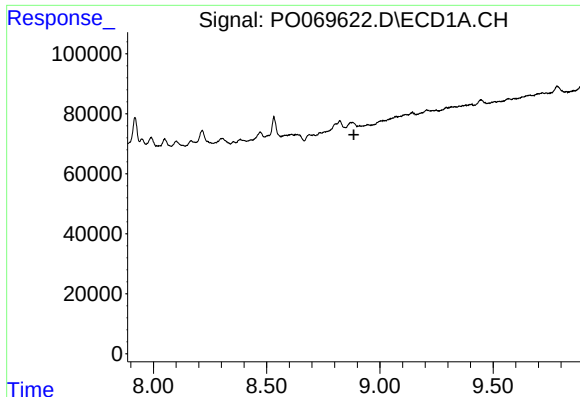

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.885 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
ST-JOES-AVE-2

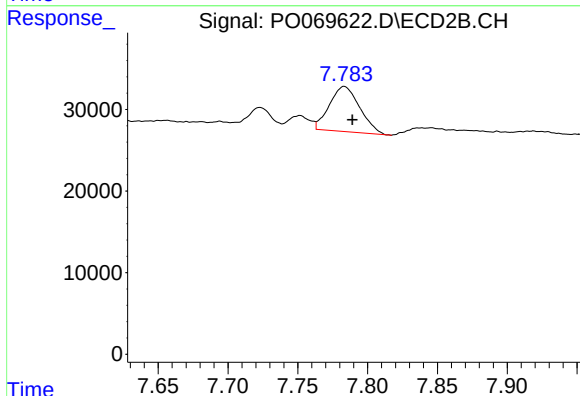


#39 AR-1262-4

R.T.: 7.783 min
Delta R.T.: -0.006 min
Response: 83230
Conc: 16.72 ng/ml

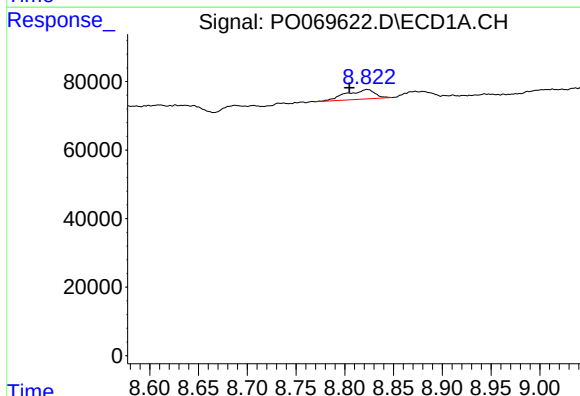


#41 AR-1268-1

R.T.: 8.823 min
Delta R.T.: 0.018 min
Response: 56766
Conc: 6.19 ng/ml

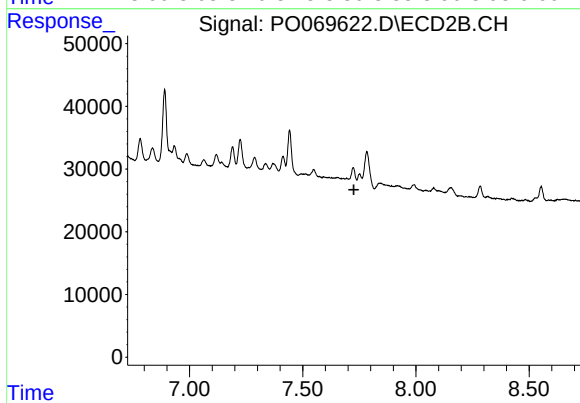

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 7.726 min
Response: 0
Conc: N.D.

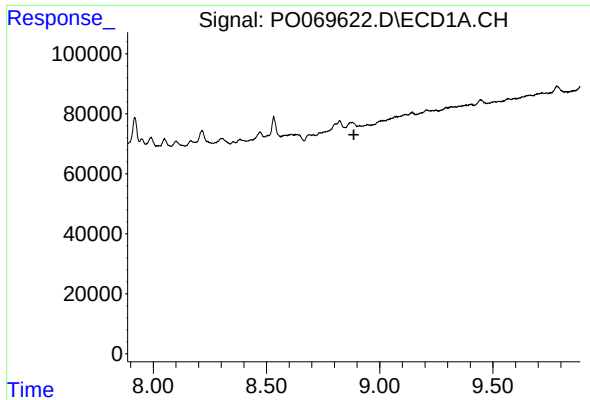

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.886 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
ST-JOES-AVE-2

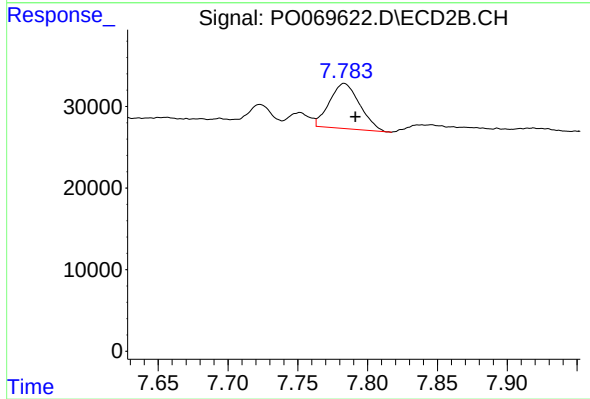

#42 AR-1268-2

R.T.: 7.783 min
Delta R.T.: -0.008 min
Response: 83230
Conc: 11.65 ng/ml