

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071420\
 Data File : P0069622.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jul 2020 15:21
 Operator : DD\AJ
 Sample : L3282-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ST-JOES-AVE-2

Manual Integrations
 APPROVED

Ankita
 7/15/2020 11:11:31 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 17:49:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 08 16:12:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.391	3.564	1107151	1178592	29.654	29.616
2) SA Decachlor...	10.051	8.771	1262939	1124004	20.991	19.805
Target Compounds						
31) L7 AR-1260-1	7.363	6.364	93228	45982	35.456m	17.434m#
32) L7 AR-1260-2	7.632	6.563	69296	101991	19.534	31.160 #
33) L7 AR-1260-3	7.991	6.709	55777	68275	19.293m	22.425
34) L7 AR-1260-4	8.215	7.190	60817	44513	20.533	16.445m
35) L7 AR-1260-5	8.532	7.442	100379	82812	14.835	12.922

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071420\
Data File : P0069622.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jul 2020 15:21
Operator : DD\AJ
Sample : L3282-02
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
ST-JOES-AVE-2


Manual Integrations
APPROVED

Ankita
7/15/2020 11:11:31 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 17:49:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 08 16:12:41 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

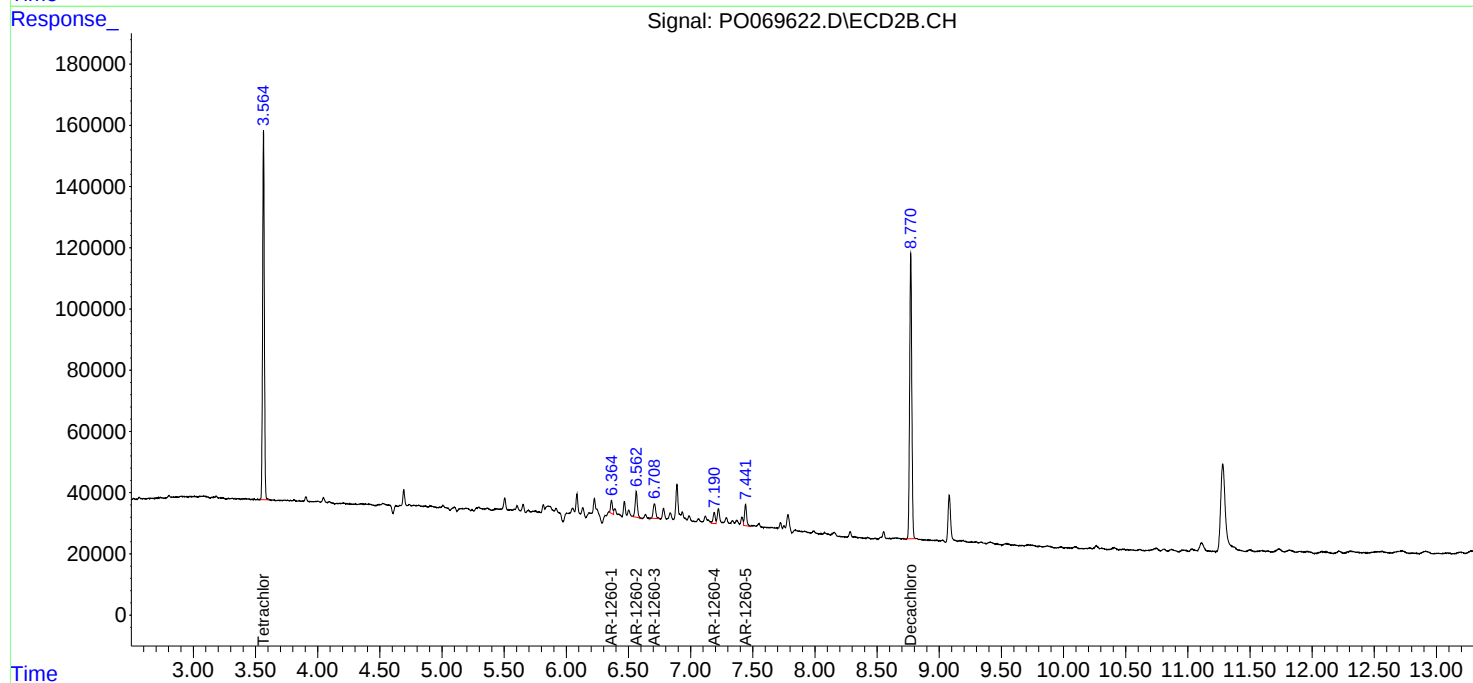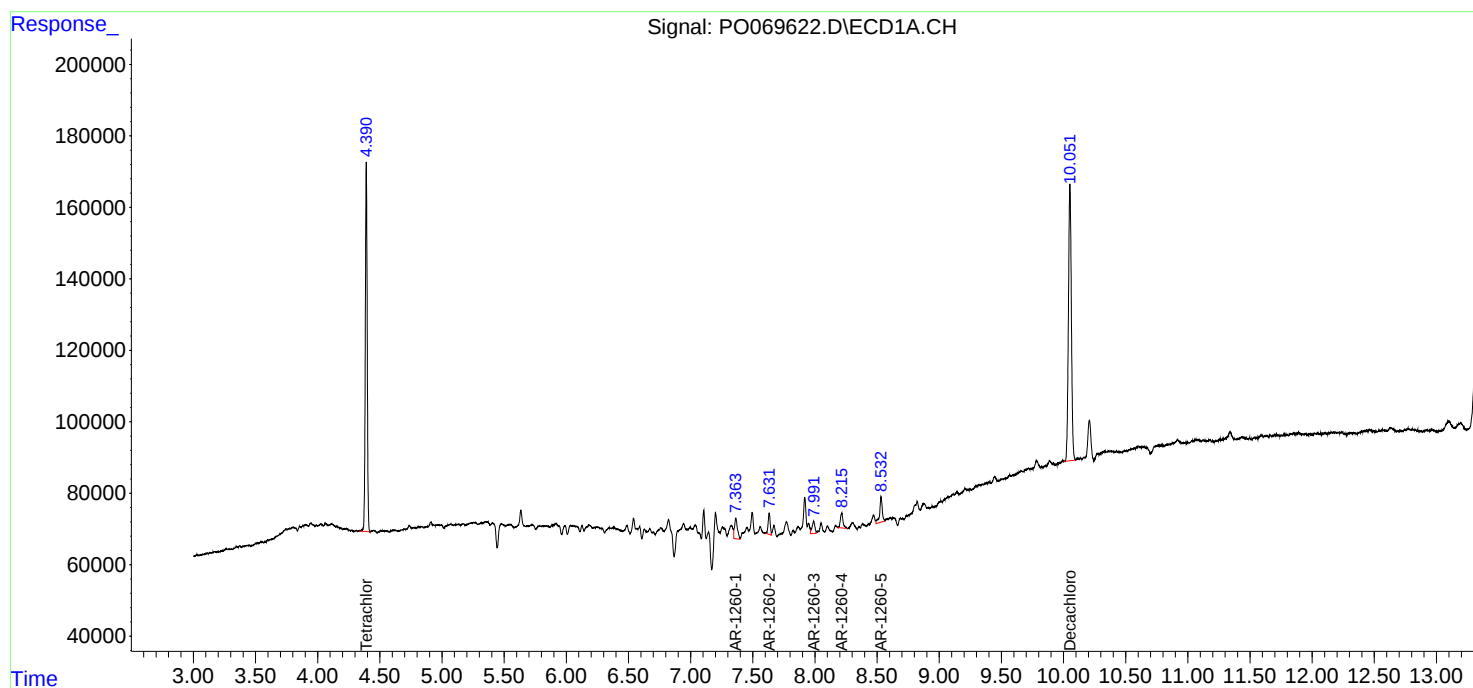

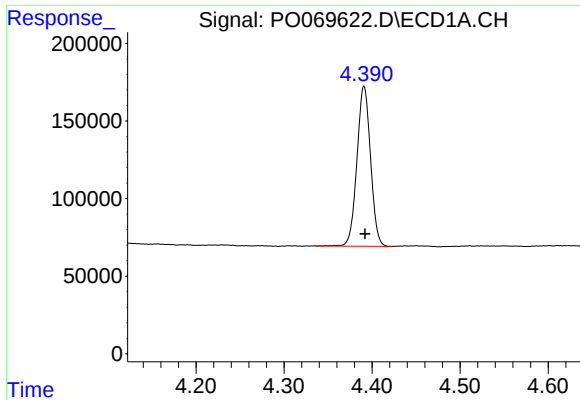


#1 Tetrachloro-m-xylene

R.T.: 4.391 min
Delta R.T.: -0.001 min
Response: 1107151
Conc: 29.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
ST-JOES-AVE-2


Manual Integrations
APPROVED

Ankita
7/15/2020 11:11:31 AM

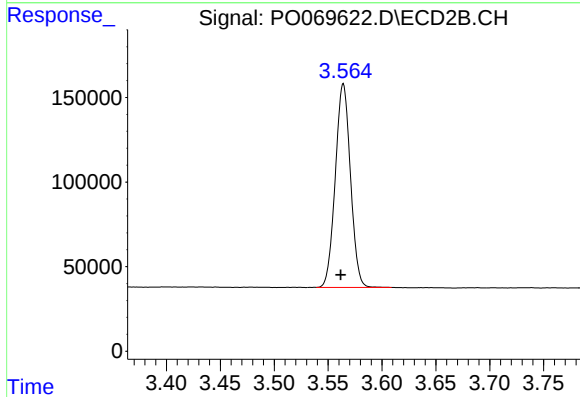


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: 0.002 min
Response: 1178592
Conc: 29.62 ng/ml

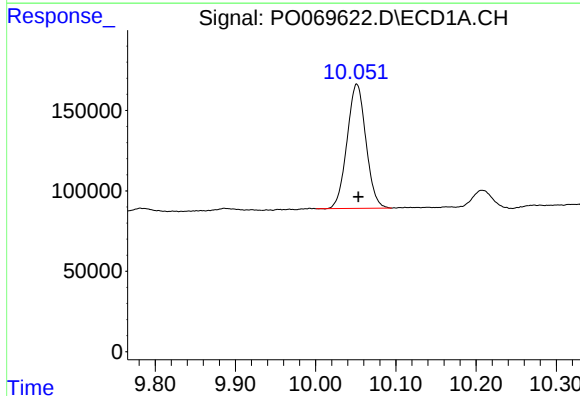


#2 Decachlorobiphenyl

R.T.: 10.051 min
Delta R.T.: -0.002 min
Response: 1262939
Conc: 20.99 ng/ml

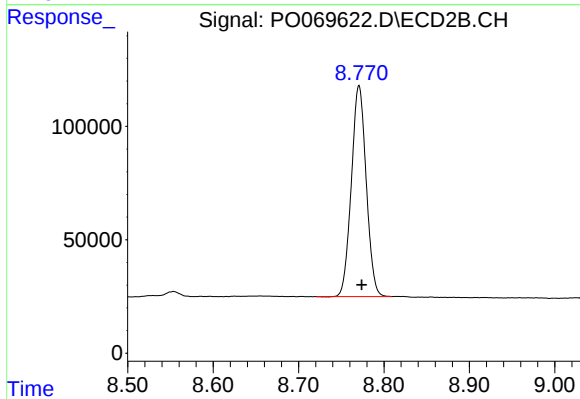

#2 Decachlorobiphenyl

R.T.: 8.771 min
Delta R.T.: -0.003 min
Response: 1124004
Conc: 19.80 ng/ml

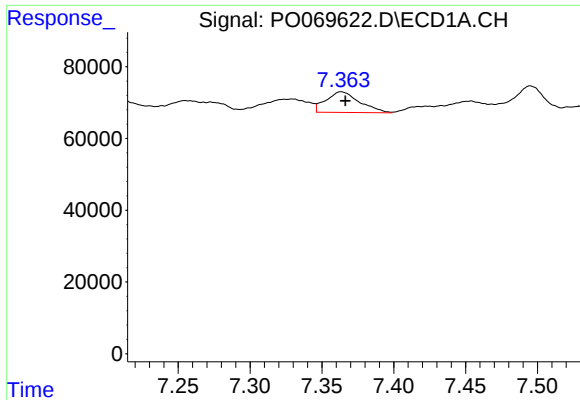


#31 AR-1260-1

R.T.: 7.363 min
Delta R.T.: -0.003 min
Response: 93228
Conc: 35.46 ng/ml m

Instrument :
ECD_O
ClientSampleId :
ST-JOES-AVE-2


Manual Integrations
APPROVED

Ankita
7/15/2020 11:11:31 AM

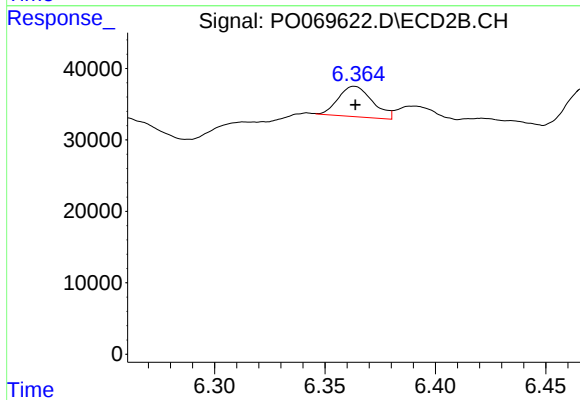


#31 AR-1260-1

R.T.: 6.364 min
Delta R.T.: 0.000 min
Response: 45982
Conc: 17.43 ng/ml m

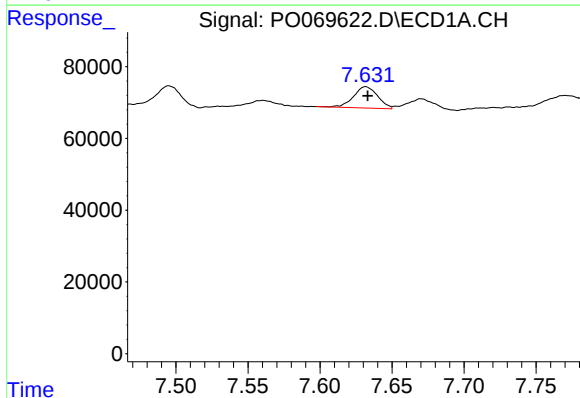


#32 AR-1260-2

R.T.: 7.632 min
Delta R.T.: -0.001 min
Response: 69296
Conc: 19.53 ng/ml

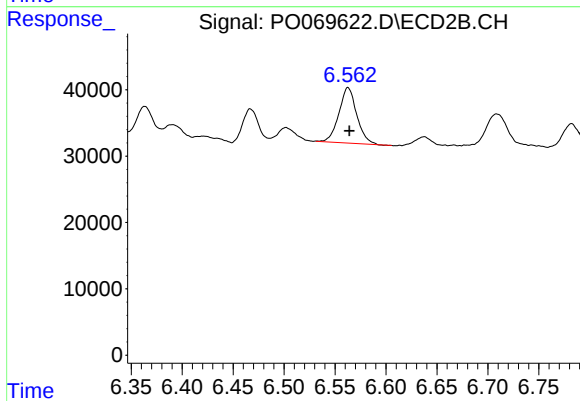

#32 AR-1260-2

R.T.: 6.563 min
Delta R.T.: -0.001 min
Response: 101991
Conc: 31.16 ng/ml

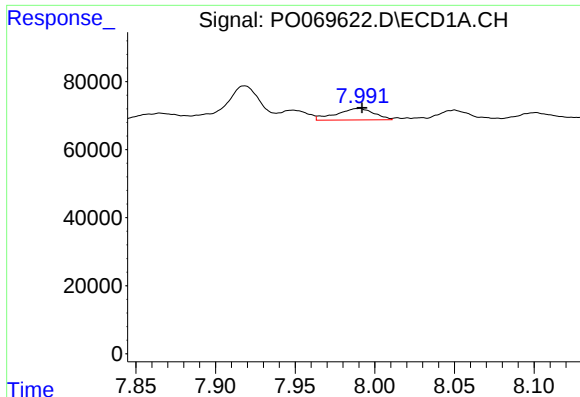


#33 AR-1260-3

R.T.: 7.991 min
Delta R.T.: -0.002 min
Response: 55777
Conc: 19.29 ng/ml m

Instrument :
ECD_O
ClientSampleId :
ST-JOES-AVE-2


Manual Integrations
APPROVED

Ankita
7/15/2020 11:11:31 AM

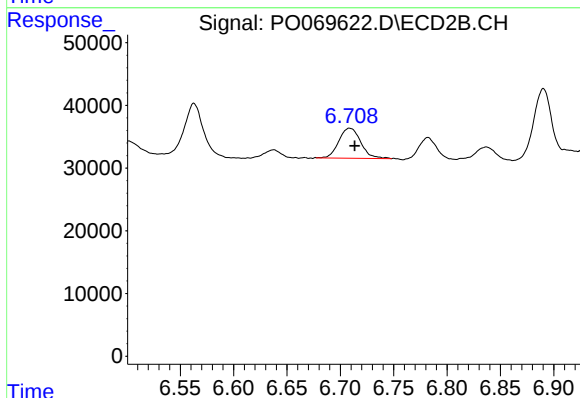


#33 AR-1260-3

R.T.: 6.709 min
Delta R.T.: -0.005 min
Response: 68275
Conc: 22.42 ng/ml

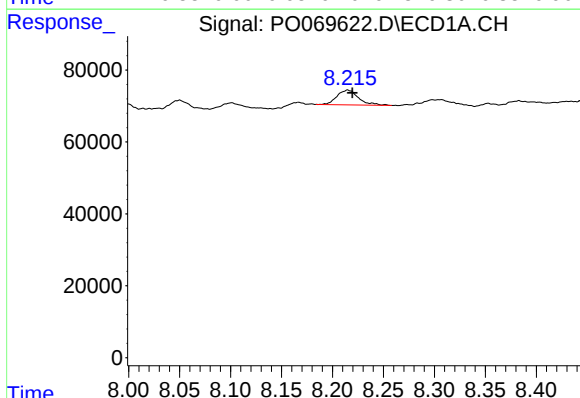


#34 AR-1260-4

R.T.: 8.215 min
Delta R.T.: -0.004 min
Response: 60817
Conc: 20.53 ng/ml

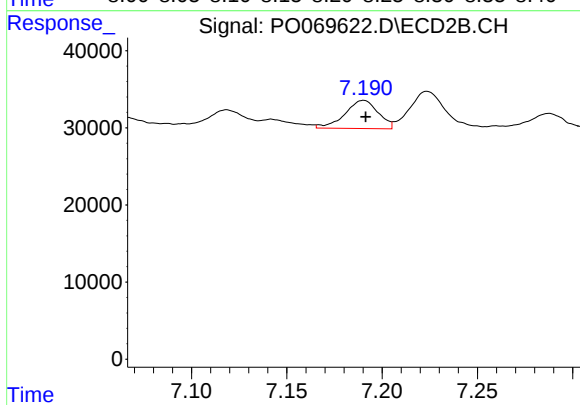

#34 AR-1260-4

R.T.: 7.190 min
Delta R.T.: -0.001 min
Response: 44513
Conc: 16.45 ng/ml m

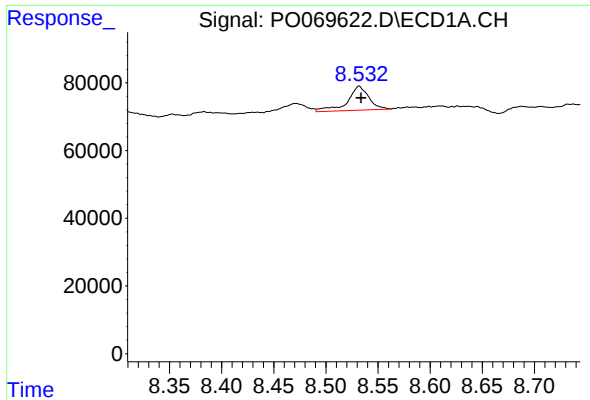


#35 AR-1260-5

R.T.: 8.532 min
Delta R.T.: -0.002 min
Response: 100379
Conc: 14.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
ST-JOES-AVE-2

Manual Integrations
APPROVED

Ankita
7/15/2020 11:11:31 AM

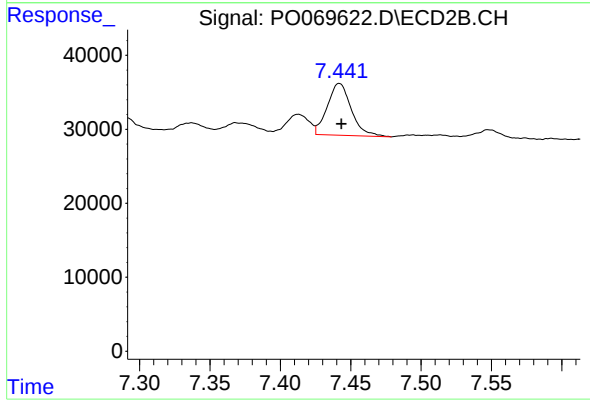

#35 AR-1260-5

R.T.: 7.442 min
Delta R.T.: -0.001 min
Response: 82812
Conc: 12.92 ng/ml