

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071420\
 Data File : P0069639.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jul 2020 22:44
 Operator : DD\AJ
 Sample : L3294-08 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S3-04-S

Manual Integrations
 APPROVED

Ankita
 7/15/2020 11:11:39 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 05:52:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 08 16:12:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.391	3.564	209751	237128	5.618	5.959
2)	SA Decachlor...	10.050	8.770	298714	313684	4.965m	5.527
Target Compounds							
26)	L6 AR-1254-1	6.593	5.653	121109	137178	60.841	52.698
27)	L6 AR-1254-2	6.823	5.815	415470	179841	129.420	77.901 #
28)	L6 AR-1254-3	7.200	6.228	578055	356650	164.590	94.967 #
29)	L6 AR-1254-4	7.494	6.467	268835	216158	89.825m	85.535
30)	L6 AR-1254-5	7.918	6.892	693214	1146925	230.396m	319.571 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071420\
Data File : PO069639.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jul 2020 22:44
Operator : DD\AJ
Sample : L3294-08 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S3-04-S


Manual Integrations
APPROVED

Ankita
7/15/2020 11:11:39 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 05:52:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO070820.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 08 16:12:41 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

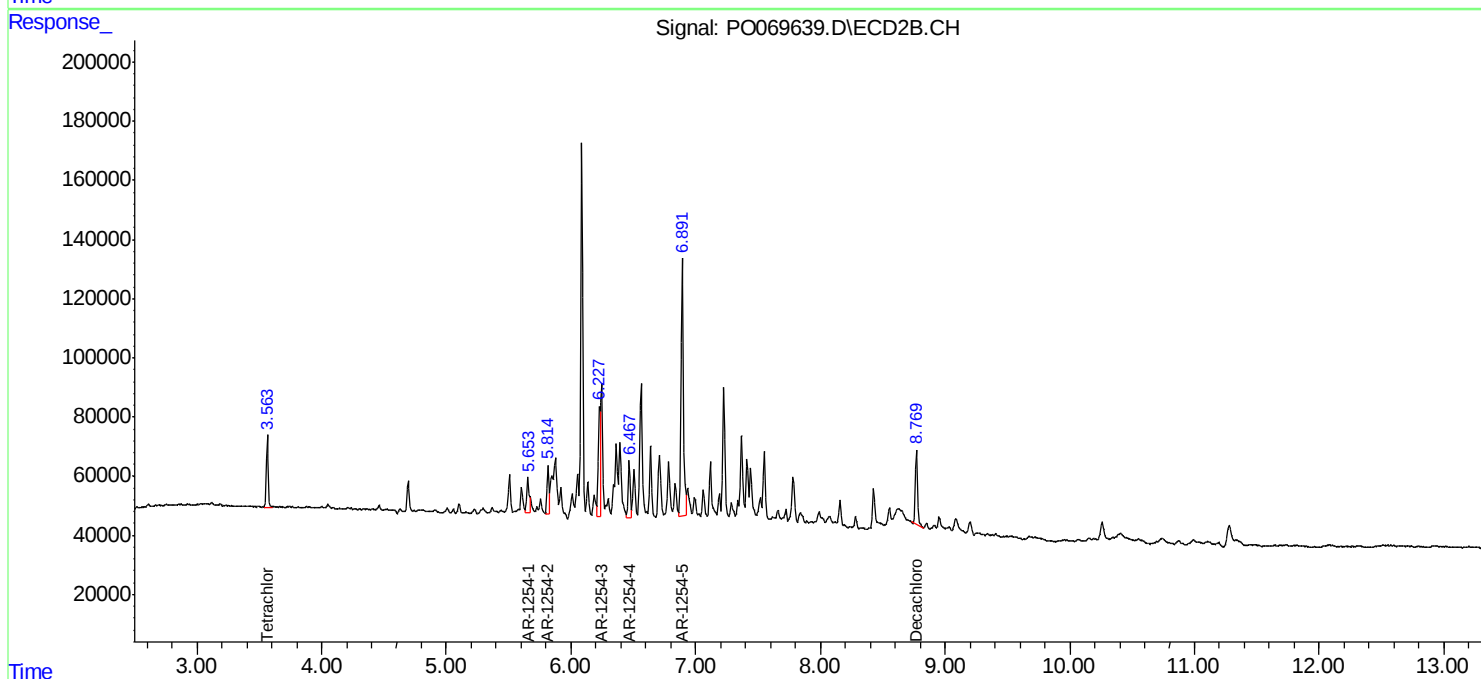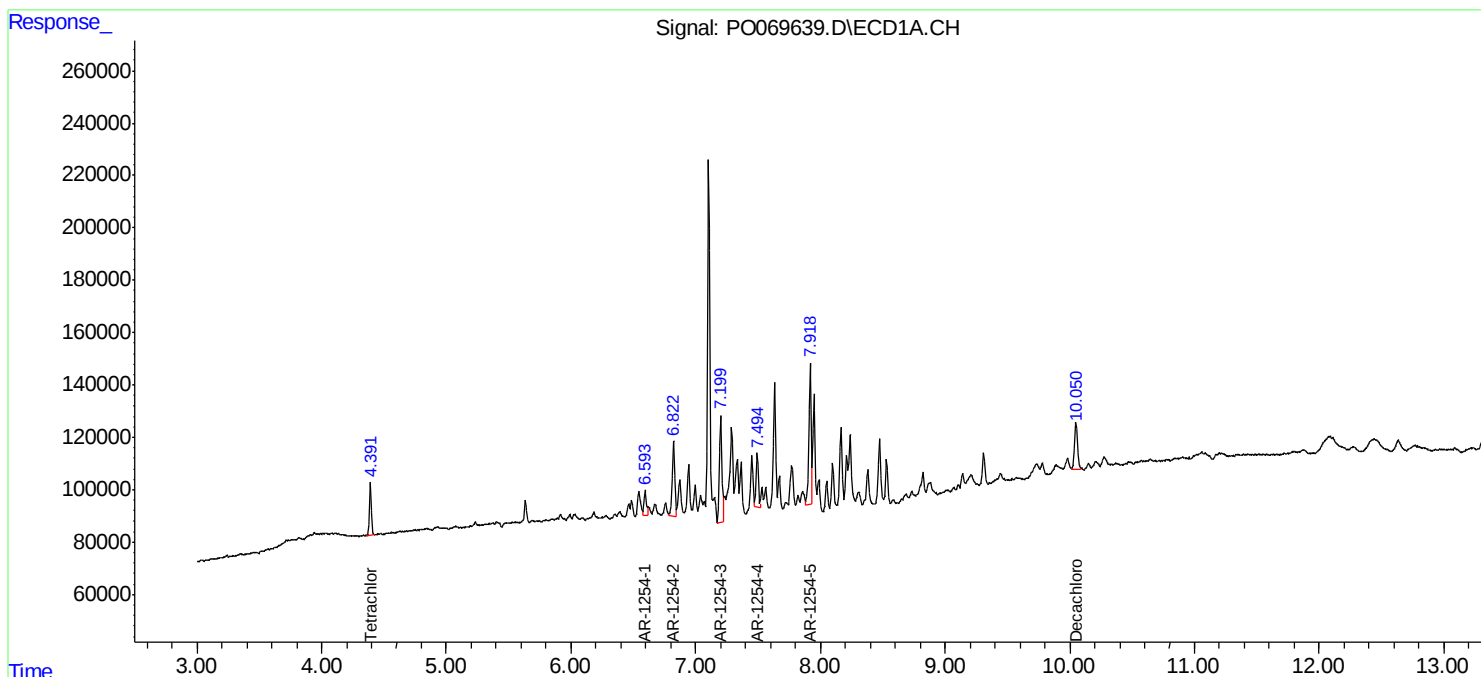

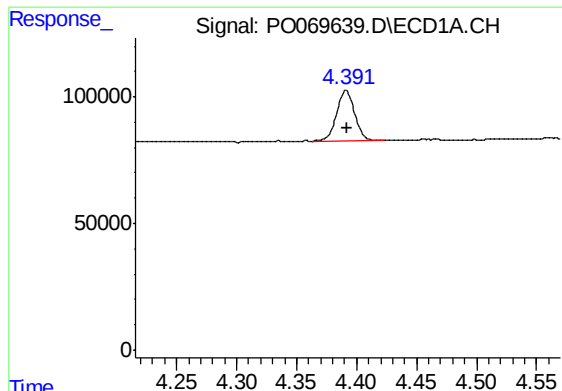


#1 Tetrachloro-m-xylene

R.T.: 4.391 min
Delta R.T.: 0.000 min
Response: 209751
Conc: 5.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
S3-04-S


Manual Integrations
APPROVED

Ankita
7/15/2020 11:11:39 AM

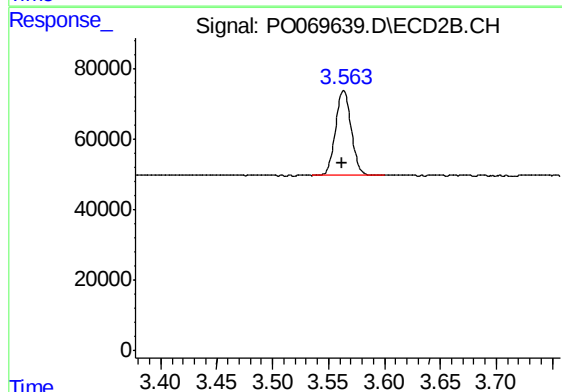


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: 0.002 min
Response: 237128
Conc: 5.96 ng/ml

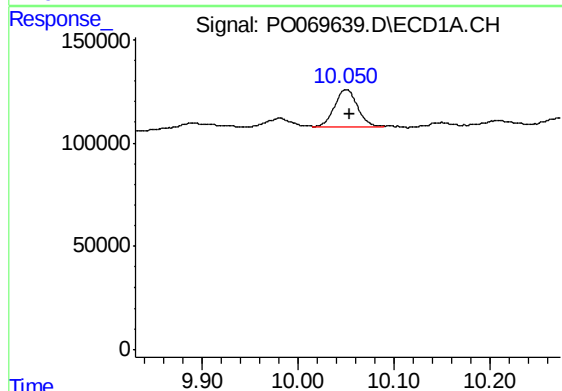


#2 Decachlorobiphenyl

R.T.: 10.050 min
Delta R.T.: -0.004 min
Response: 298714
Conc: 4.96 ng/ml m

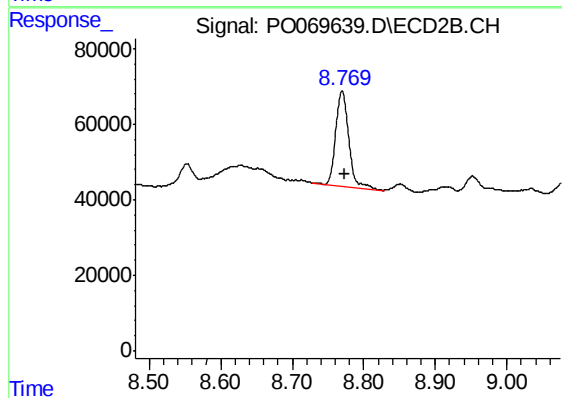

#2 Decachlorobiphenyl

R.T.: 8.770 min
Delta R.T.: -0.004 min
Response: 313684
Conc: 5.53 ng/ml

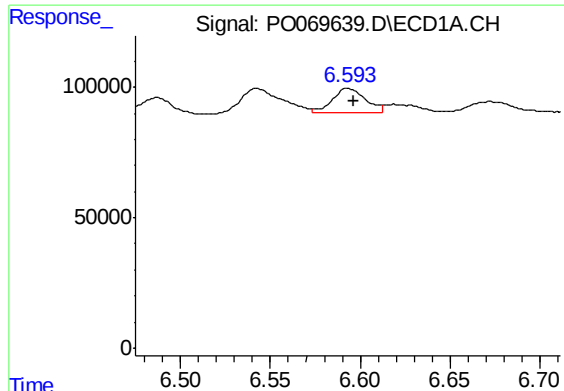


#26 AR-1254-1

R.T.: 6.593 min
Delta R.T.: -0.003 min
Response: 121109
Conc: 60.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
S3-04-S


Manual Integrations
APPROVED

Ankita
7/15/2020 11:11:39 AM

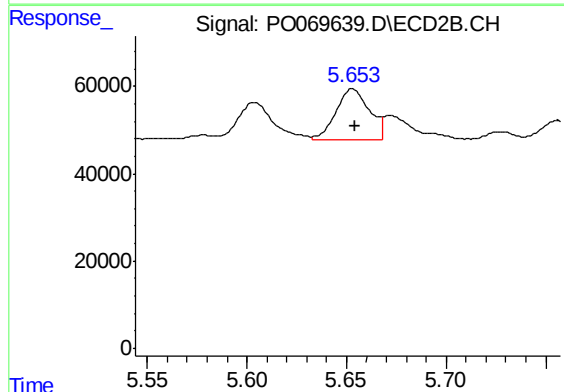


#26 AR-1254-1

R.T.: 5.653 min
Delta R.T.: 0.000 min
Response: 137178
Conc: 52.70 ng/ml

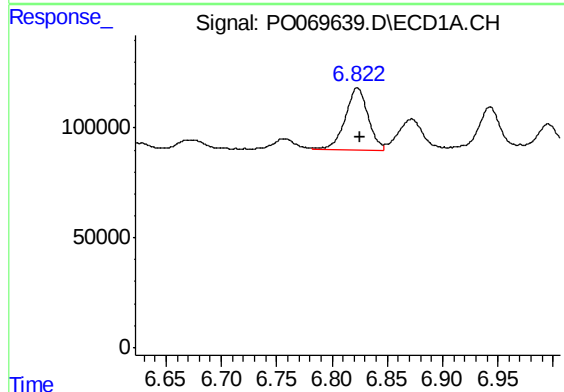


#27 AR-1254-2

R.T.: 6.823 min
Delta R.T.: -0.002 min
Response: 415470
Conc: 129.42 ng/ml

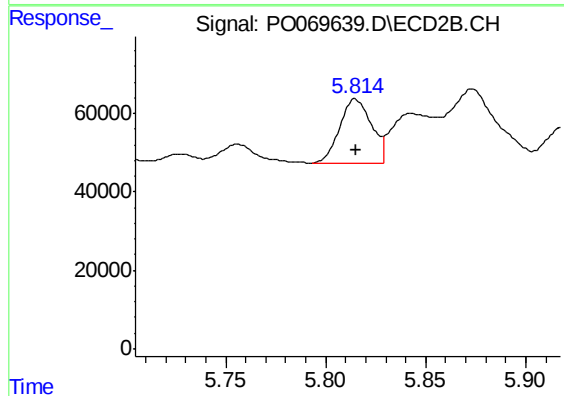

#27 AR-1254-2

R.T.: 5.815 min
Delta R.T.: 0.000 min
Response: 179841
Conc: 77.90 ng/ml

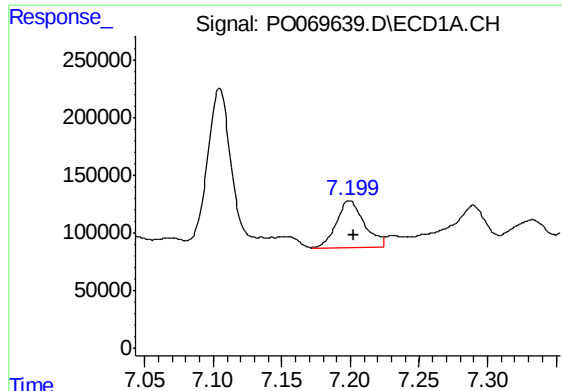


#28 AR-1254-3

R.T.: 7.200 min
Delta R.T.: -0.003 min
Response: 578055
Conc: 164.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
S3-04-S


Manual Integrations
APPROVED

Ankita
7/15/2020 11:11:39 AM

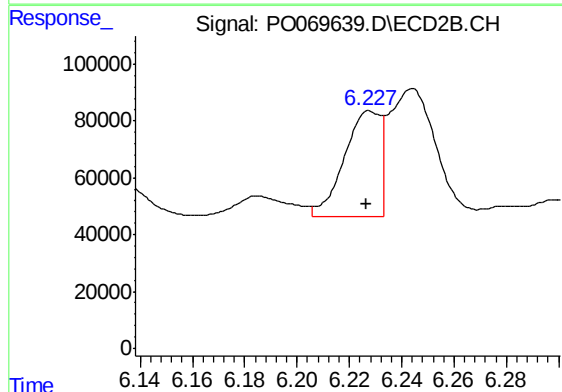


#28 AR-1254-3

R.T.: 6.228 min
Delta R.T.: 0.001 min
Response: 356650
Conc: 94.97 ng/ml

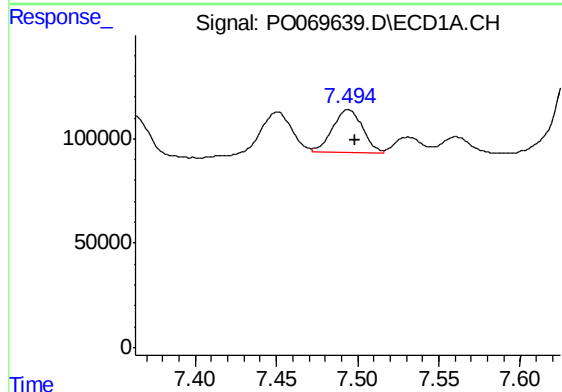


#29 AR-1254-4

R.T.: 7.494 min
Delta R.T.: -0.005 min
Response: 268835
Conc: 89.82 ng/ml m

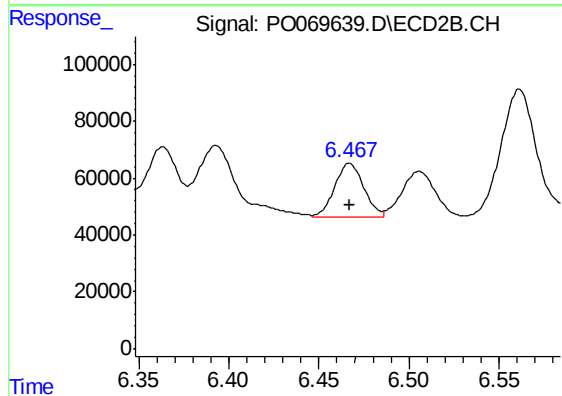

#29 AR-1254-4

R.T.: 6.467 min
Delta R.T.: 0.000 min
Response: 216158
Conc: 85.53 ng/ml

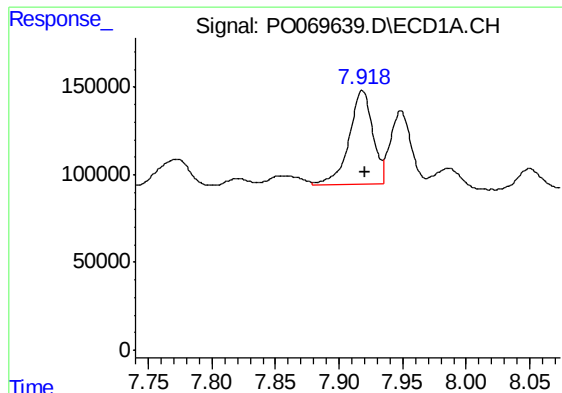


#30 AR-1254-5

R.T.: 7.918 min
Delta R.T.: -0.003 min
Response: 693214
Conc: 230.40 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S3-04-S

Manual Integrations
APPROVED

Ankita
7/15/2020 11:11:39 AM

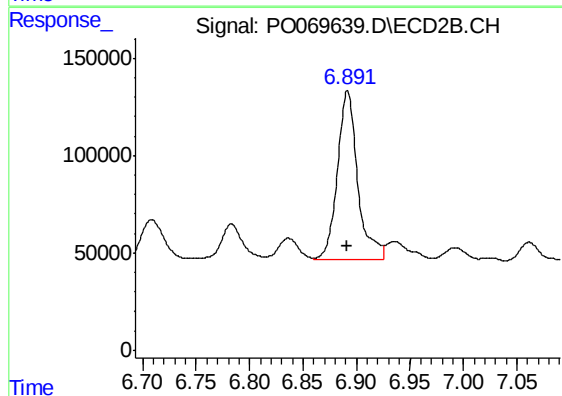

#30 AR-1254-5

R.T.: 6.892 min
Delta R.T.: 0.000 min
Response: 1146925
Conc: 319.57 ng/ml