

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071420\
 Data File : P0069642.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jul 2020 23:36
 Operator : DD\AJ
 Sample : L3294-11 5X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S3-06-B

Manual Integrations
 APPROVED

Ankita
 7/15/2020 11:11:45 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 05:54:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 08 16:12:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.391	3.564	183432	266283	4.913	6.691 #
2) SA Decachlor...	10.049	8.771	844203	1012081	14.031m	17.833m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071420\
Data File : P0069642.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jul 2020 23:36
Operator : DD\AJ
Sample : L3294-11 5X
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S3-06-B


Manual Integrations
APPROVED

Ankita
7/15/2020 11:11:45 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 05:54:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 08 16:12:41 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

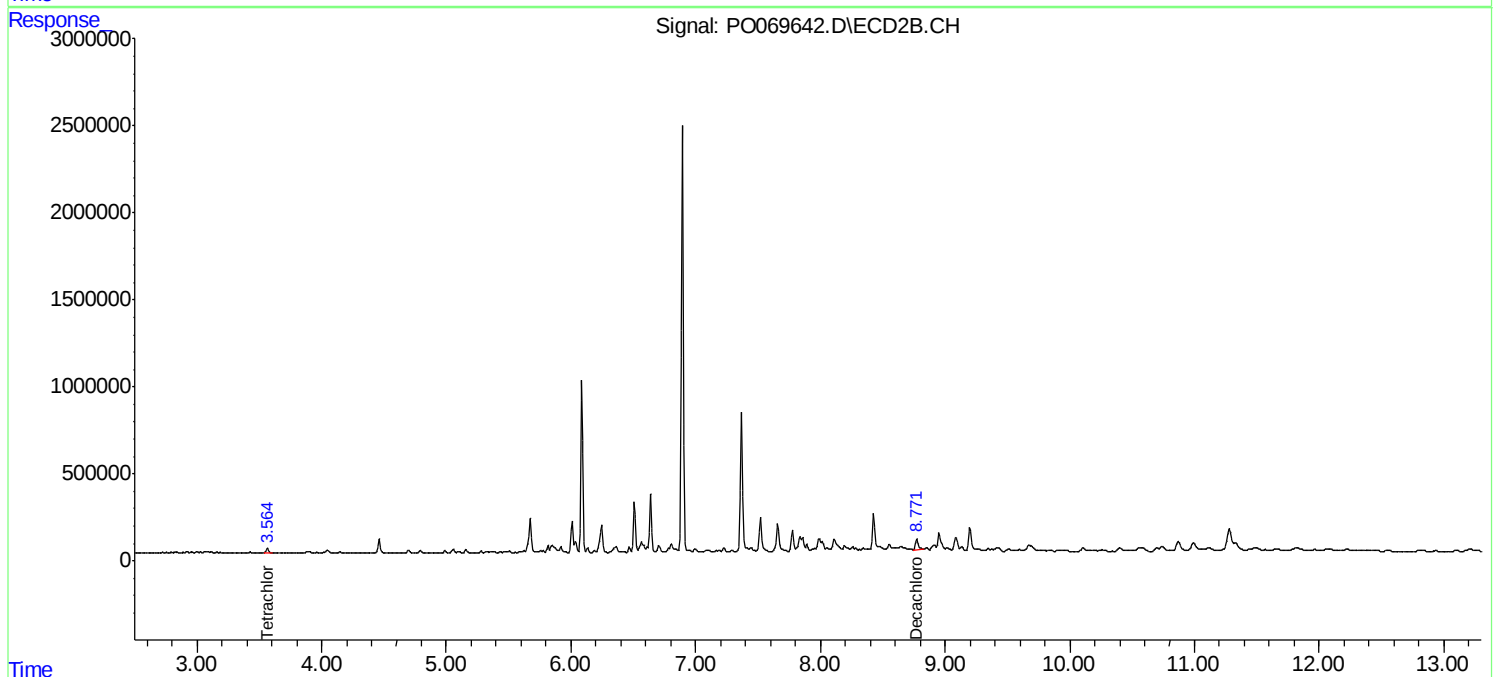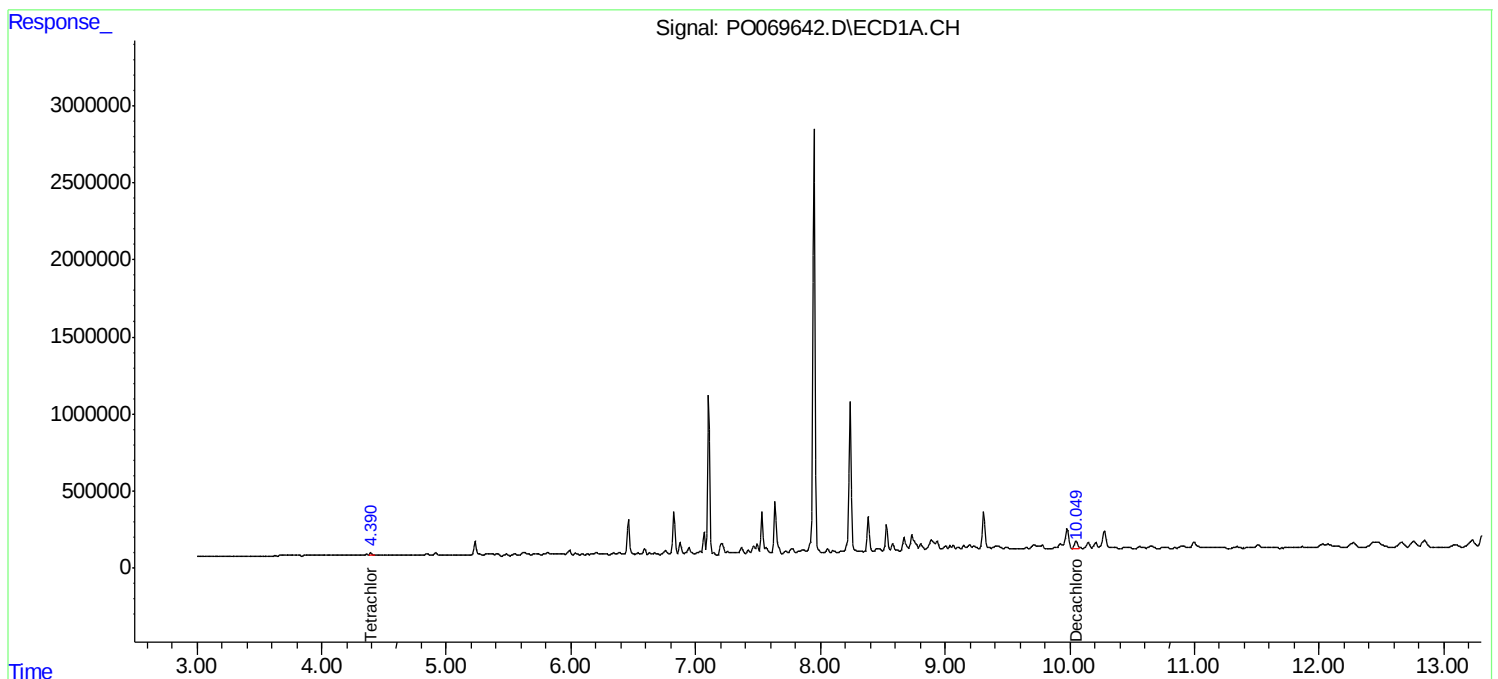

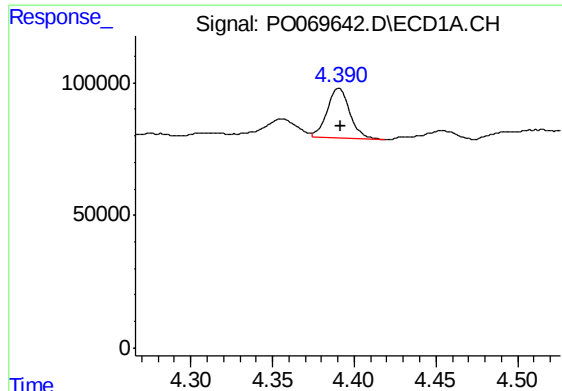


#1 Tetrachloro-m-xylene

R.T.: 4.391 min
Delta R.T.: -0.001 min
Response: 183432
Conc: 4.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
S3-06-B


Manual Integrations
APPROVED

Ankita
7/15/2020 11:11:45 AM

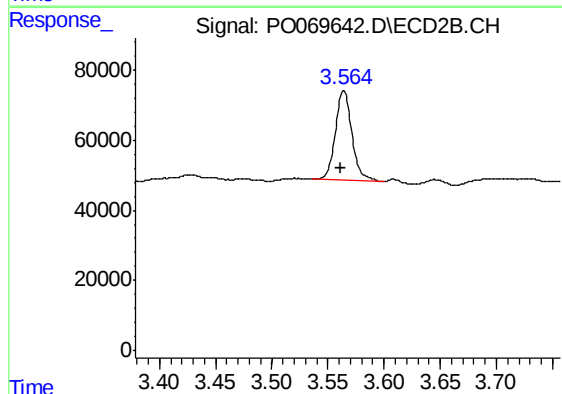


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: 0.002 min
Response: 266283
Conc: 6.69 ng/ml

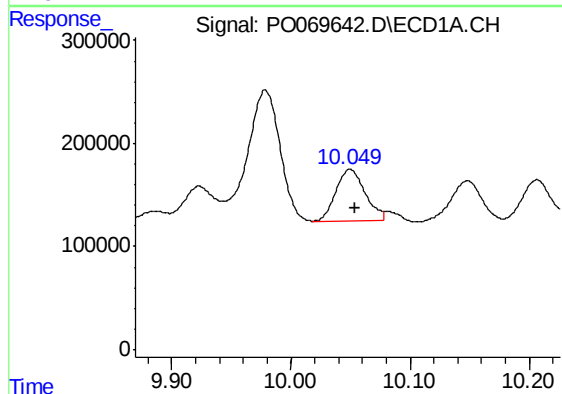

#2 Decachlorobiphenyl

R.T.: 10.049 min
Delta R.T.: -0.004 min
Response: 844203
Conc: 14.03 ng/ml m

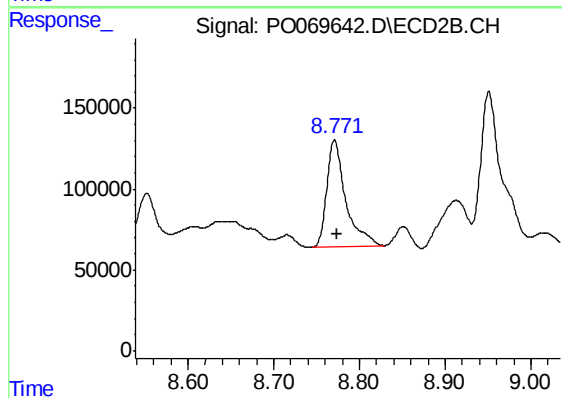

#2 Decachlorobiphenyl

R.T.: 8.771 min
Delta R.T.: -0.004 min
Response: 1012081
Conc: 17.83 ng/ml m