

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071420\
 Data File : P0069658.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jul 2020 4:29
 Operator : DD\AJ
 Sample : L3294-24
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S1-02-B-01

Manual Integrations
 APPROVED

Ankita
 7/15/2020 11:11:58 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 15 06:02:42 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 08 16:12:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.392	3.565	862763	908046	23.108	22.817
2)	SA Decachlor...	10.051	8.771	971530	936853	16.147	16.507

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071420\
Data File : PO069658.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jul 2020 4:29
Operator : DD\AJ
Sample : L3294-24
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S1-02-B-01


Manual Integrations
APPROVED

Ankita
7/15/2020 11:11:58 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 06:02:42 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO070820.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 08 16:12:41 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

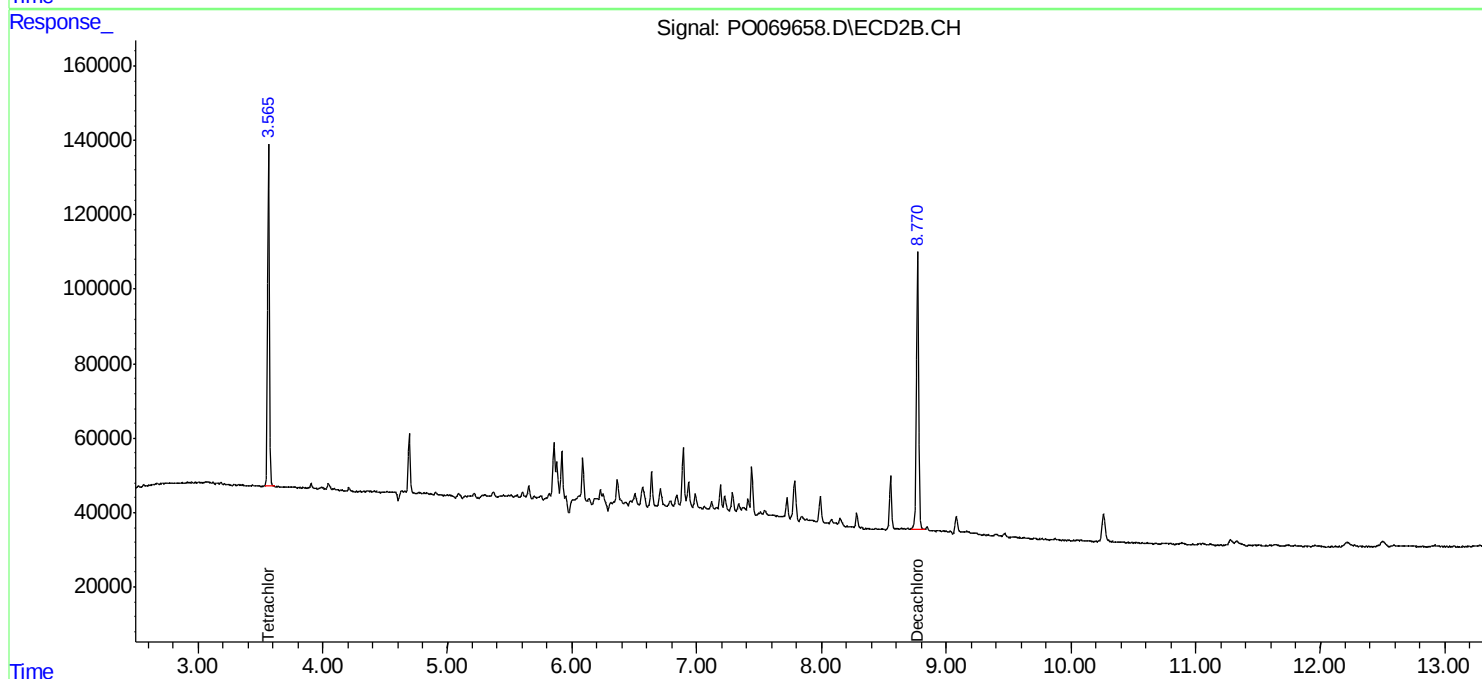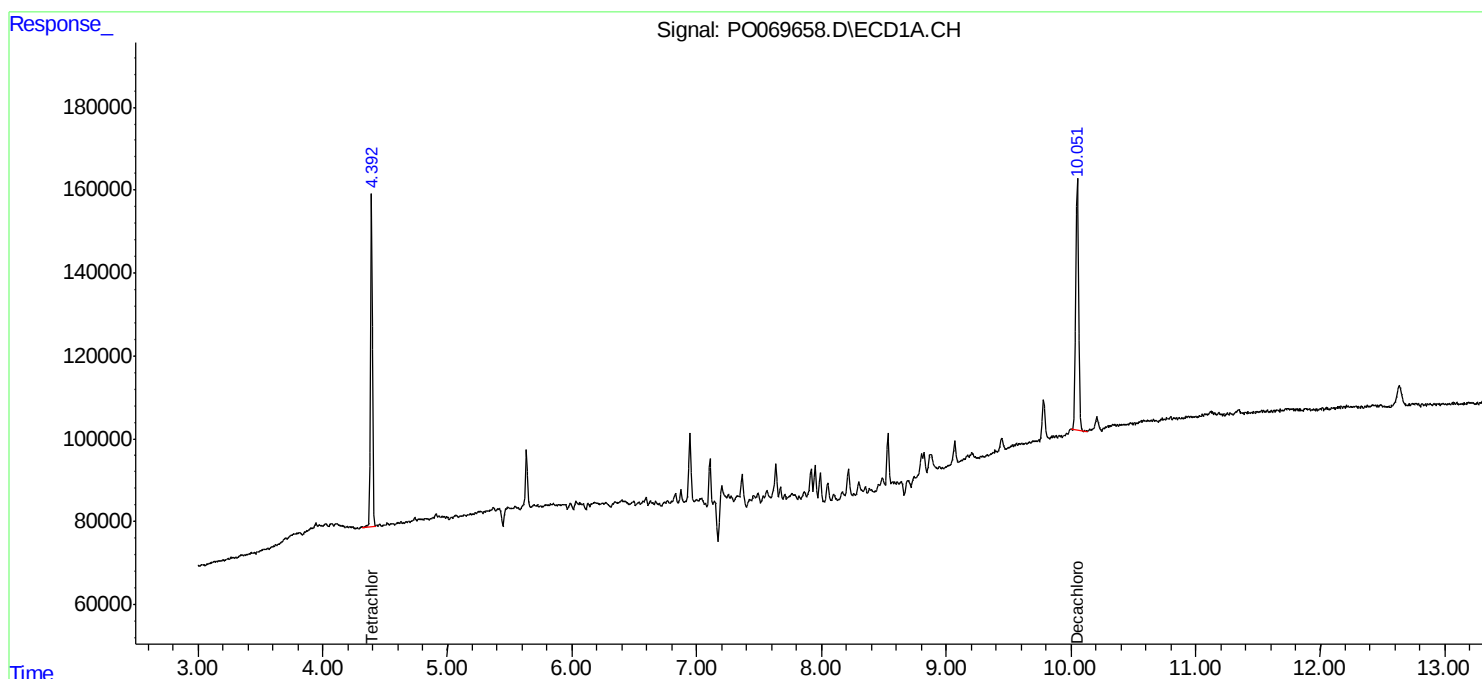

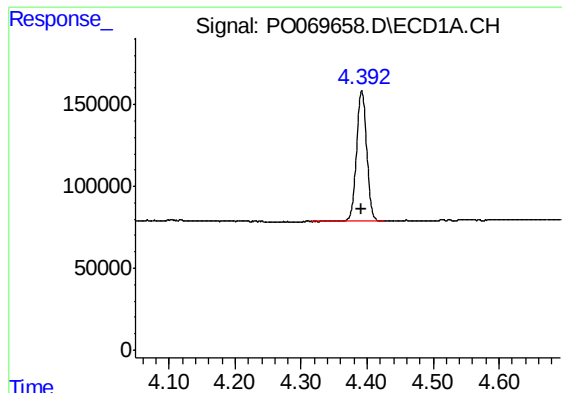


#1 Tetrachloro-m-xylene

R.T.: 4.392 min
Delta R.T.: 0.000 min
Response: 862763
Conc: 23.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
S1-02-B-01


Manual Integrations
APPROVED

Ankita
7/15/2020 11:11:58 AM

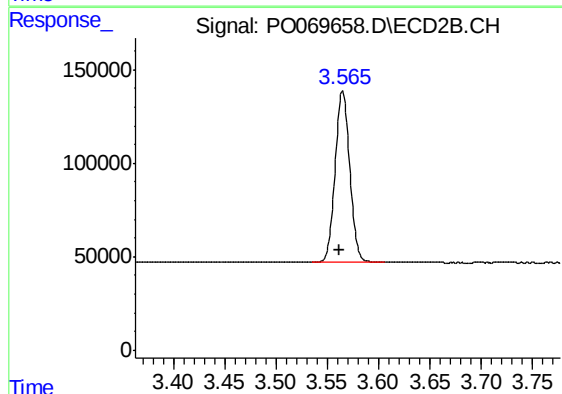


#1 Tetrachloro-m-xylene

R.T.: 3.565 min
Delta R.T.: 0.003 min
Response: 908046
Conc: 22.82 ng/ml

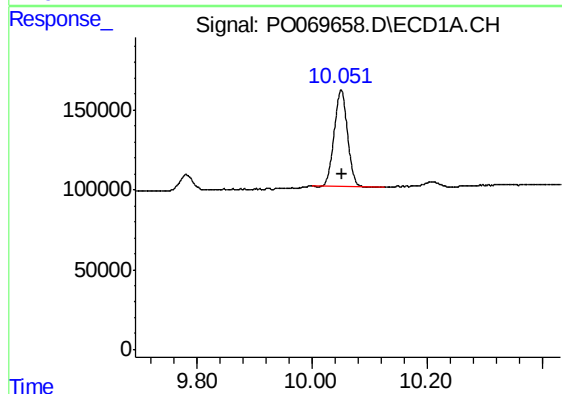

#2 Decachlorobiphenyl

R.T.: 10.051 min
Delta R.T.: -0.002 min
Response: 971530
Conc: 16.15 ng/ml

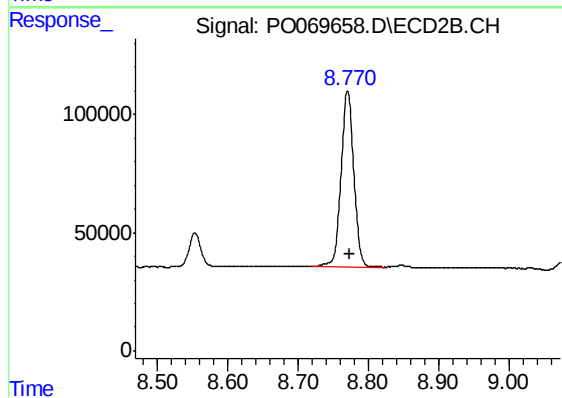

#2 Decachlorobiphenyl

R.T.: 8.771 min
Delta R.T.: -0.003 min
Response: 936853
Conc: 16.51 ng/ml