

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071423\
 Data File : P0096178.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jul 2023 16:36
 Operator : YP/AJ
 Sample : 03615-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 2880

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/17/2023
 Supervised By :Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 05:34:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 04 02:14:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.413	3.634	10654666	4221320	3.434m	3.131
2) SA Decachlor...	10.238	8.667	10495387	5607570	5.228	4.798

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071423\
Data File : PO096178.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jul 2023 16:36
Operator : YP/AJ
Sample : 03615-08
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
2880


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/17/2023
Supervised By :Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 05:34:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO070123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 04 02:14:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

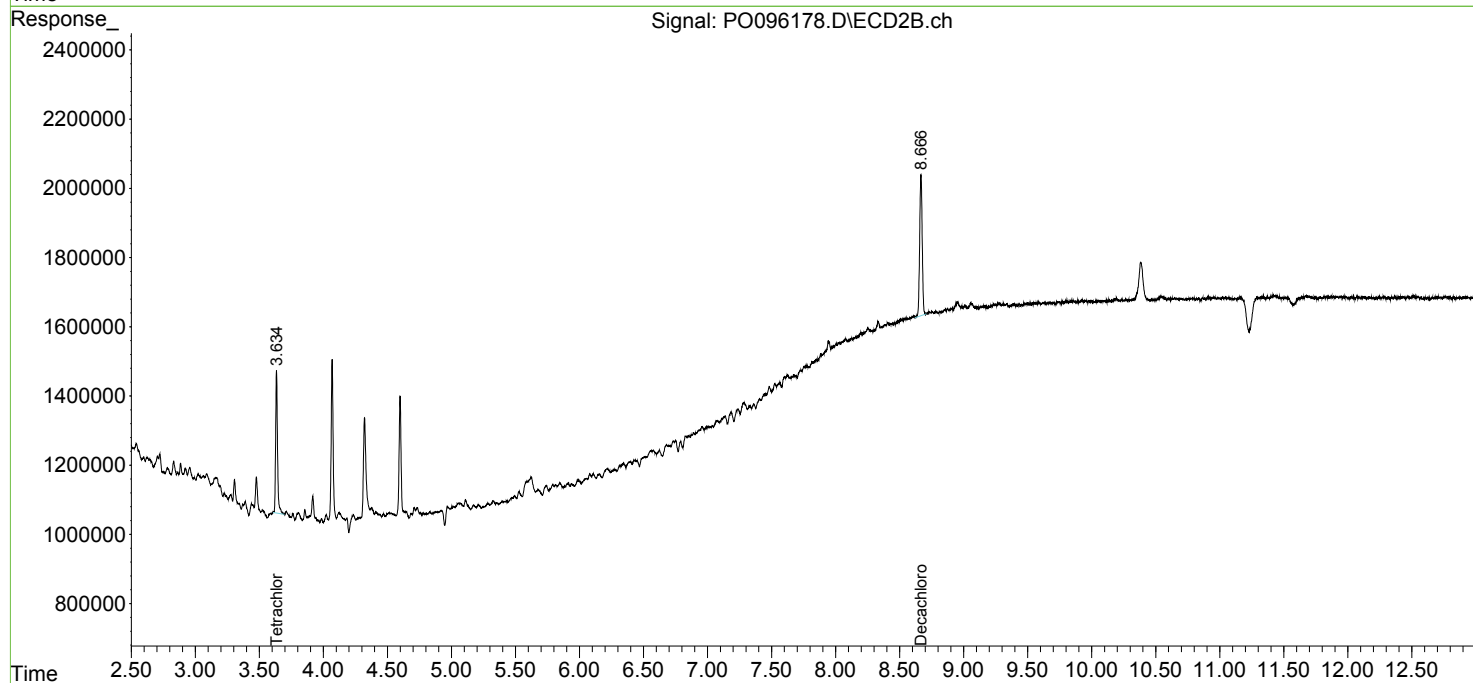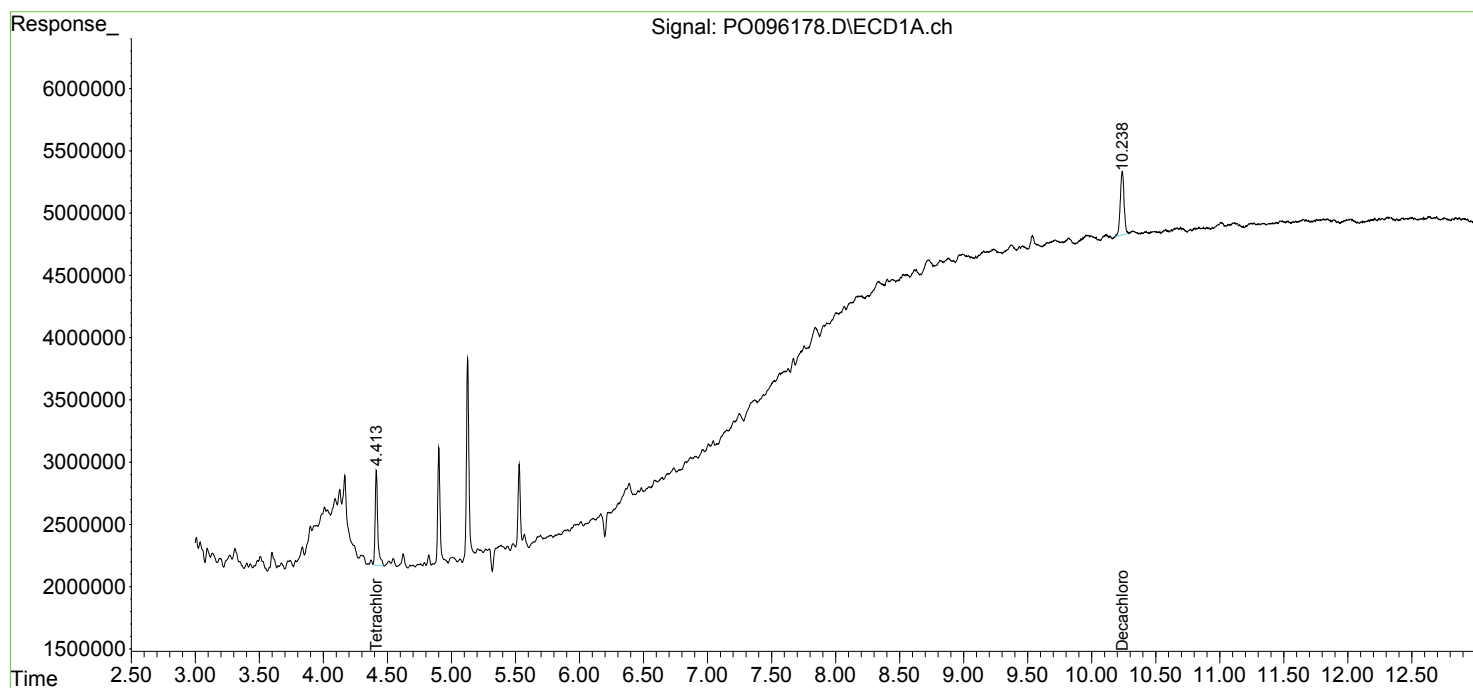

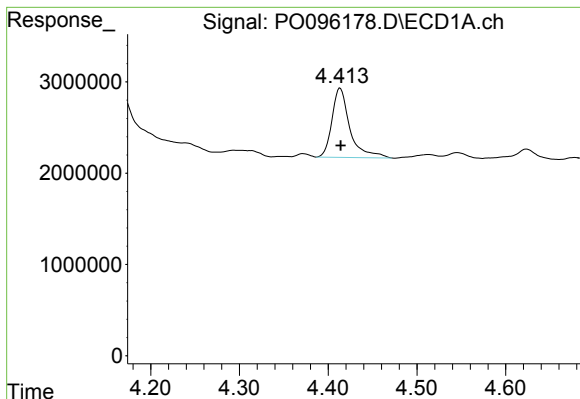


#1 Tetrachloro-m-xylene

R.T.: 4.413 min
Delta R.T.: -0.001 min
Response: 10654666
Conc: 3.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
2880


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/17/2023
Supervised By :Ankita Jodhani 07/17/2023

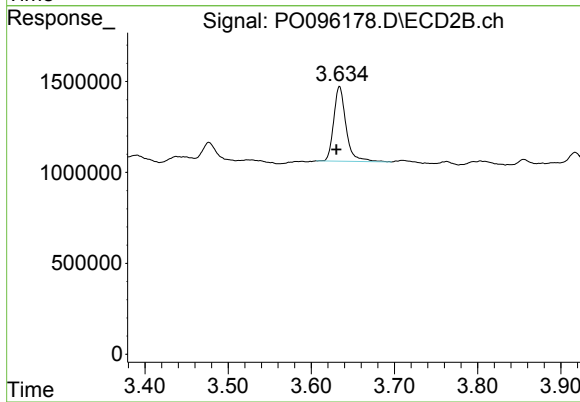


#1 Tetrachloro-m-xylene

R.T.: 3.634 min
Delta R.T.: 0.004 min
Response: 4221320
Conc: 3.13 ng/ml

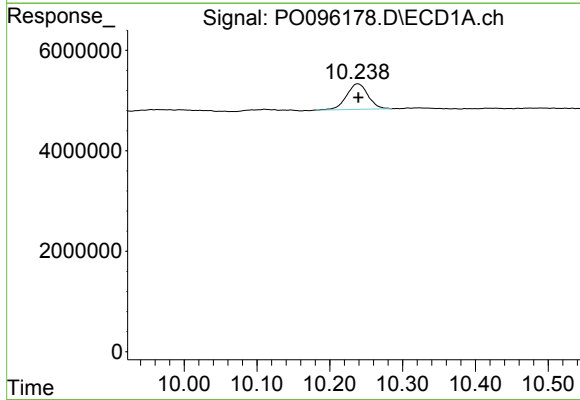

#2 Decachlorobiphenyl

R.T.: 10.238 min
Delta R.T.: 0.000 min
Response: 10495387
Conc: 5.23 ng/ml

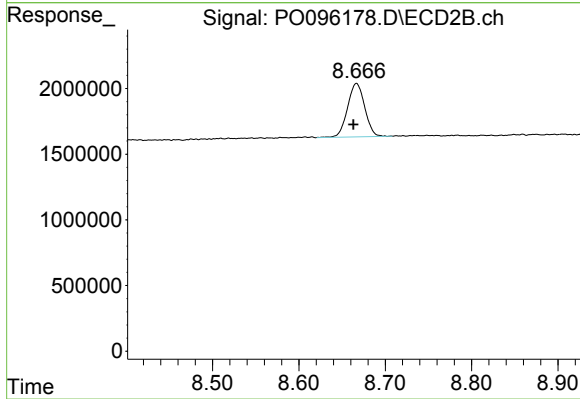

#2 Decachlorobiphenyl

R.T.: 8.667 min
Delta R.T.: 0.003 min
Response: 5607570
Conc: 4.80 ng/ml