

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071423\
 Data File : P0096183.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jul 2023 18:01
 Operator : YP/AJ
 Sample : 03620-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 713-D

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/17/2023
 Supervised By :Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 05:42:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 04 02:14:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.413	3.633	50897031	19139005	16.404m	14.195m
2) SA Decachlor...	10.237	8.665	30688007	15983107	15.287	13.675

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071423\
Data File : P0096183.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jul 2023 18:01
Operator : YP/AJ
Sample : 03620-04
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
713-D


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/17/2023
Supervised By :Ankita Jodhani 07/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 05:42:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 04 02:14:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

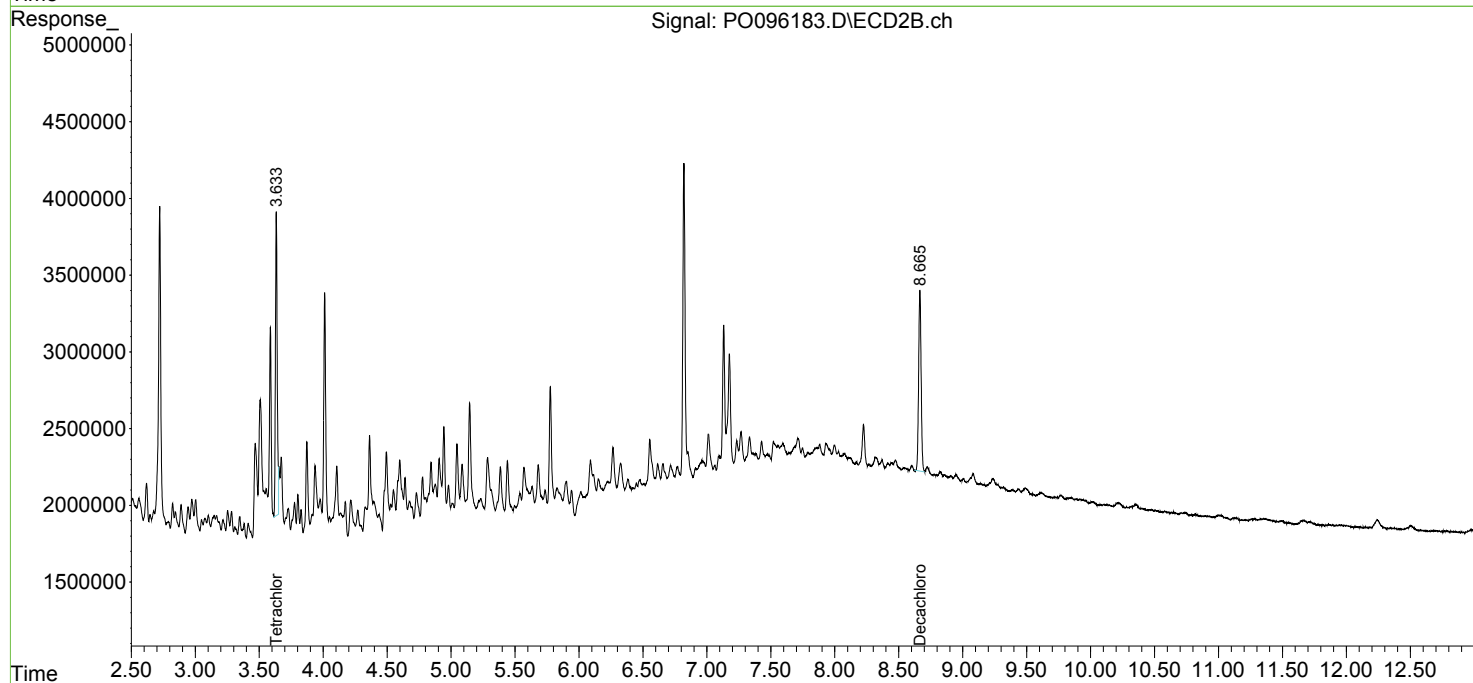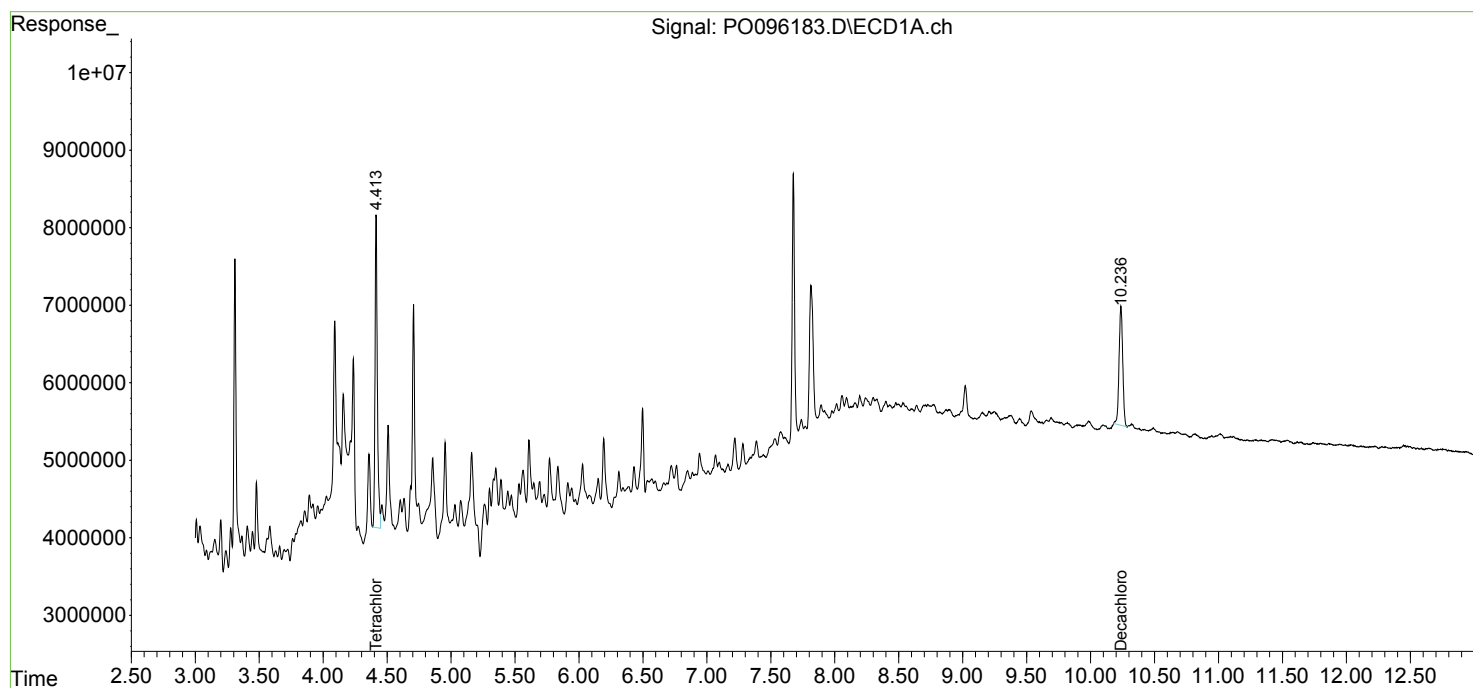

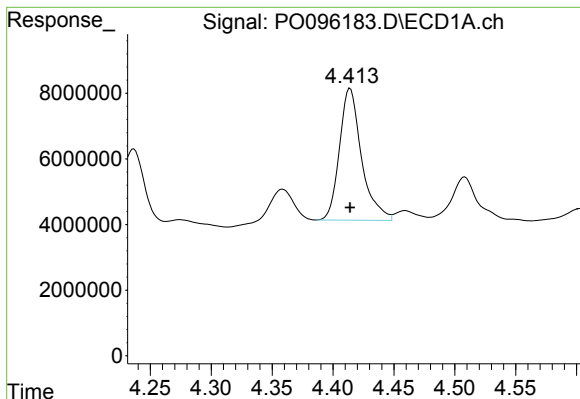


#1 Tetrachloro-m-xylene

R.T.: 4.413 min
Delta R.T.: 0.000 min
Response: 50897031
Conc: 16.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
713-D


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/17/2023
Supervised By :Ankita Jodhani 07/17/2023

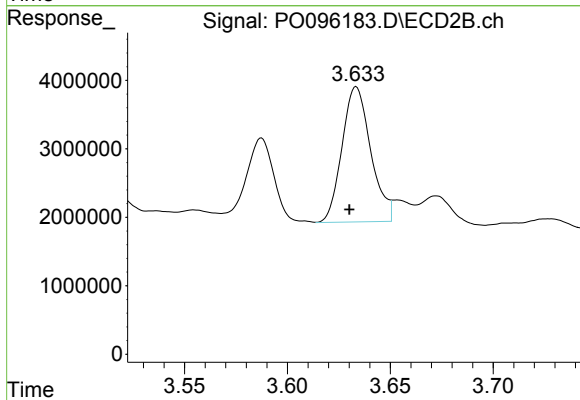


#1 Tetrachloro-m-xylene

R.T.: 3.633 min
Delta R.T.: 0.003 min
Response: 19139005
Conc: 14.20 ng/ml m

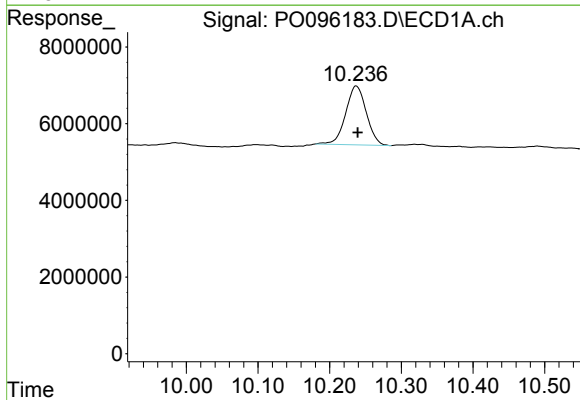

#2 Decachlorobiphenyl

R.T.: 10.237 min
Delta R.T.: -0.002 min
Response: 30688007
Conc: 15.29 ng/ml

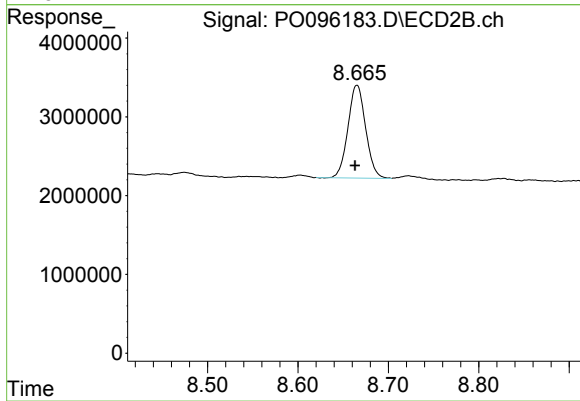

#2 Decachlorobiphenyl

R.T.: 8.665 min
Delta R.T.: 0.002 min
Response: 15983107
Conc: 13.67 ng/ml