

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071520\
Data File : P0069666.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jul 2020 9:03
Operator : DD\AJ
Sample : L3294-06
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
S3-03-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 13:33:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 08 16:12:41 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.391	3.564	906960	937043	24.292	23.546
2)	SA Decachlor...	10.048	8.769	725450	720534	12.057	12.696

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071520\
Data File : P0069666.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jul 2020 9:03
Operator : DD\AJ
Sample : L3294-06
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
S3-03-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 13:33:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 08 16:12:41 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

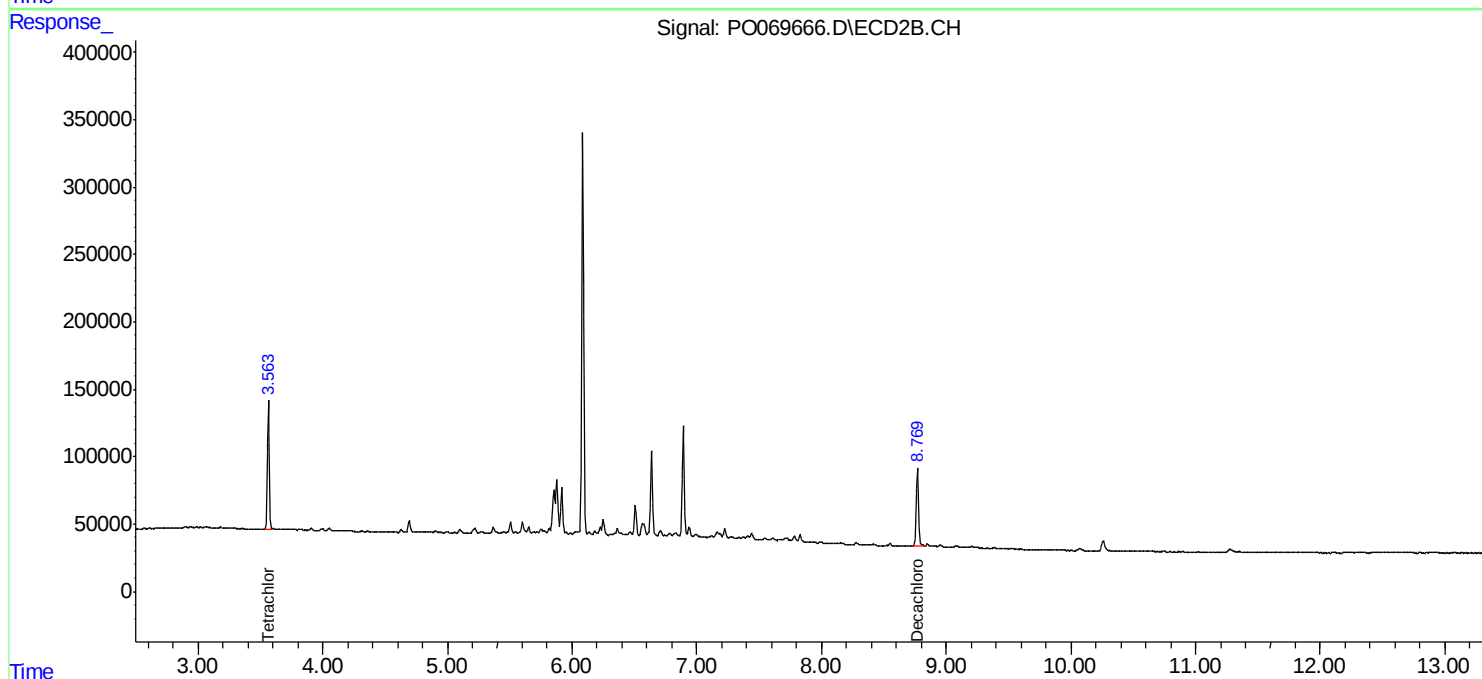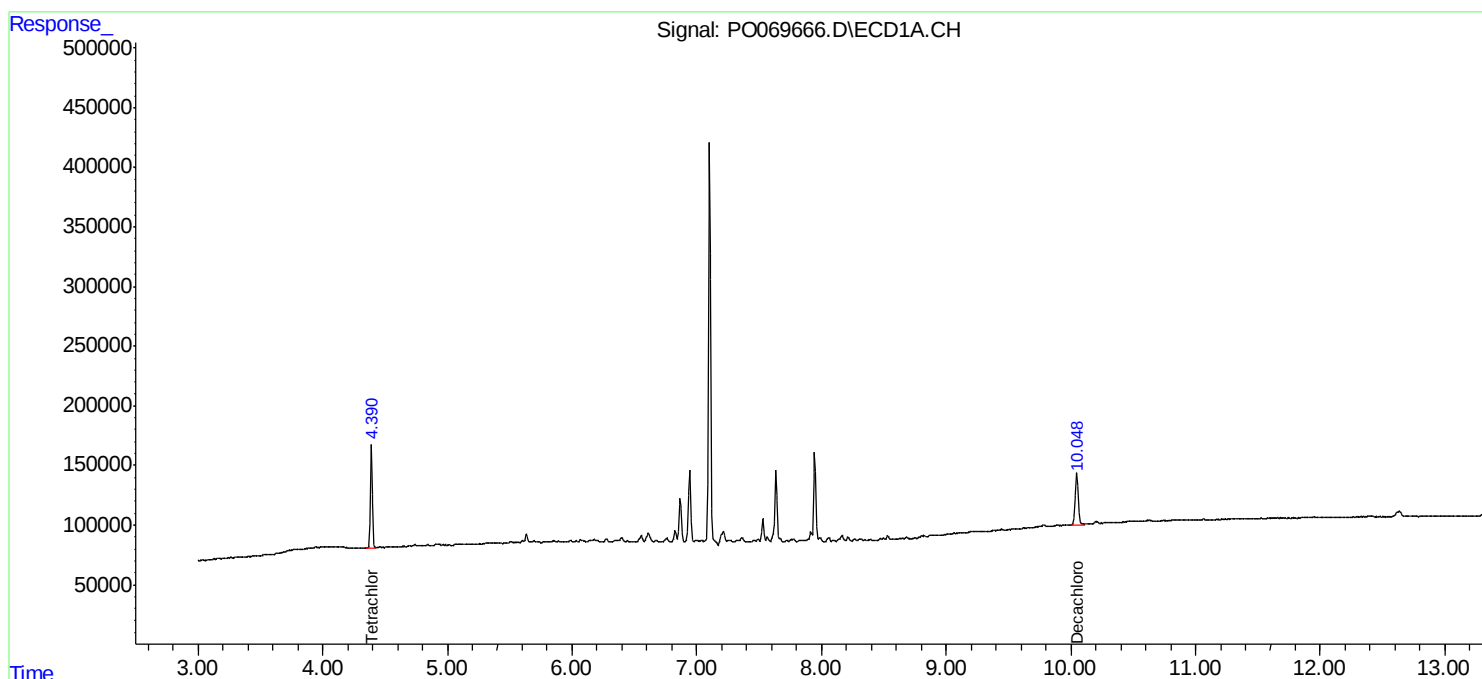


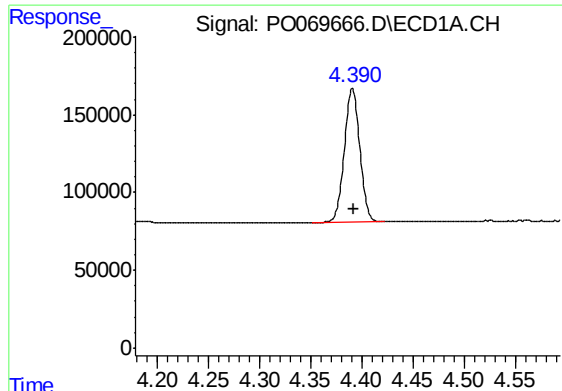

#1 Tetrachloro-m-xylene


R.T.: 4.391 min
Delta R.T.: -0.001 min
Response: 906960
Conc: 24.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
S3-03-S

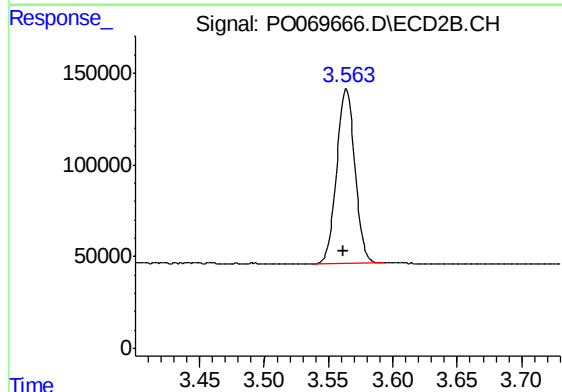


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: 0.002 min
Response: 937043
Conc: 23.55 ng/ml

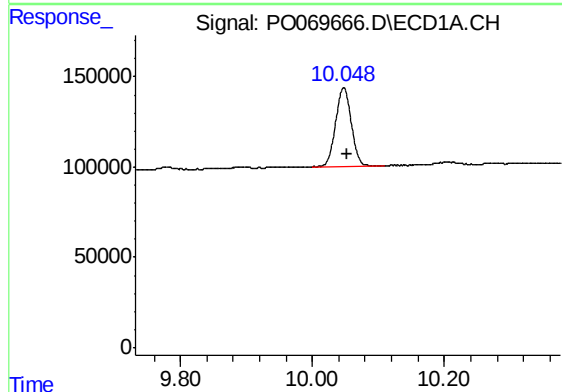

#2 Decachlorobiphenyl

R.T.: 10.048 min
Delta R.T.: -0.005 min
Response: 725450
Conc: 12.06 ng/ml

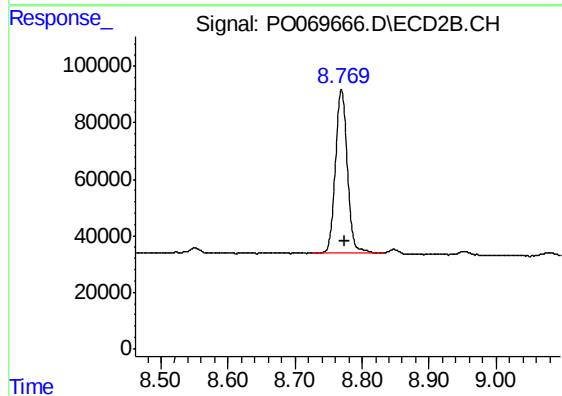

#2 Decachlorobiphenyl

R.T.: 8.769 min
Delta R.T.: -0.005 min
Response: 720534
Conc: 12.70 ng/ml