

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071520\
Data File : P0069669.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jul 2020 9:54
Operator : DD\AJ
Sample : L3294-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
S3-06-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 13:34:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 08 16:12:41 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.391	3.564	967721	1186774	25.919	29.821
2) SA Decachlor...	10.047	8.771	4369929	4249436	72.631m	74.875m

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071520\
Data File : P0069669.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jul 2020 9:54
Operator : DD\AJ
Sample : L3294-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
S3-06-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 15 13:34:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 08 16:12:41 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

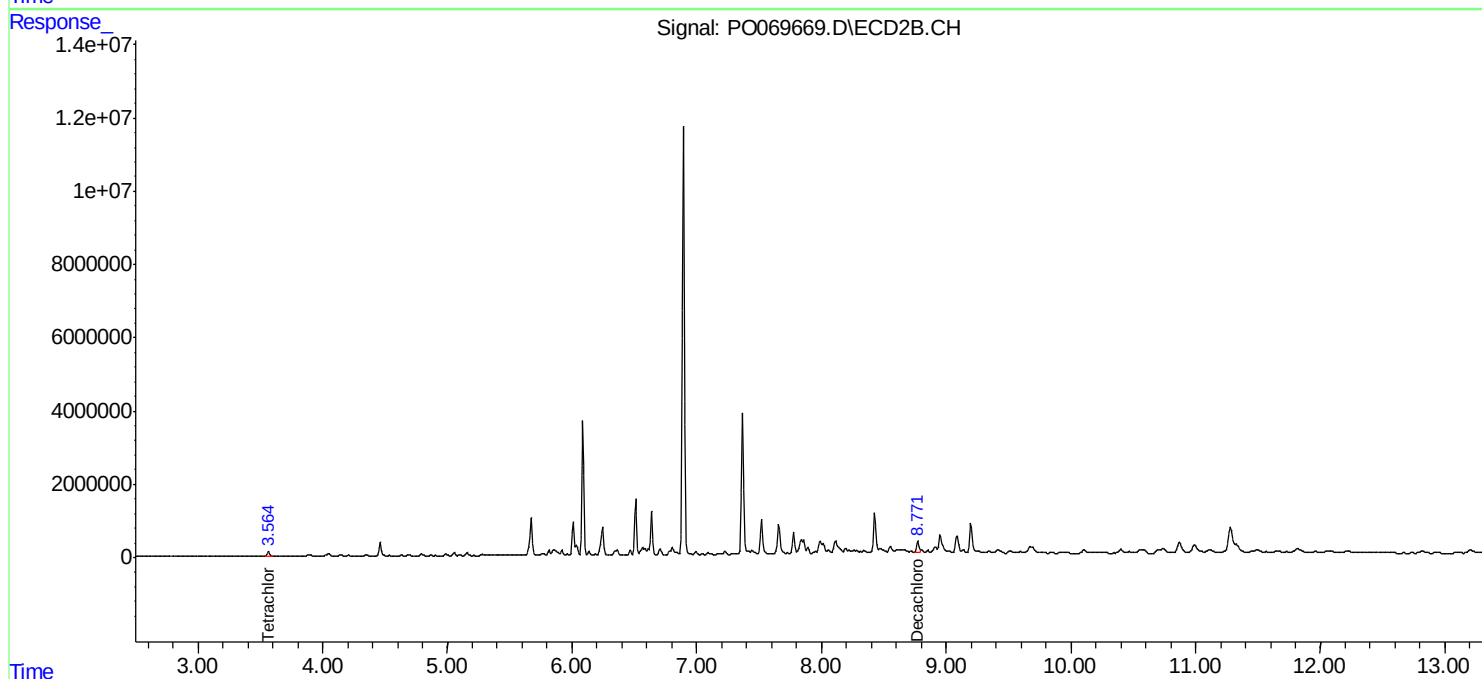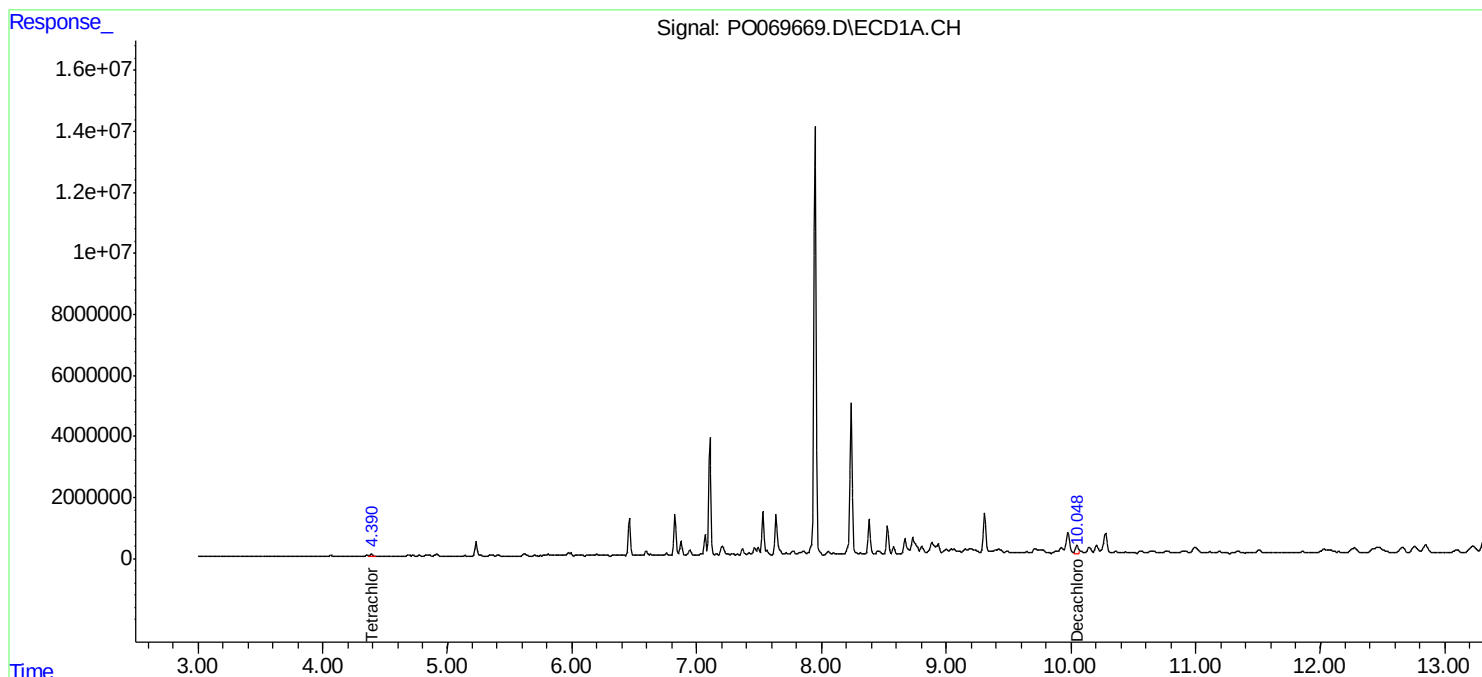


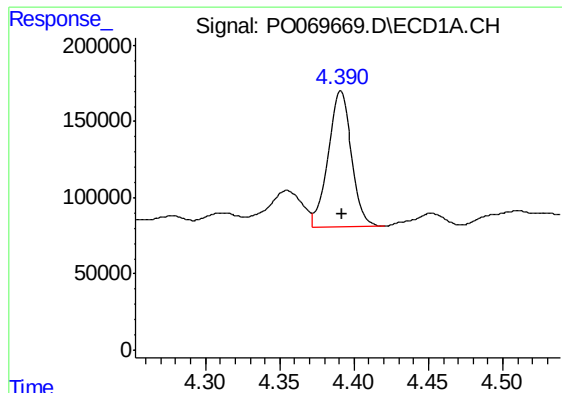

#1 Tetrachloro-m-xylene


R.T.: 4.391 min
Delta R.T.: -0.001 min
Response: 967721
Conc: 25.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
S3-06-B

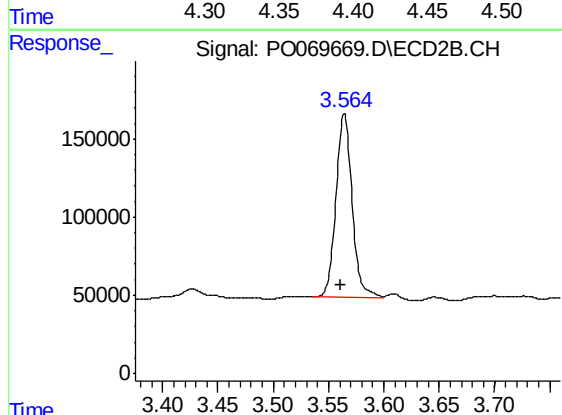


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: 0.003 min
Response: 1186774
Conc: 29.82 ng/ml

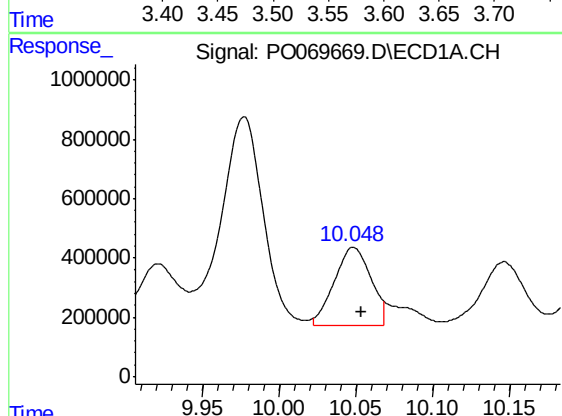

#2 Decachlorobiphenyl

R.T.: 10.047 min
Delta R.T.: -0.006 min
Response: 4369929
Conc: 72.63 ng/ml m

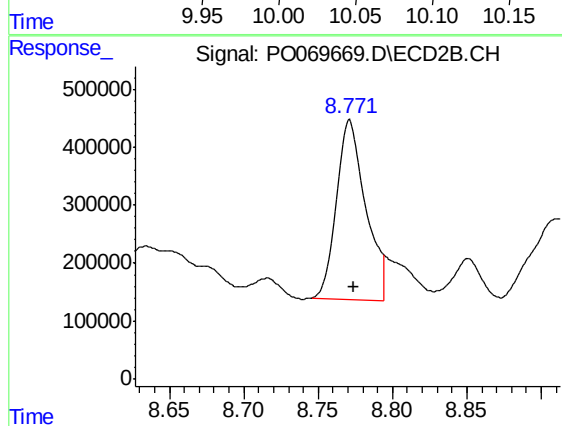

#2 Decachlorobiphenyl

R.T.: 8.771 min
Delta R.T.: -0.003 min
Response: 4249436
Conc: 74.87 ng/ml m