

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071520\
 Data File : P0069696.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jul 2020 23:37
 Operator : DD\AJ
 Sample : L3316-04
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S5-03-B

Manual Integrations
 APPROVED

Ankita
 7/16/2020 11:11:13 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 06:10:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 08 16:12:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.391	3.565	1069762	1074884	28.652	27.010
2)	SA Decachlor...	10.044	8.768	1366047	1215539	22.705m	21.418
Target Compounds							
31)	L7 AR-1260-1	7.362	6.363	458804	541748	174.489	205.397
32)	L7 AR-1260-2	7.630	6.563	825562	807760	232.723	246.783
33)	L7 AR-1260-3	7.986	6.708	336242	439586	116.307	144.380
34)	L7 AR-1260-4	8.211	7.189	476570	307821	160.898	113.722 #
35)	L7 AR-1260-5	8.528	7.441	553170	594318	81.753	92.737

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071520\
Data File : P0069696.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jul 2020 23:37
Operator : DD\AJ
Sample : L3316-04
Misc :
ALS Vial : 46 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S5-03-B


Manual Integrations
APPROVED

Ankita
7/16/2020 11:11:13 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 06:10:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 08 16:12:41 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

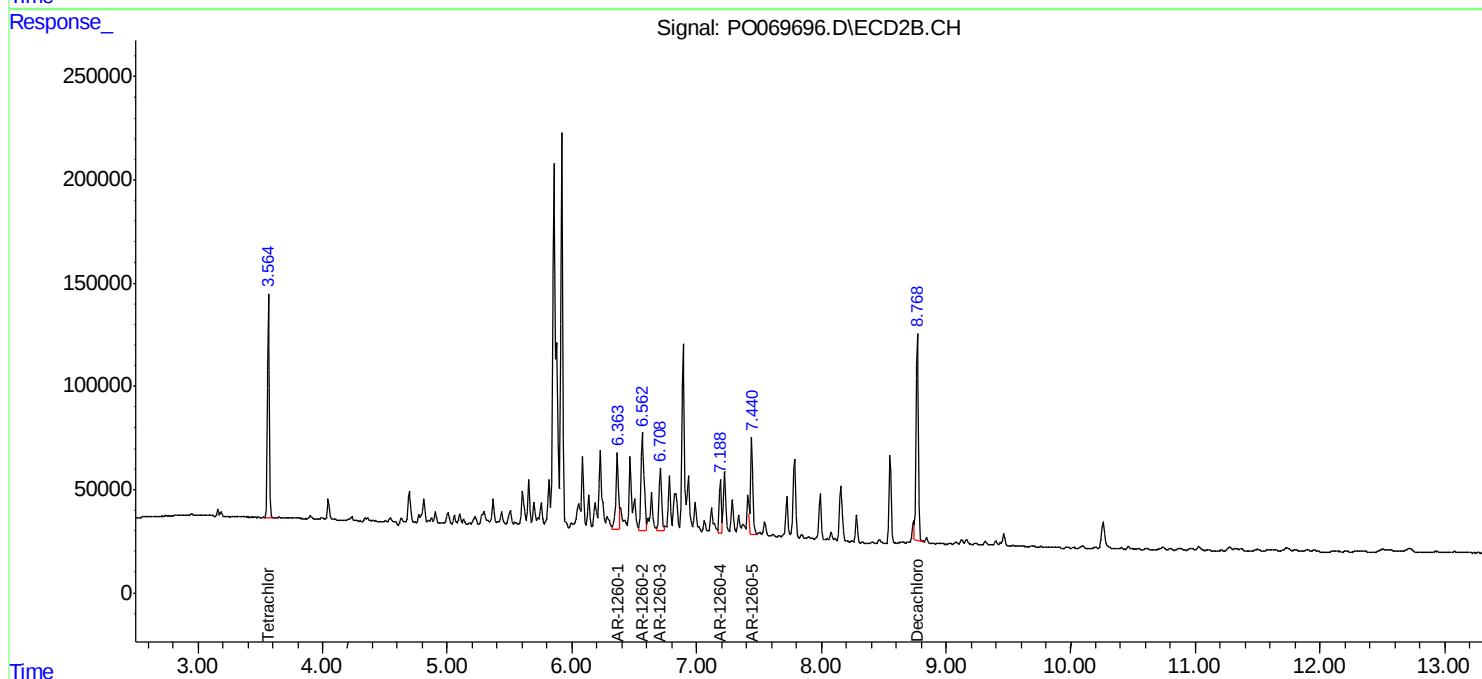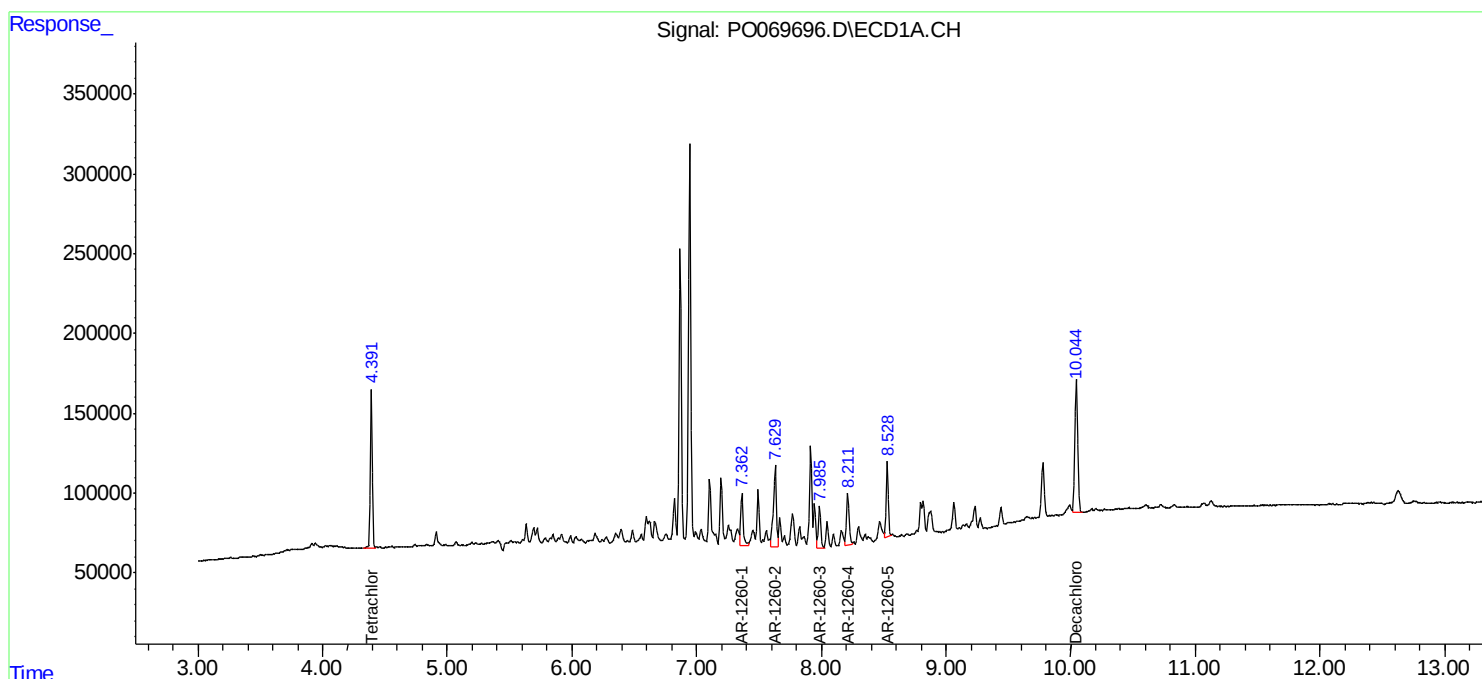

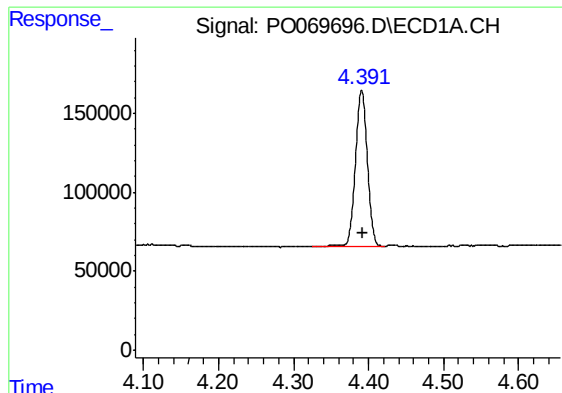


#1 Tetrachloro-m-xylene

R.T.: 4.391 min
Delta R.T.: -0.001 min
Response: 1069762
Conc: 28.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-03-B


Manual Integrations
APPROVED

Ankita
7/16/2020 11:11:13 AM

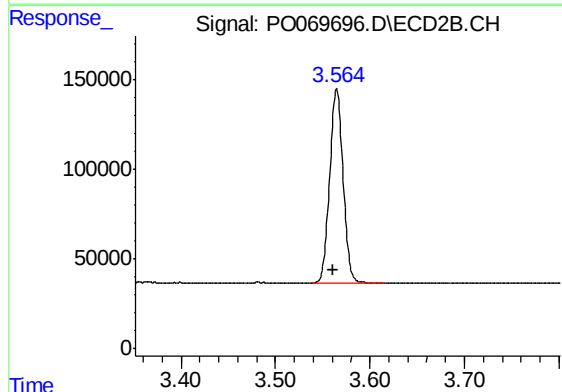


#1 Tetrachloro-m-xylene

R.T.: 3.565 min
Delta R.T.: 0.003 min
Response: 1074884
Conc: 27.01 ng/ml

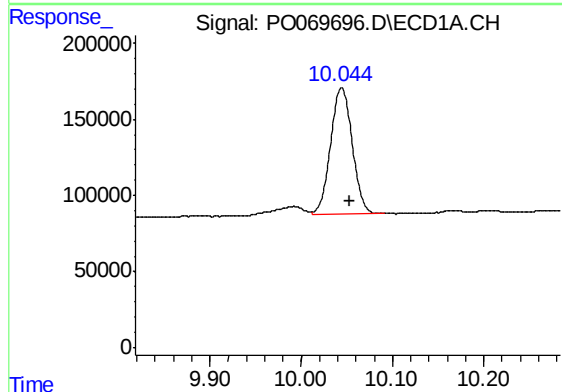


#2 Decachlorobiphenyl

R.T.: 10.044 min
Delta R.T.: -0.009 min
Response: 1366047
Conc: 22.70 ng/ml m

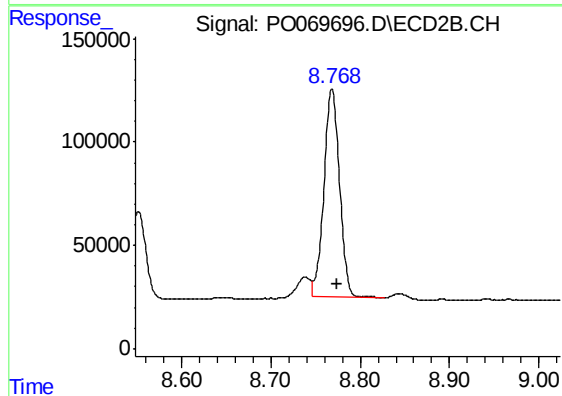

#2 Decachlorobiphenyl

R.T.: 8.768 min
Delta R.T.: -0.006 min
Response: 1215539
Conc: 21.42 ng/ml

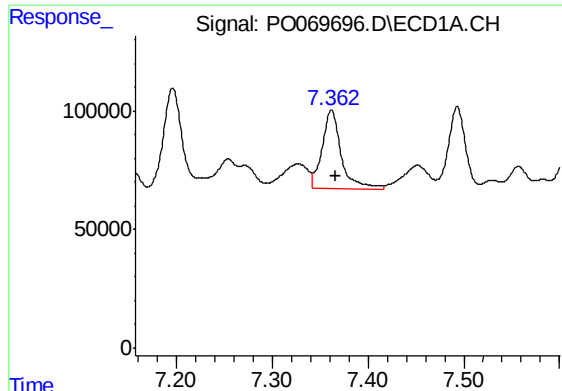


#31 AR-1260-1

R.T.: 7.362 min
Delta R.T.: -0.004 min
Response: 458804
Conc: 174.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-03-B


Manual Integrations
APPROVED

Ankita
7/16/2020 11:11:13 AM

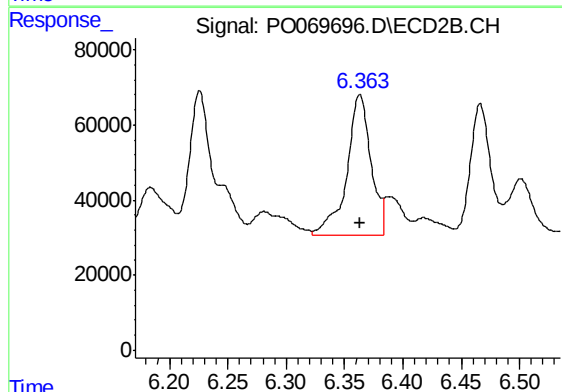


#31 AR-1260-1

R.T.: 6.363 min
Delta R.T.: 0.000 min
Response: 541748
Conc: 205.40 ng/ml

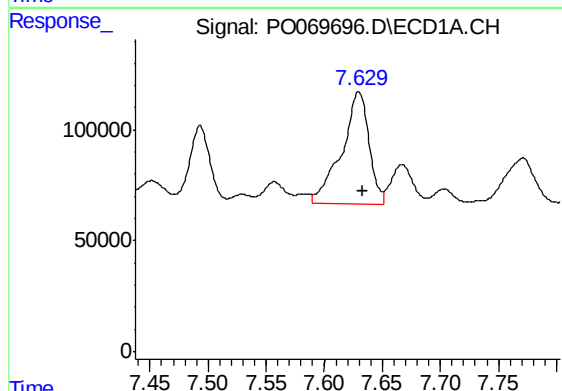


#32 AR-1260-2

R.T.: 7.630 min
Delta R.T.: -0.003 min
Response: 825562
Conc: 232.72 ng/ml

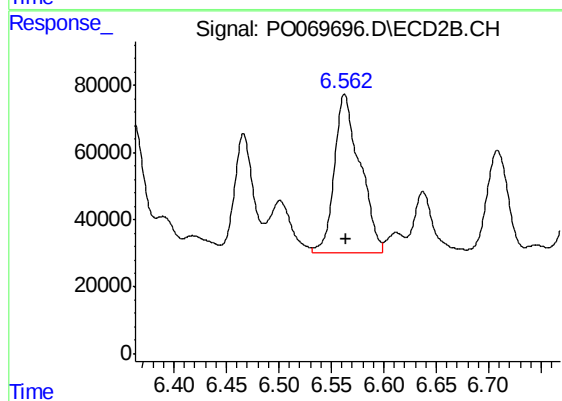

#32 AR-1260-2

R.T.: 6.563 min
Delta R.T.: -0.001 min
Response: 807760
Conc: 246.78 ng/ml

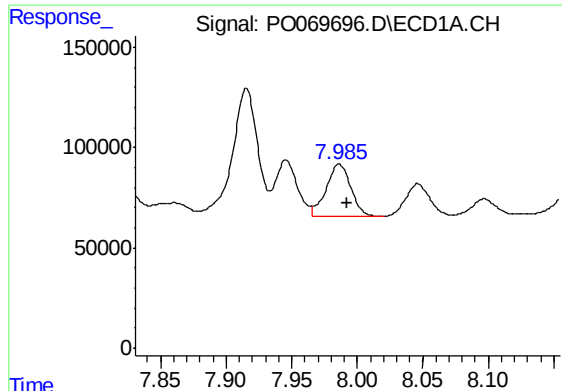


#33 AR-1260-3

R.T.: 7.986 min
Delta R.T.: -0.006 min
Response: 336242
Conc: 116.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-03-B


Manual Integrations
APPROVED

Ankita
7/16/2020 11:11:13 AM

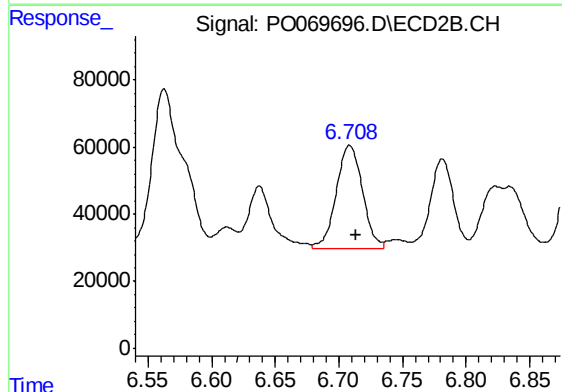


#33 AR-1260-3

R.T.: 6.708 min
Delta R.T.: -0.005 min
Response: 439586
Conc: 144.38 ng/ml

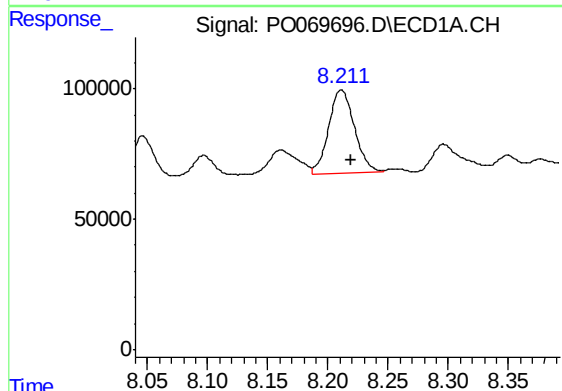


#34 AR-1260-4

R.T.: 8.211 min
Delta R.T.: -0.008 min
Response: 476570
Conc: 160.90 ng/ml

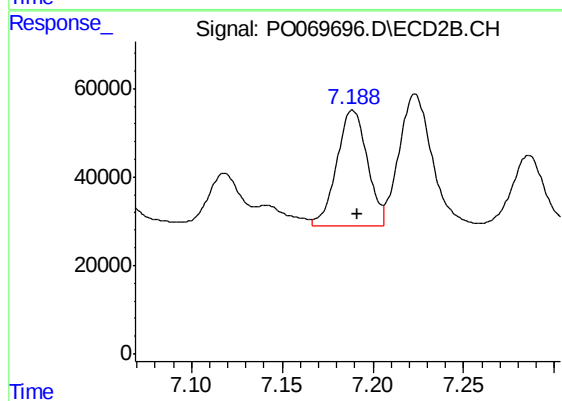

#34 AR-1260-4

R.T.: 7.189 min
Delta R.T.: -0.003 min
Response: 307821
Conc: 113.72 ng/ml

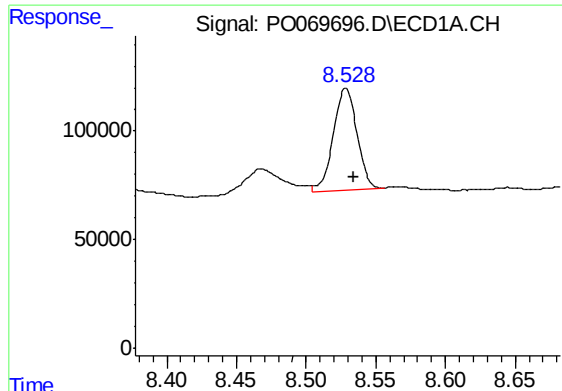


#35 AR-1260-5

R.T.: 8.528 min
Delta R.T.: -0.005 min
Response: 553170
Conc: 81.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-03-B

Manual Integrations
APPROVED

Ankita
7/16/2020 11:11:13 AM

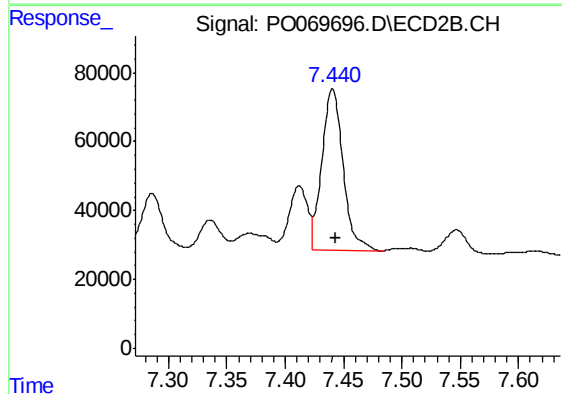

#35 AR-1260-5

R.T.: 7.441 min
Delta R.T.: -0.003 min
Response: 594318
Conc: 92.74 ng/ml