

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071521\
 Data File : P0079569.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jul 2021 13:01
 Operator : DD\AJ
 Sample : M3047-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-EF-01-020-ABCD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 02:34:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 10 00:52:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.017	4.222	1437326	548361	21.498	19.122
2) SA Decachlor...	11.143	9.686	1120416	493731	22.029	18.656

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071521\
Data File : P0079569.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jul 2021 13:01
Operator : DD\AJ
Sample : M3047-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-EF-01-020-ABCD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 02:34:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 10 00:52:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

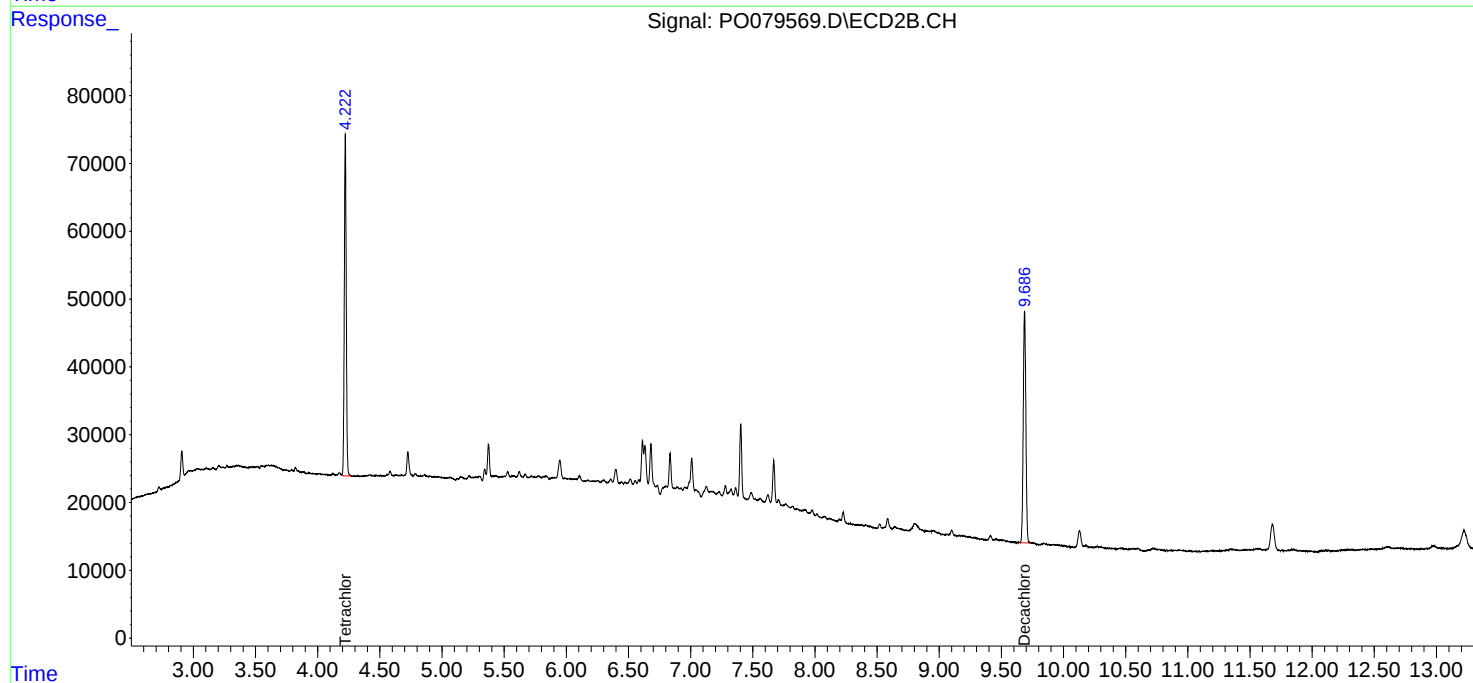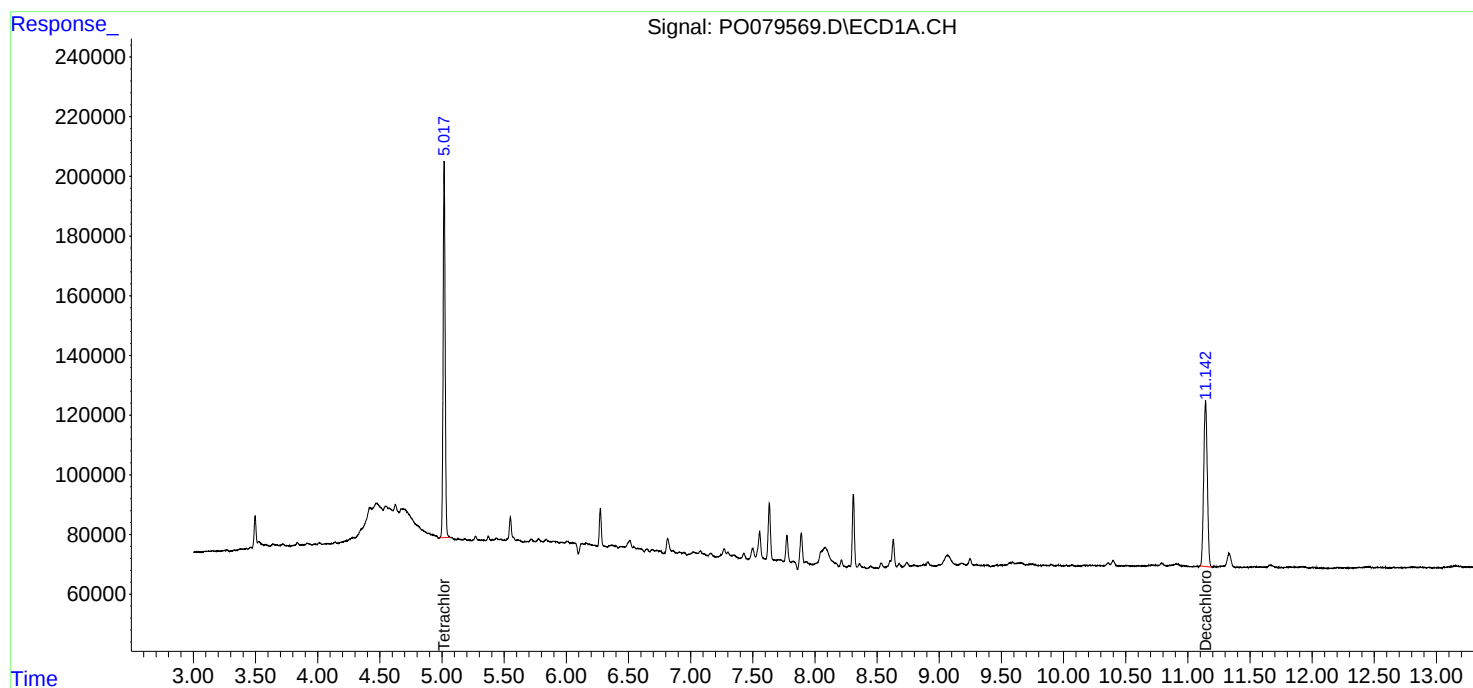


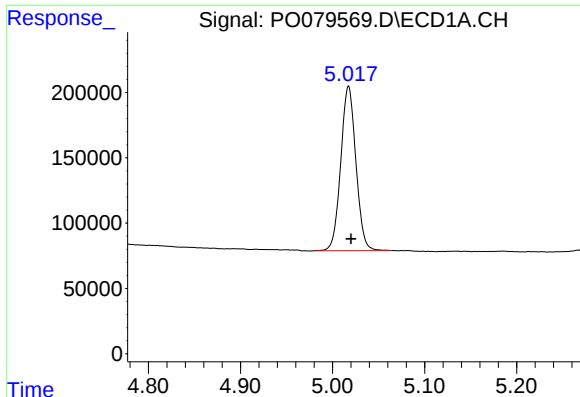

#1 Tetrachloro-m-xylene


R.T.: 5.017 min
Delta R.T.: -0.003 min
Response: 1437326
Conc: 21.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-EF-01-020-ABCD

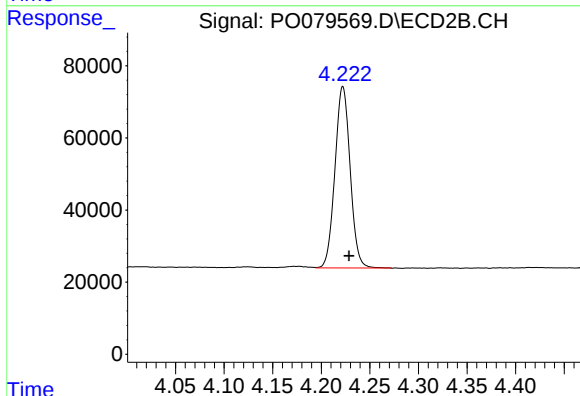


#1 Tetrachloro-m-xylene

R.T.: 4.222 min
Delta R.T.: -0.007 min
Response: 548361
Conc: 19.12 ng/ml

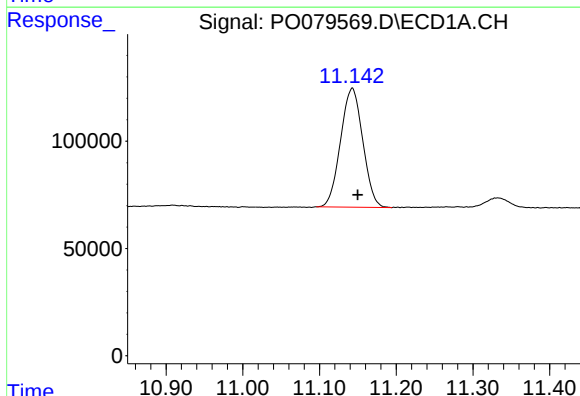

#2 Decachlorobiphenyl

R.T.: 11.143 min
Delta R.T.: -0.007 min
Response: 1120416
Conc: 22.03 ng/ml

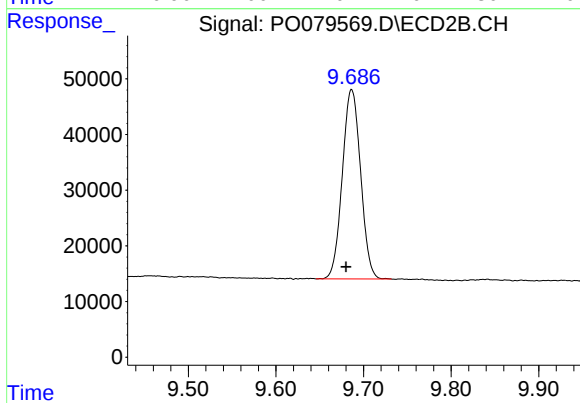

#2 Decachlorobiphenyl

R.T.: 9.686 min
Delta R.T.: 0.006 min
Response: 493731
Conc: 18.66 ng/ml