

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071521\
 Data File : P0079571.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jul 2021 13:35
 Operator : DD\AJ
 Sample : M3038-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-07-COMP

Manual Integrations
 APPROVED

mohammad
 7/16/2021 11:37:36 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 02:37:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 10 00:52:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.019	4.222	1590467	613330	23.788	21.388m
2) SA Decachlor...	11.144	9.689	1100225	504324	21.632	19.056

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071521\
Data File : P0079571.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jul 2021 13:35
Operator : DD\AJ
Sample : M3038-04
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-07-COMP


Manual Integrations
APPROVED

mohammad
7/16/2021 11:37:36 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 02:37:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 10 00:52:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

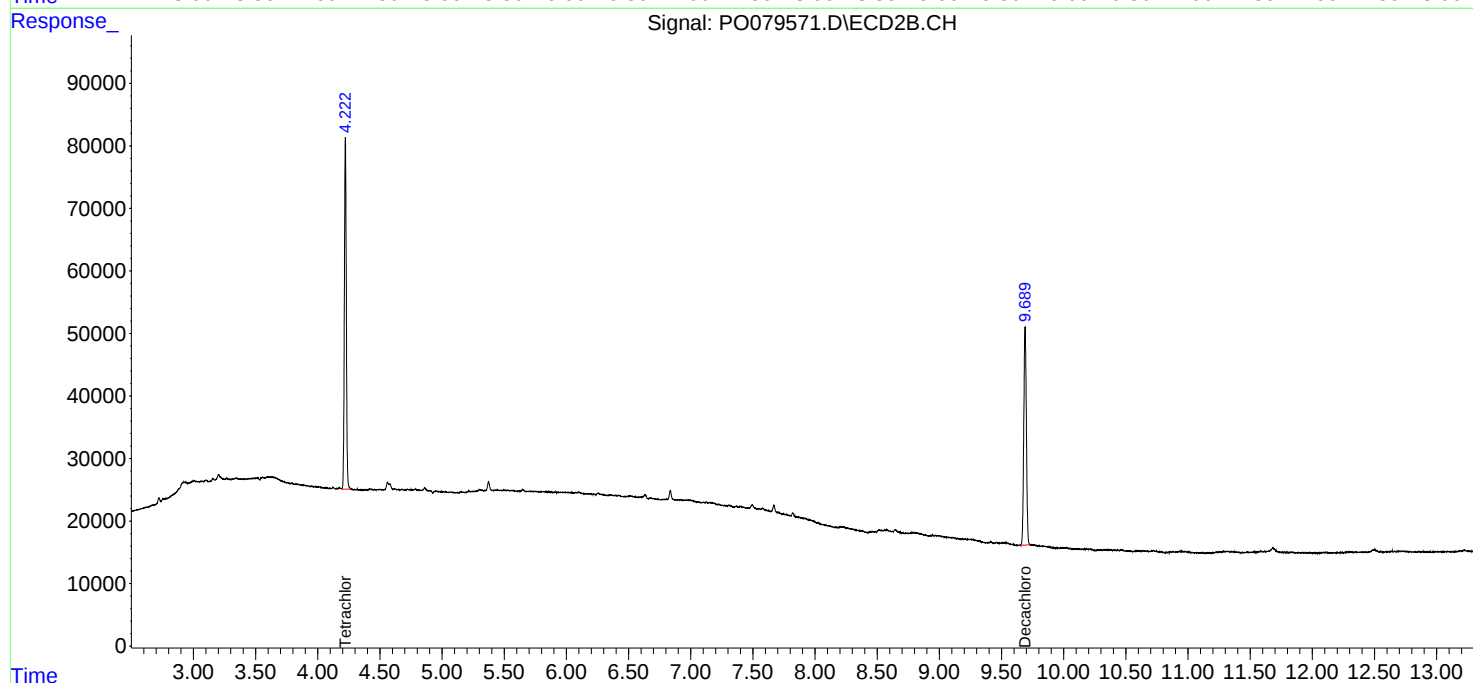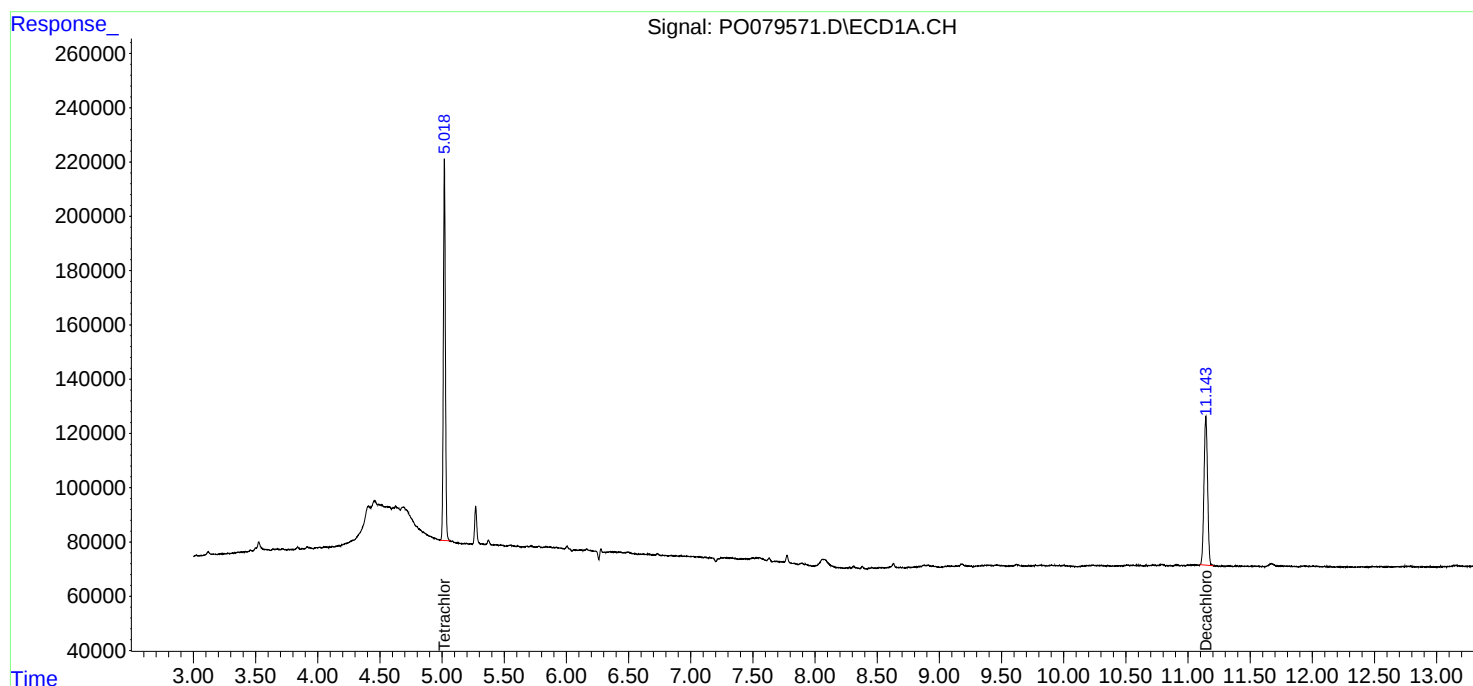

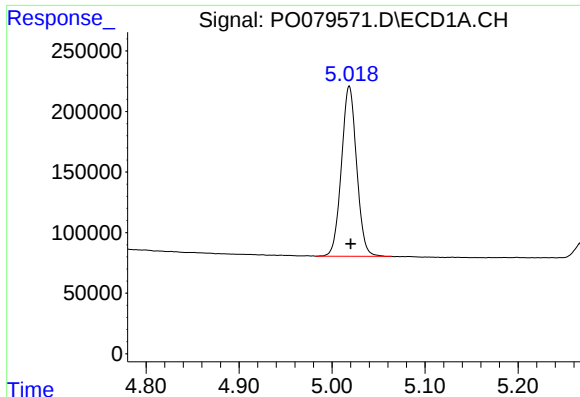


#1 Tetrachloro-m-xylene

R.T.: 5.019 min
Delta R.T.: -0.001 min
Response: 1590467
Conc: 23.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-07-COMP


Manual Integrations
APPROVED

mohammad
7/16/2021 11:37:36 AM

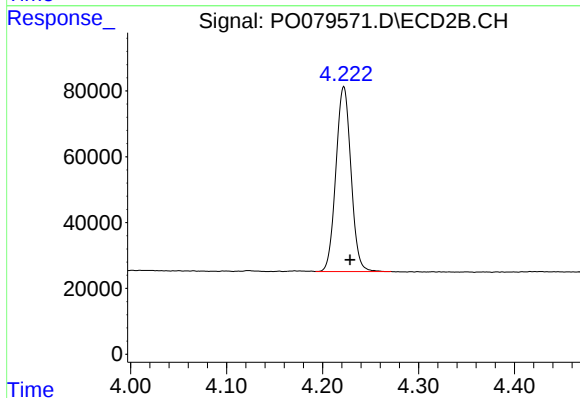


#1 Tetrachloro-m-xylene

R.T.: 4.222 min
Delta R.T.: -0.007 min
Response: 613330
Conc: 21.39 ng/ml m

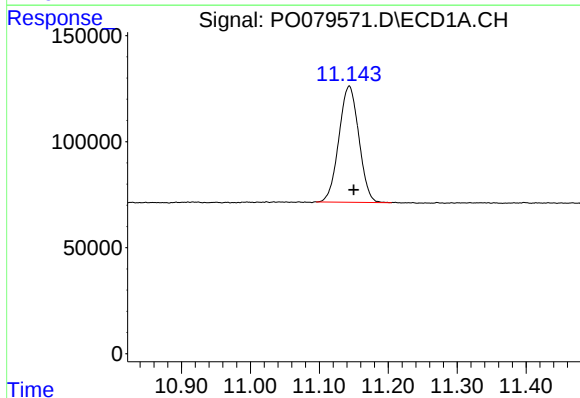

#2 Decachlorobiphenyl

R.T.: 11.144 min
Delta R.T.: -0.006 min
Response: 1100225
Conc: 21.63 ng/ml

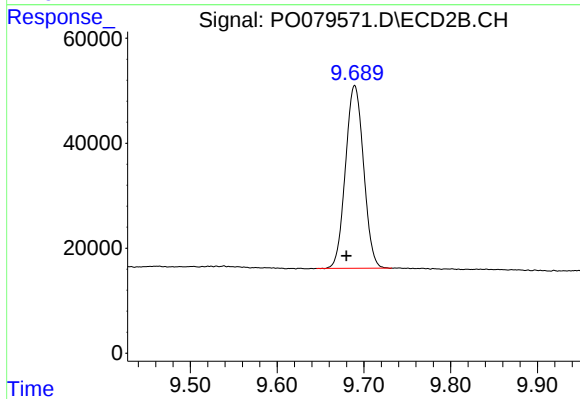

#2 Decachlorobiphenyl

R.T.: 9.689 min
Delta R.T.: 0.009 min
Response: 504324
Conc: 19.06 ng/ml