

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071521\
 Data File : P0079582.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jul 2021 16:46
 Operator : DD\AJ
 Sample : M3039-12
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-05-COMP

Manual Integrations
 APPROVED

mohammad
 7/16/2021 11:37:43 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 02:46:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 10 00:52:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.018	4.226	1490378	581798	22.291	20.288m
2) SA Decachlor...	11.142	9.692	1012890	480572	19.915	18.159

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071521\
Data File : P0079582.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jul 2021 16:46
Operator : DD\AJ
Sample : M3039-12
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-05-COMP


Manual Integrations
APPROVED

mohammad
7/16/2021 11:37:43 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 02:46:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 10 00:52:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

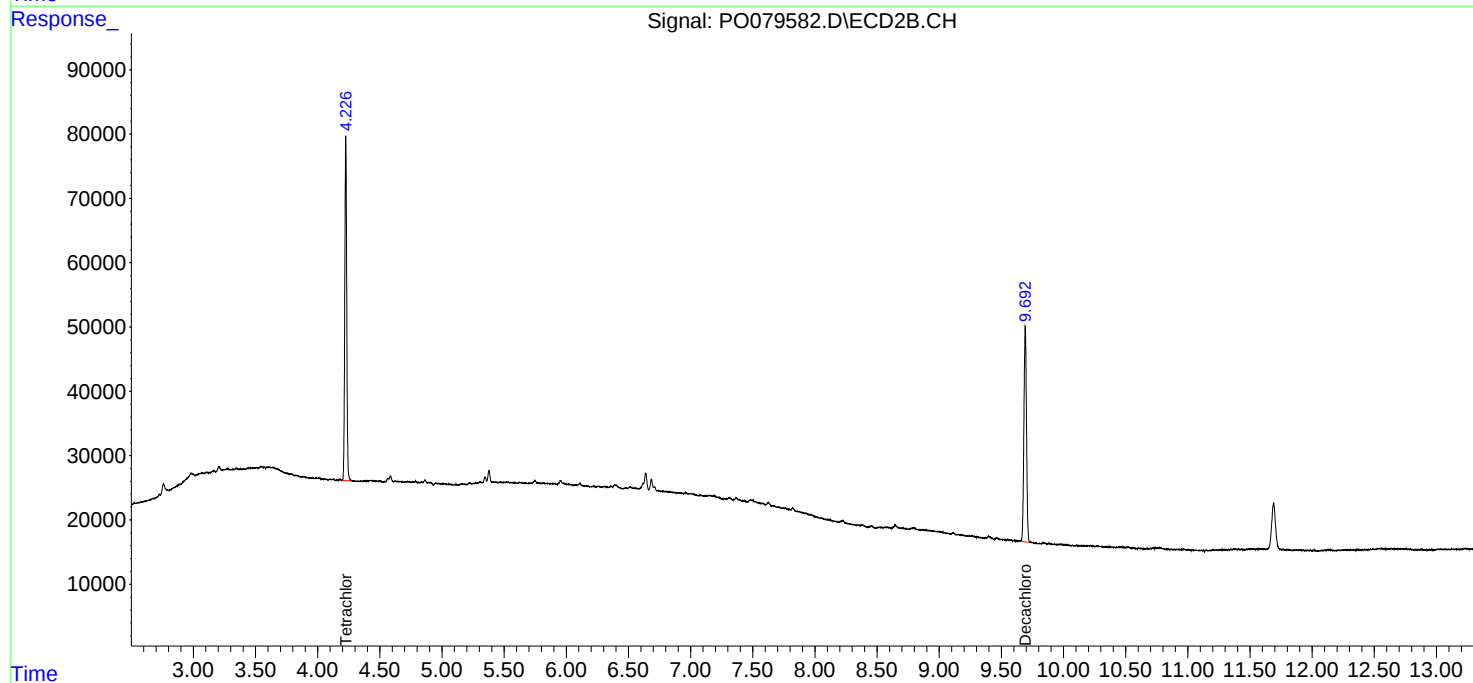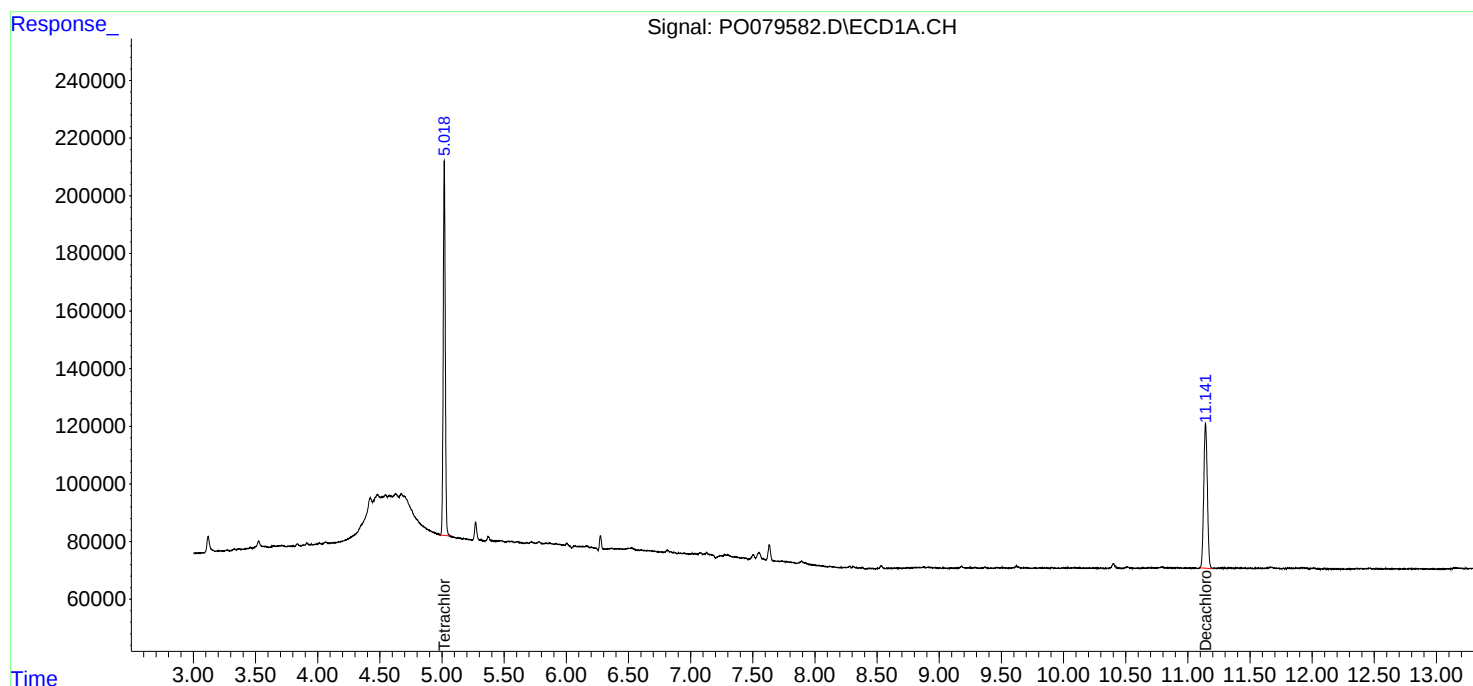

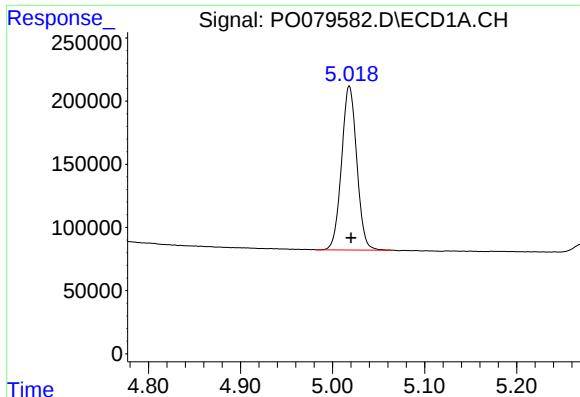


#1 Tetrachloro-m-xylene

R.T.: 5.018 min
Delta R.T.: -0.002 min
Response: 1490378
Conc: 22.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-05-COMP


Manual Integrations
APPROVED

mohammad
7/16/2021 11:37:43 AM

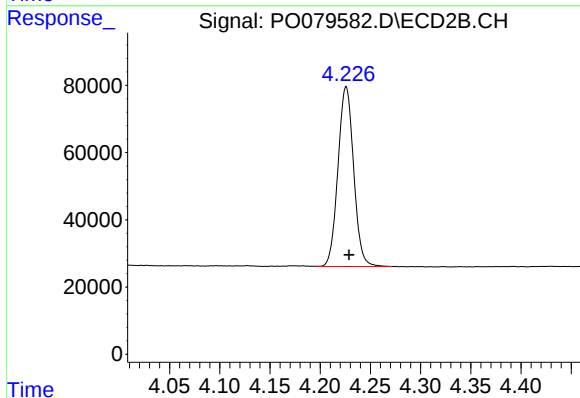


#1 Tetrachloro-m-xylene

R.T.: 4.226 min
Delta R.T.: -0.003 min
Response: 581798
Conc: 20.29 ng/ml m

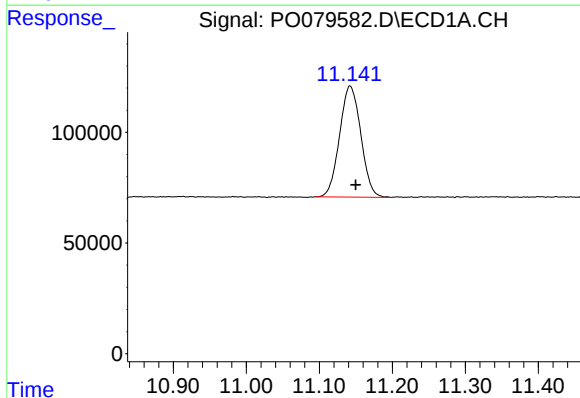

#2 Decachlorobiphenyl

R.T.: 11.142 min
Delta R.T.: -0.008 min
Response: 1012890
Conc: 19.91 ng/ml

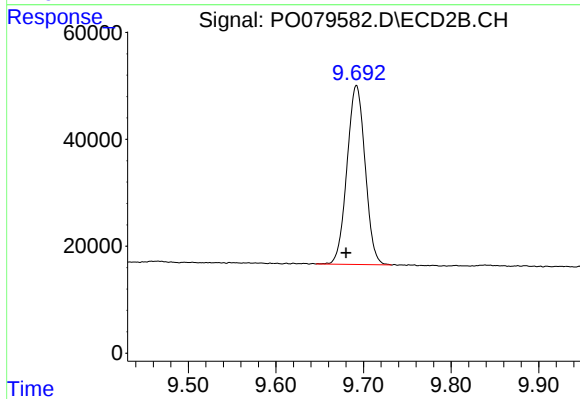

#2 Decachlorobiphenyl

R.T.: 9.692 min
Delta R.T.: 0.012 min
Response: 480572
Conc: 18.16 ng/ml