

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071521\
 Data File : P0079584.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jul 2021 17:21
 Operator : DD\AJ
 Sample : M3040-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-PS-01-076

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 02:43:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 10 00:52:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.019	4.227	1361748	530086	20.367	18.485
2)	SA Decachlor...	11.144	9.695	639656	302025	12.577	11.412

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071521\
Data File : P0079584.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jul 2021 17:21
Operator : DD\AJ
Sample : M3040-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-076

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 02:43:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 10 00:52:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

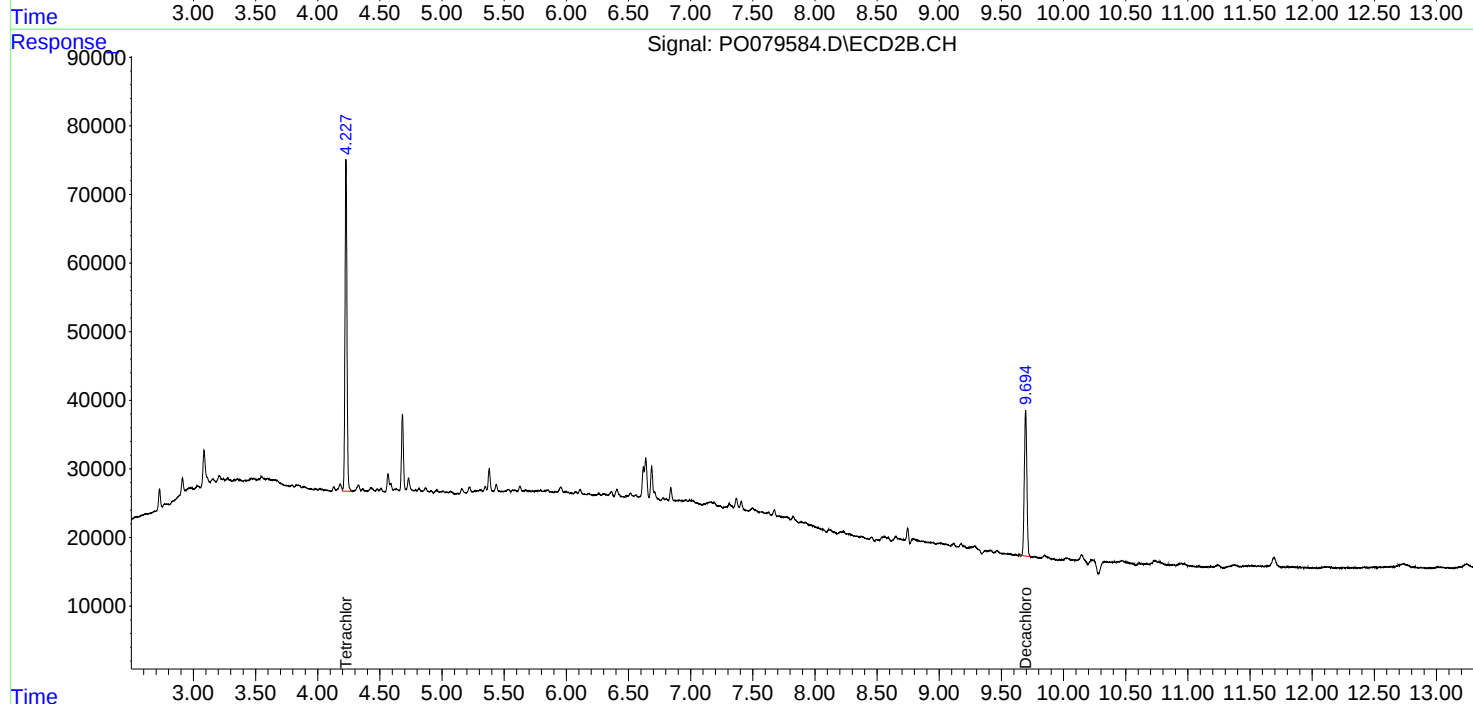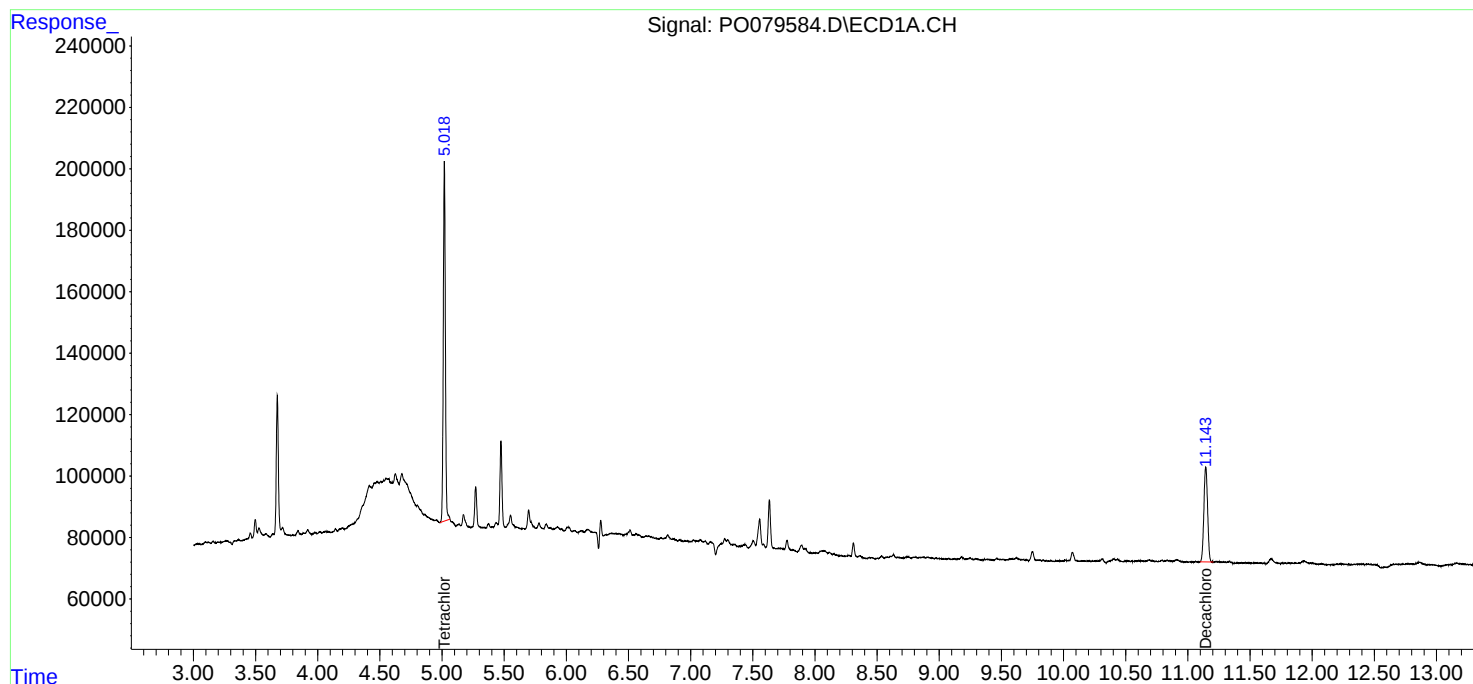


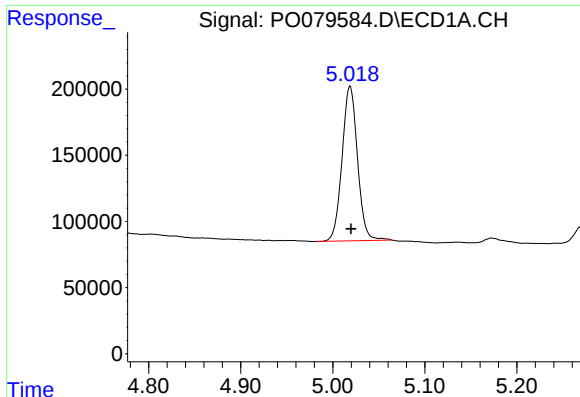

#1 Tetrachloro-m-xylene


R.T.: 5.019 min
Delta R.T.: -0.001 min
Response: 1361748
Conc: 20.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-076

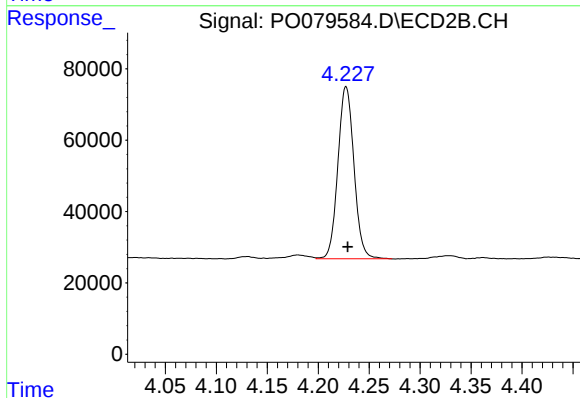


#1 Tetrachloro-m-xylene

R.T.: 4.227 min
Delta R.T.: -0.001 min
Response: 530086
Conc: 18.49 ng/ml

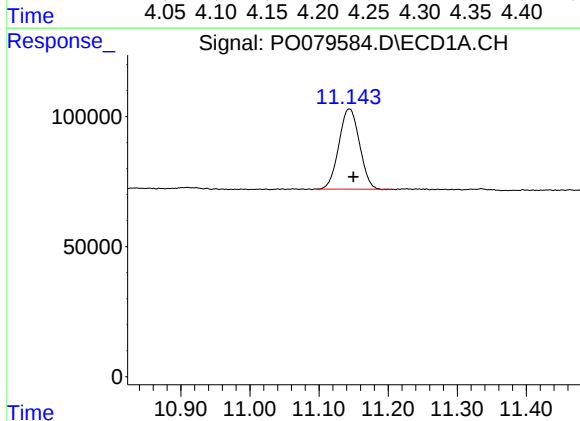

#2 Decachlorobiphenyl

R.T.: 11.144 min
Delta R.T.: -0.006 min
Response: 639656
Conc: 12.58 ng/ml

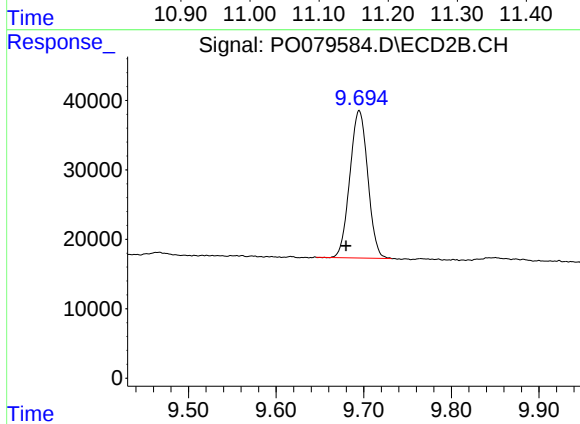

#2 Decachlorobiphenyl

R.T.: 9.695 min
Delta R.T.: 0.015 min
Response: 302025
Conc: 11.41 ng/ml