

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0071525\
 Data File : P0112281.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jul 2025 11:20
 Operator : YP/AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 01:40:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 10:50:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
2)	SA Decachlor...	8.696	8.647	431547	64807	0.063	0.038 #
Target Compounds							
3)	L1 AR-1016-1	4.769	4.757	206927	210403	0.608	0.944 #
4)	L1 AR-1016-2	4.788	4.779	655451	216587	1.318	0.658 #
5)	L1 AR-1016-3	4.842	4.943	934341	295591	2.886	1.740 #
6)	L1 AR-1016-4	4.952	5.002	2287648	196532	8.908	1.432 #
7)	L1 AR-1016-5	5.213	5.207	5770687	561394	21.087	3.255 #
8)	L2 AR-1221-1	3.887	3.881	185175	127954	1.588	1.555
9)	L2 AR-1221-2	3.961	3.958	350576	53398	4.447	0.900 #
12)	L3 AR-1232-2	4.513	4.766	216942	217693	1.909	1.422 #
13)	L3 AR-1232-3	4.788	4.935	655451	188057	2.862	2.491
14)	L3 AR-1232-4	4.952	5.023	2287648	118356	20.015	1.794 #
15)	L3 AR-1232-5	5.007	5.186	3426259	407869	46.679	5.492 #
16)	L4 AR-1242-1	4.753	4.741	244154	245811	0.843	1.268 #
17)	L4 AR-1242-2	4.769	4.757	206927	210403	0.486	0.743 #
18)	L4 AR-1242-3	4.842	4.935	934341	188057	3.414	1.291 #
19)	L4 AR-1242-4	4.952	5.023	2287648	118356	10.153	0.834 #
20)	L4 AR-1242-5	5.613	5.524	3431865	2551230	16.213	14.038
21)	L5 AR-1248-1	4.769	4.741	206927	245811	0.912	1.592 #
22)	L5 AR-1248-2	5.007	4.979	3426259	1407527	11.112	6.840 #
23)	L5 AR-1248-3	5.213	5.023	5770687	118356	14.167	0.551 #
24)	L5 AR-1248-4	5.580	5.186	6578002	407869	11.397	1.576 #
25)	L5 AR-1248-5	5.613	5.588	3431865	876912	8.793	3.500 #
26)	L6 AR-1254-1	5.580	5.524	6578002	2551230	10.694	6.693 #
27)	L6 AR-1254-2	5.705	5.706	1175626	12012292	2.195	36.202 #
28)	L6 AR-1254-3	6.134	6.103	9209413	11974724	10.969	24.842 #
29)	L6 AR-1254-4	6.347	6.310	487844	319304	1.014	1.225
30)	L6 AR-1254-5	6.763	6.728	3980.5E6	1881.9E6	5143.127	5280.816
31)	L7 AR-1260-1	6.242	6.238	65296	681926	0.130	2.431 #
32)	L7 AR-1260-2	6.441	6.437	9102724	25987	12.332	0.076 #
33)	L7 AR-1260-3	6.763f	6.601	3980.5E6	-10698	6072.649	N.D. #
34)	L7 AR-1260-4	7.067	6.987f	5623154	2545728	12.919	12.688
35)	L7 AR-1260-5	7.303	7.303	1929190	123738	1.528	0.276 #
36)	L8 AR-1262-1	6.763f	6.728f	3980.5E6	1881.9E6	3896.019	4620.072
37)	L8 AR-1262-2	7.303	7.303	1929190	123738	1.177	0.241 #
38)	L8 AR-1262-3	7.592	7.557	1377837	2627603	2.146	14.636 #
39)	L8 AR-1262-4	7.662	7.557f	58965	2627603	0.055	9.032 #
40)	L8 AR-1262-5	8.164	8.125	8391955	101137	18.726	0.956 #
41)	L9 AR-1268-1	7.592	7.557	1377837	2627603	0.750	5.347 #
42)	L9 AR-1268-2	7.662	7.557f	58965	2627603	0.038	6.298 #
43)	L9 AR-1268-3	7.818f	7.813	219678	76874	0.169	0.243 #
44)	L9 AR-1268-4	8.164	8.125	8391955	101137	17.468	0.907 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071525\
Data File : P0112281.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2025 11:20
Operator : YP/AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 01:40:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 09 10:50:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
45) L9	AR-1268-5	8.433	8.384	495364	153498	0.152	0.211 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071525\
Data File : PO112281.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jul 2025 11:20
Operator : YP/AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 01:40:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 09 10:50:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

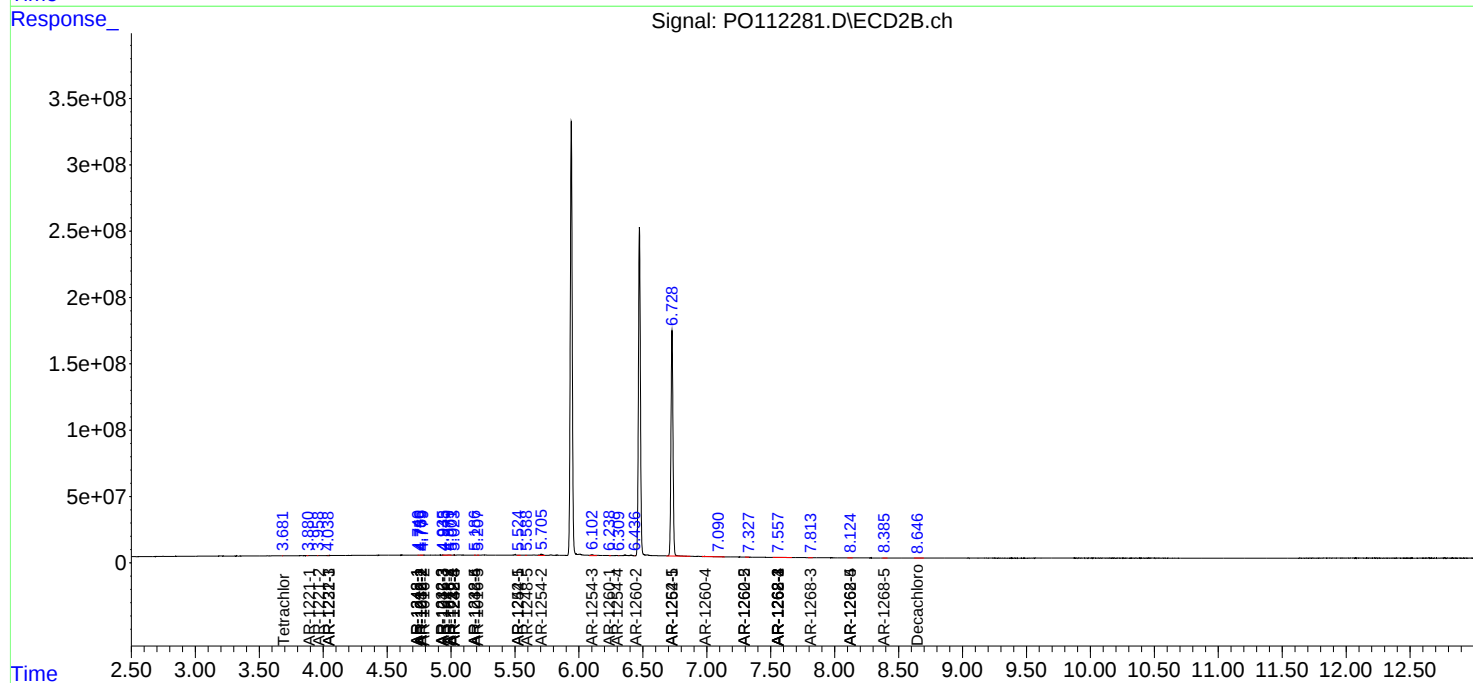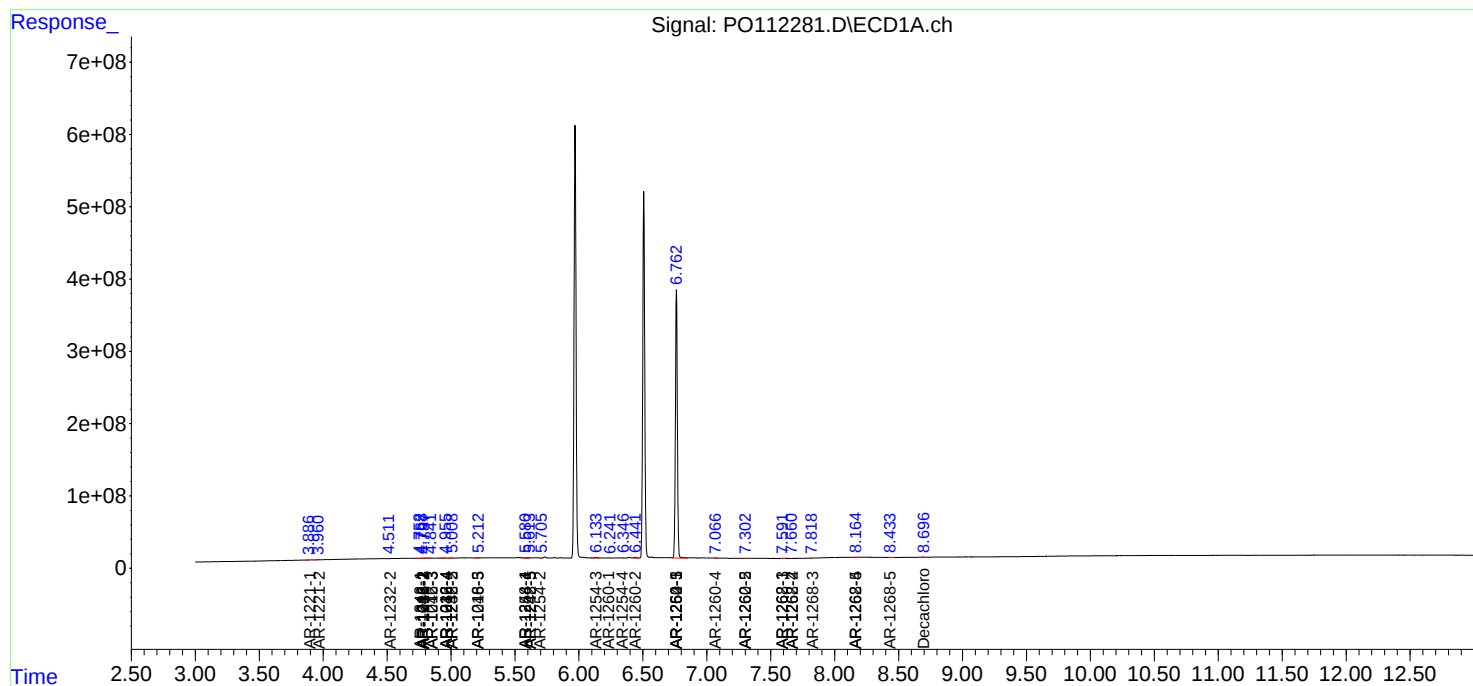


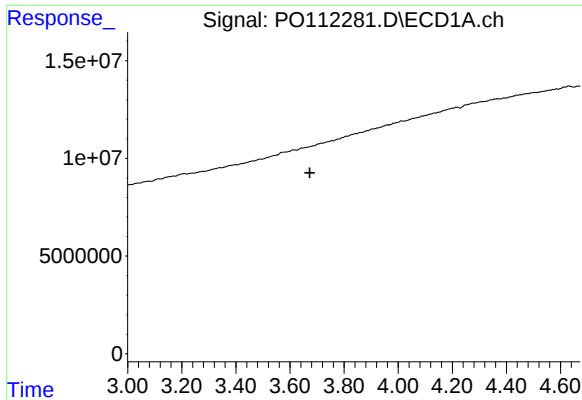

#1 Tetrachloro-m-xylene


R.T.: 3.716 min
Delta R.T.: 0.043 min
Response: -595679
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

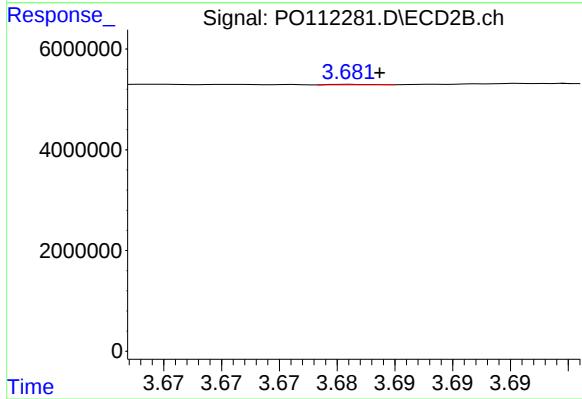


#1 Tetrachloro-m-xylene

R.T.: 3.681 min
Delta R.T.: -0.003 min
Response: 22902
Conc: 0.00 ng/ml

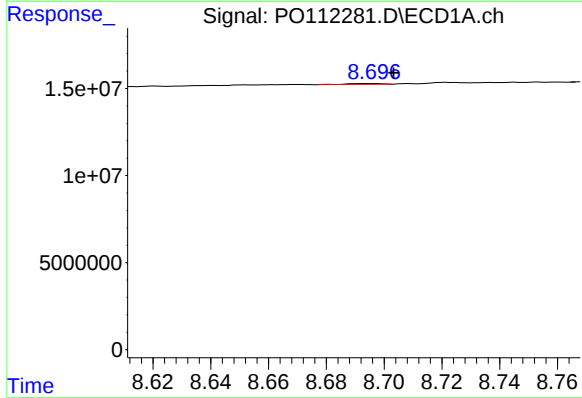


#2 Decachlorobiphenyl

R.T.: 8.696 min
Delta R.T.: -0.007 min
Response: 431547
Conc: 0.06 ng/ml

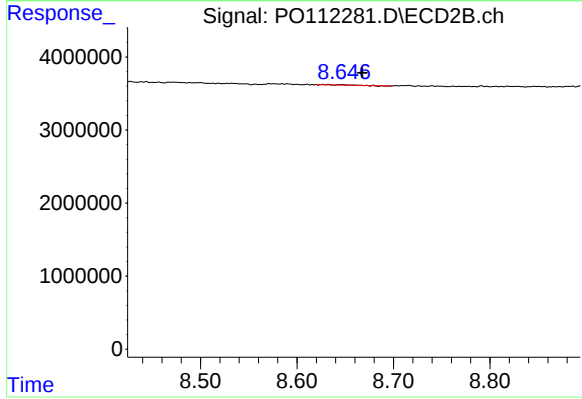

#2 Decachlorobiphenyl


R.T.: 8.647 min
Delta R.T.: -0.021 min
Response: 64807
Conc: 0.04 ng/ml

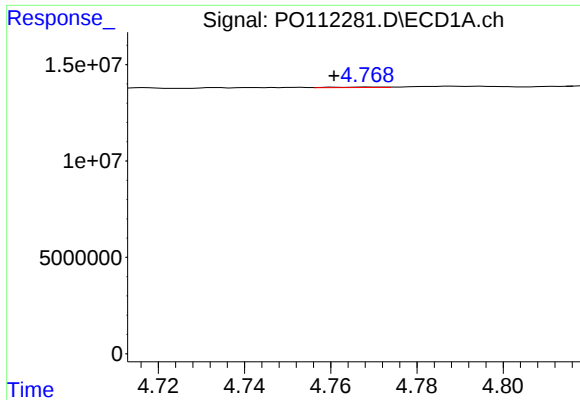

#3 AR-1016-1


R.T.: 4.769 min
Delta R.T.: 0.008 min
Response: 206927
Conc: 0.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

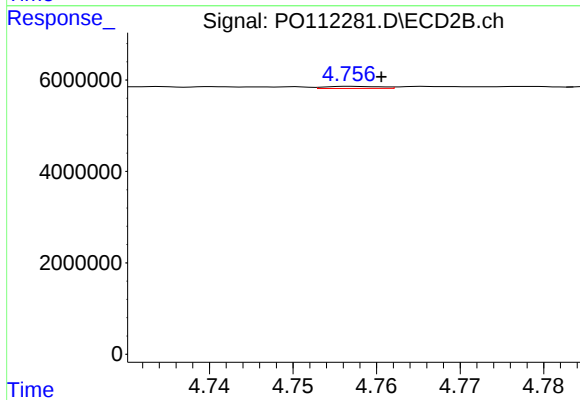


#3 AR-1016-1

R.T.: 4.757 min
Delta R.T.: -0.004 min
Response: 210403
Conc: 0.94 ng/ml

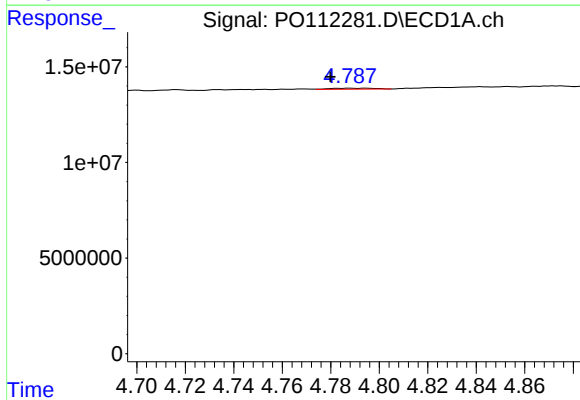


#4 AR-1016-2

R.T.: 4.788 min
Delta R.T.: 0.008 min
Response: 655451
Conc: 1.32 ng/ml

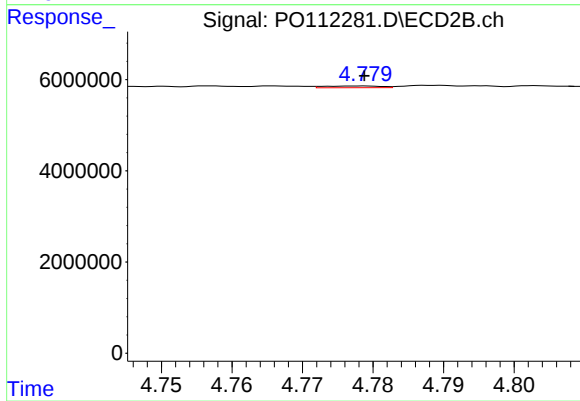

#4 AR-1016-2


R.T.: 4.779 min
Delta R.T.: 0.000 min
Response: 216587
Conc: 0.66 ng/ml

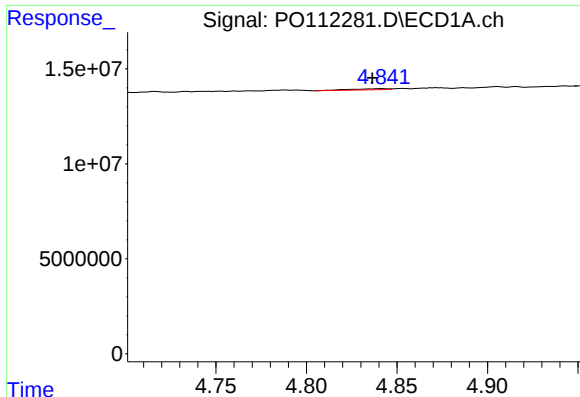

#5 AR-1016-3


R.T.: 4.842 min
Delta R.T.: 0.006 min
Response: 934341
Conc: 2.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

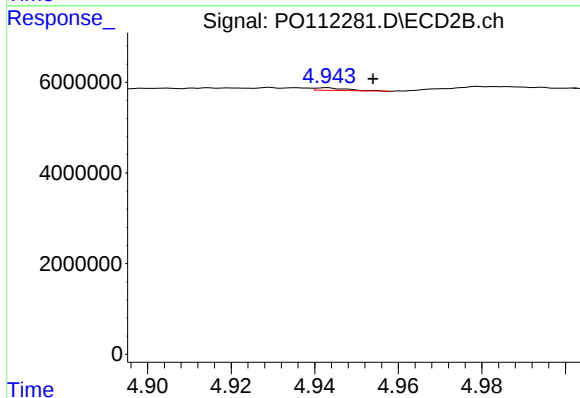


#5 AR-1016-3

R.T.: 4.943 min
Delta R.T.: -0.011 min
Response: 295591
Conc: 1.74 ng/ml

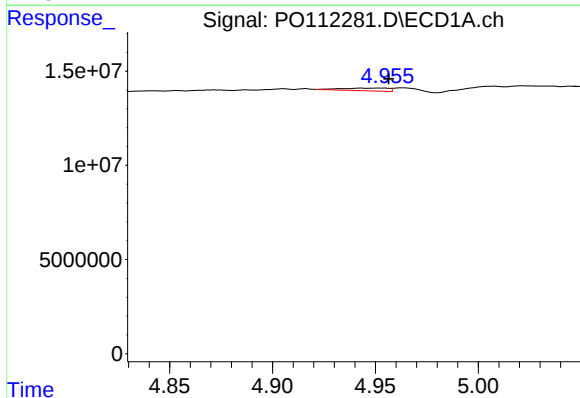


#6 AR-1016-4

R.T.: 4.952 min
Delta R.T.: -0.004 min
Response: 2287648
Conc: 8.91 ng/ml

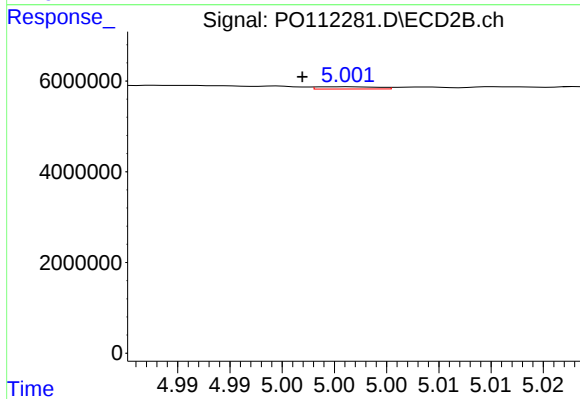

#6 AR-1016-4


R.T.: 5.002 min
Delta R.T.: 0.005 min
Response: 196532
Conc: 1.43 ng/ml

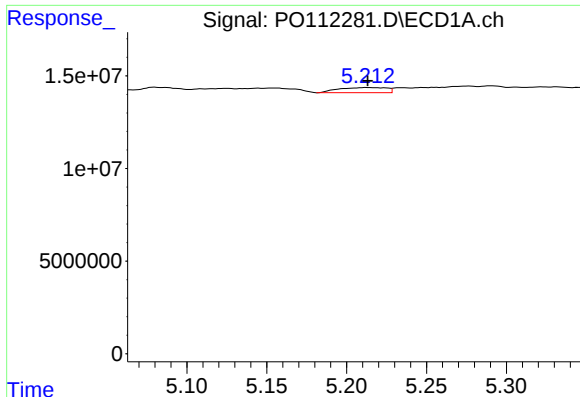

#7 AR-1016-5


R.T.: 5.213 min
Delta R.T.: 0.000 min
Response: 5770687
Conc: 21.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

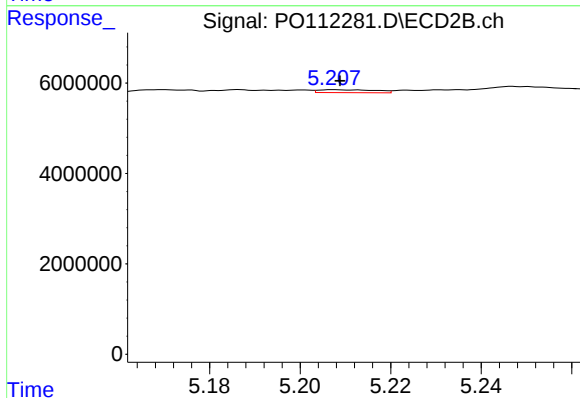


#7 AR-1016-5

R.T.: 5.207 min
Delta R.T.: -0.001 min
Response: 561394
Conc: 3.26 ng/ml

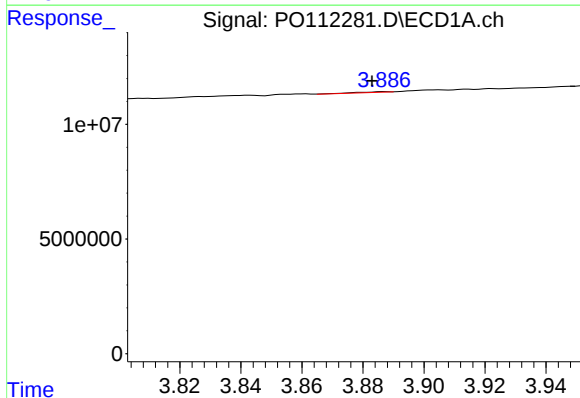


#8 AR-1221-1

R.T.: 3.887 min
Delta R.T.: 0.004 min
Response: 185175
Conc: 1.59 ng/ml

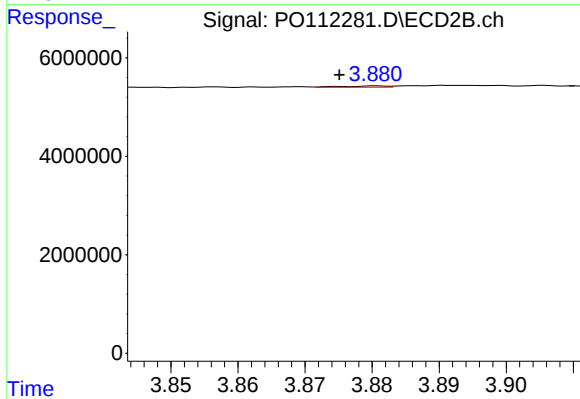

#8 AR-1221-1


R.T.: 3.881 min
Delta R.T.: 0.005 min
Response: 127954
Conc: 1.55 ng/ml

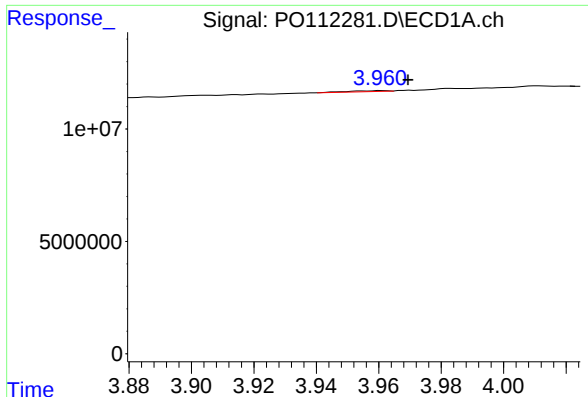

#9 AR-1221-2


R.T.: 3.961 min
Delta R.T.: -0.008 min
Response: 350576
Conc: 4.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

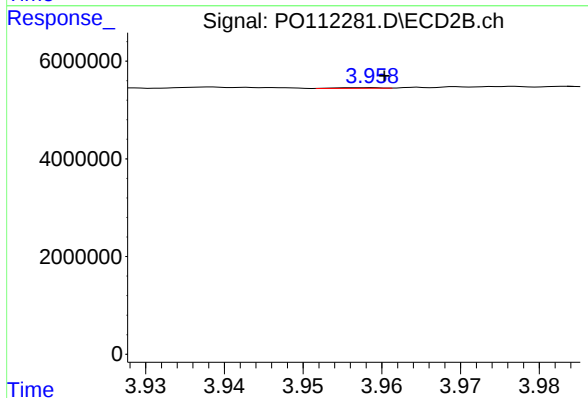


#9 AR-1221-2

R.T.: 3.958 min
Delta R.T.: -0.002 min
Response: 53398
Conc: 0.90 ng/ml

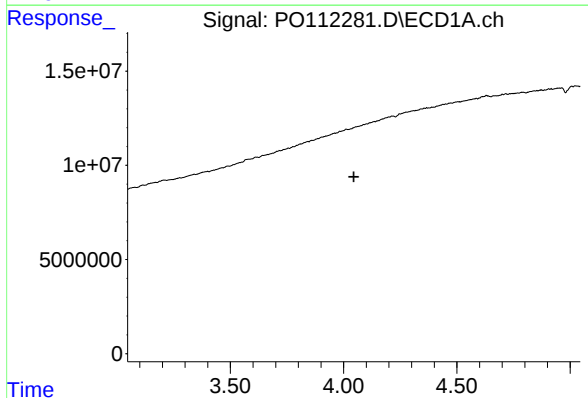


#10 AR-1221-3

R.T.: 4.102 min
Delta R.T.: 0.057 min
Response: -719070
Conc: N.D.

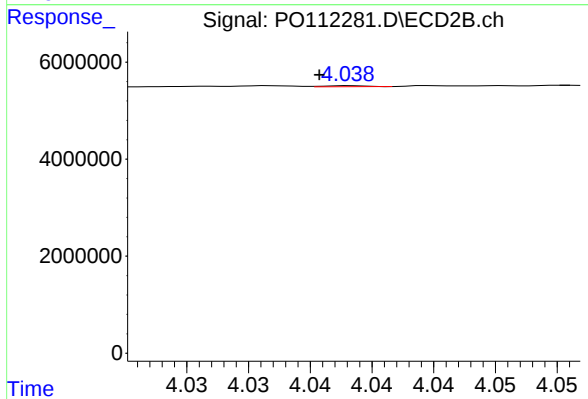

#10 AR-1221-3


R.T.: 4.038 min
Delta R.T.: 0.003 min
Response: 48569
Conc: 0.26 ng/ml

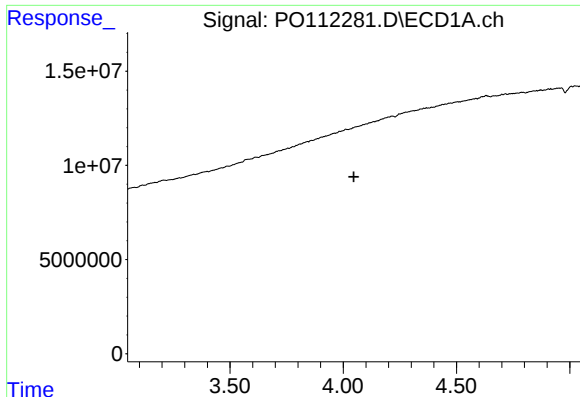

#11 AR-1232-1


R.T.: 4.102 min
Delta R.T.: 0.055 min
Response: -719070
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

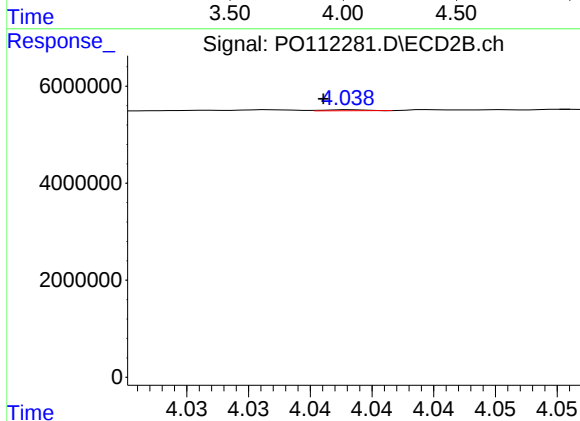


#11 AR-1232-1

R.T.: 4.038 min
Delta R.T.: 0.002 min
Response: 48569
Conc: 0.32 ng/ml

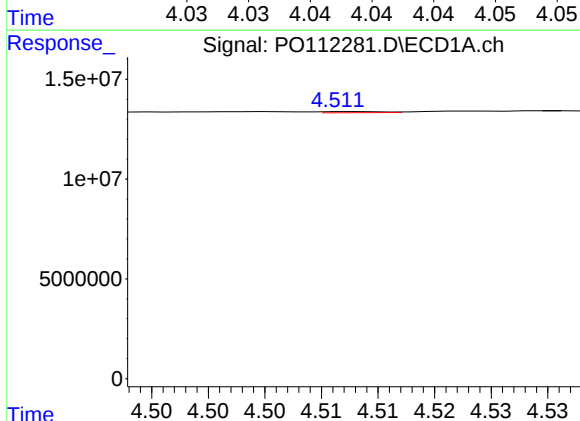


#12 AR-1232-2

R.T.: 4.513 min
Delta R.T.: -0.026 min
Response: 216942
Conc: 1.91 ng/ml

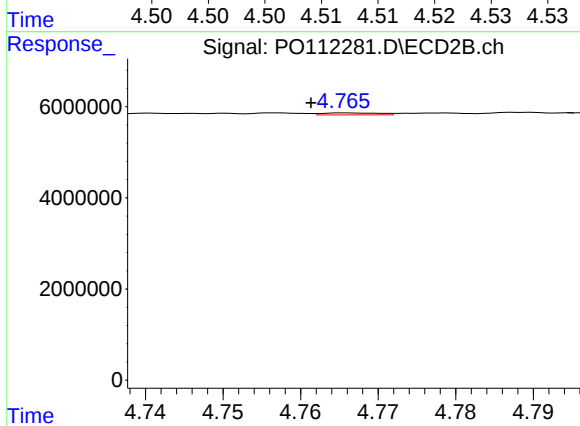

#12 AR-1232-2


R.T.: 4.766 min
Delta R.T.: 0.004 min
Response: 217693
Conc: 1.42 ng/ml

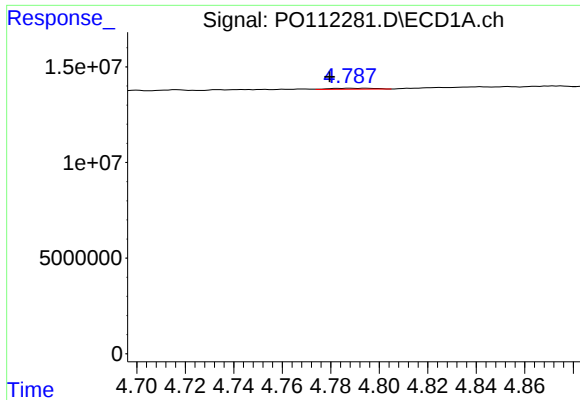

#13 AR-1232-3


R.T.: 4.788 min
Delta R.T.: 0.008 min
Response: 655451
Conc: 2.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

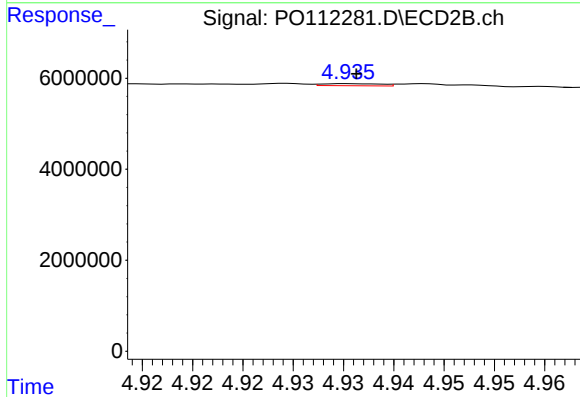


#13 AR-1232-3

R.T.: 4.935 min
Delta R.T.: 0.000 min
Response: 188057
Conc: 2.49 ng/ml

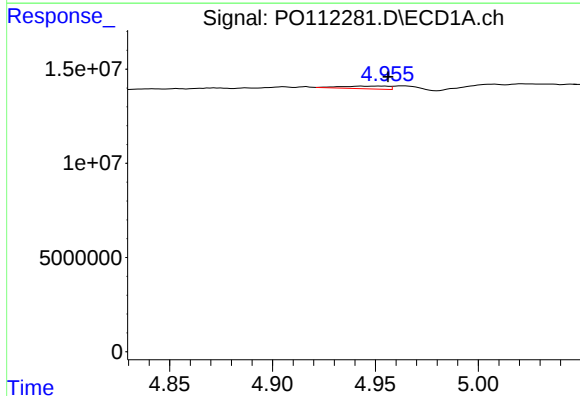


#14 AR-1232-4

R.T.: 4.952 min
Delta R.T.: -0.004 min
Response: 2287648
Conc: 20.01 ng/ml

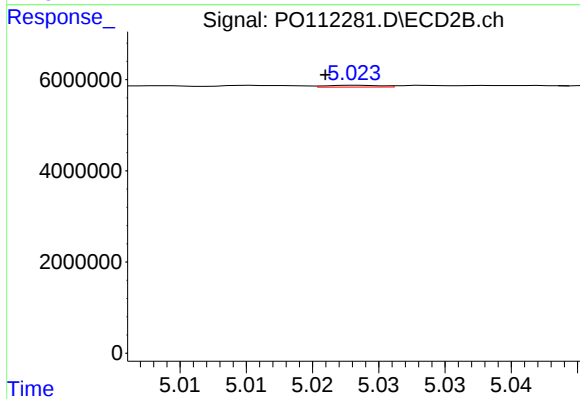

#14 AR-1232-4


R.T.: 5.023 min
Delta R.T.: 0.002 min
Response: 118356
Conc: 1.79 ng/ml

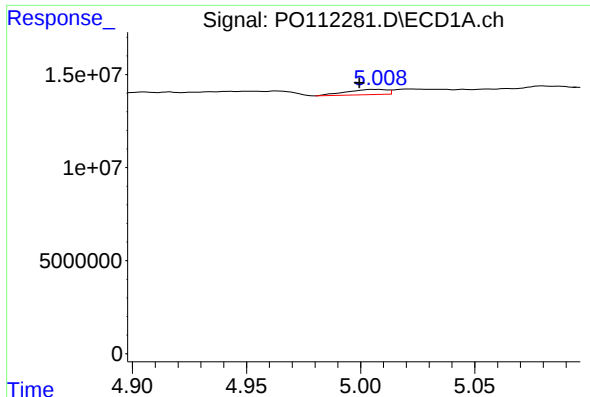

#15 AR-1232-5


R.T.: 5.007 min
Delta R.T.: 0.008 min
Response: 3426259
Conc: 46.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

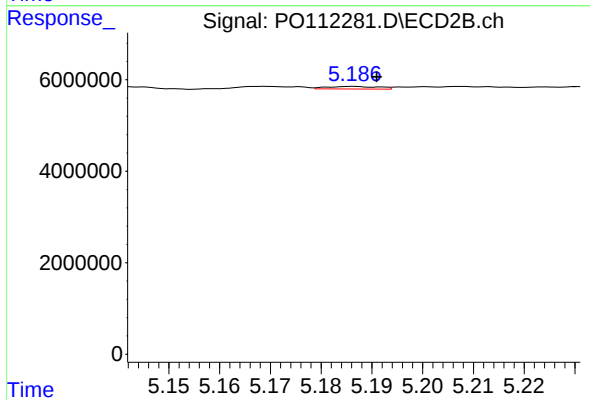


#15 AR-1232-5

R.T.: 5.186 min
Delta R.T.: -0.005 min
Response: 407869
Conc: 5.49 ng/ml

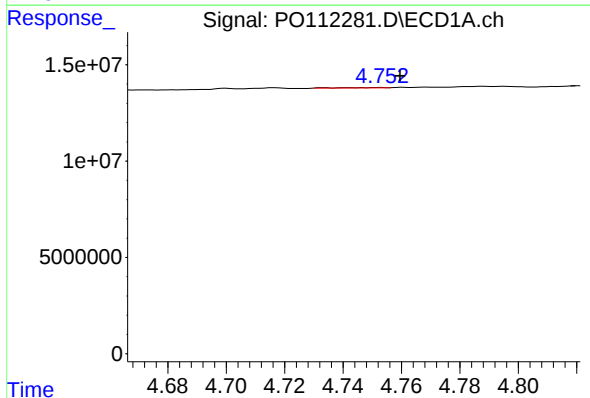


#16 AR-1242-1

R.T.: 4.753 min
Delta R.T.: -0.007 min
Response: 244154
Conc: 0.84 ng/ml

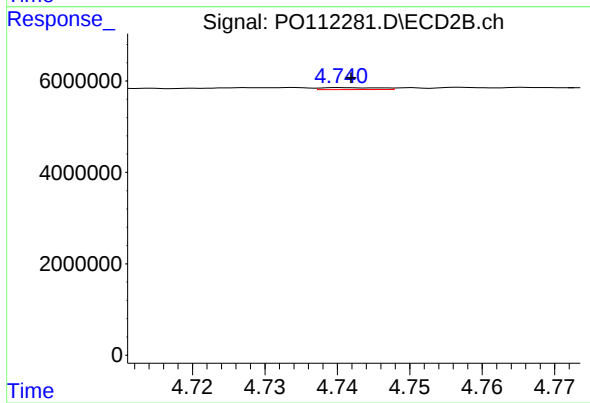

#16 AR-1242-1


R.T.: 4.741 min
Delta R.T.: -0.001 min
Response: 245811
Conc: 1.27 ng/ml

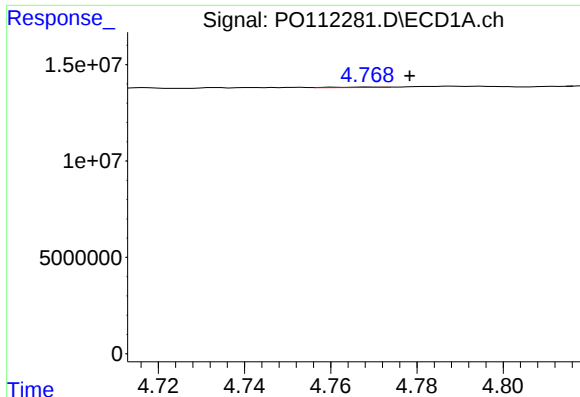

#17 AR-1242-2


R.T.: 4.769 min
Delta R.T.: -0.010 min
Response: 206927
Conc: 0.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

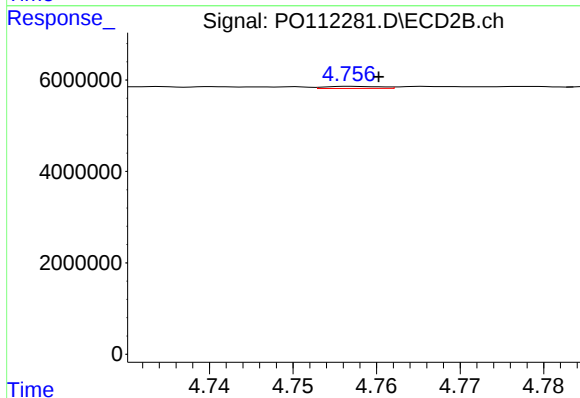


#17 AR-1242-2

R.T.: 4.757 min
Delta R.T.: -0.003 min
Response: 210403
Conc: 0.74 ng/ml

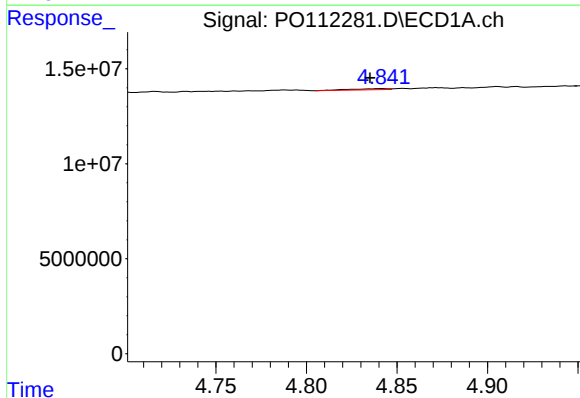


#18 AR-1242-3

R.T.: 4.842 min
Delta R.T.: 0.007 min
Response: 934341
Conc: 3.41 ng/ml

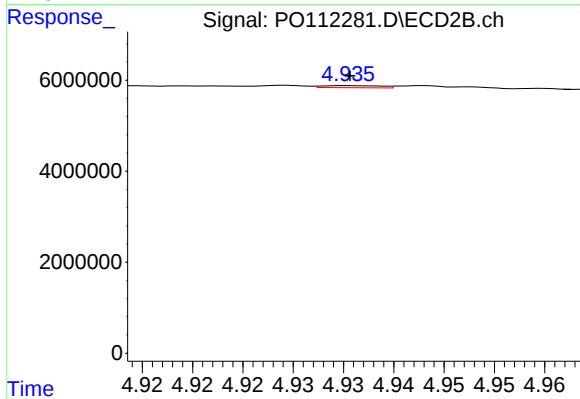

#18 AR-1242-3


R.T.: 4.935 min
Delta R.T.: 0.000 min
Response: 188057
Conc: 1.29 ng/ml

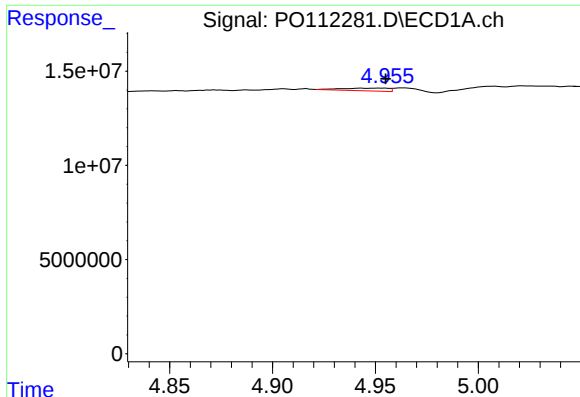

#19 AR-1242-4


R.T.: 4.952 min
Delta R.T.: -0.003 min
Response: 2287648
Conc: 10.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

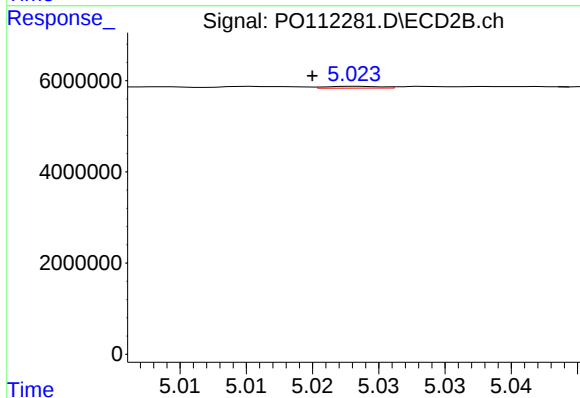


#19 AR-1242-4

R.T.: 5.023 min
Delta R.T.: 0.003 min
Response: 118356
Conc: 0.83 ng/ml

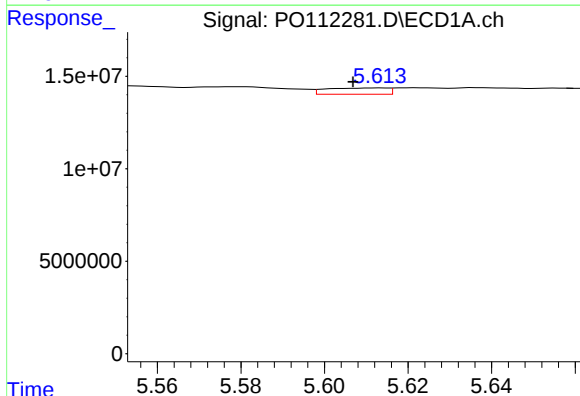


#20 AR-1242-5

R.T.: 5.613 min
Delta R.T.: 0.006 min
Response: 3431865
Conc: 16.21 ng/ml

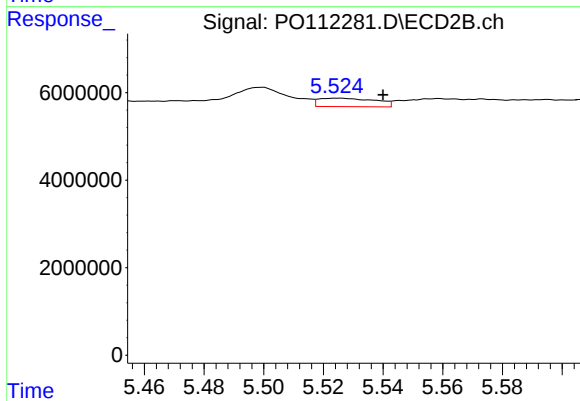

#20 AR-1242-5


R.T.: 5.524 min
Delta R.T.: -0.016 min
Response: 2551230
Conc: 14.04 ng/ml

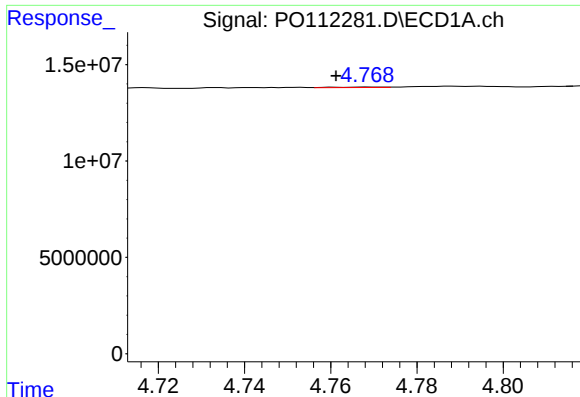

#21 AR-1248-1


R.T.: 4.769 min
Delta R.T.: 0.008 min
Response: 206927
Conc: 0.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

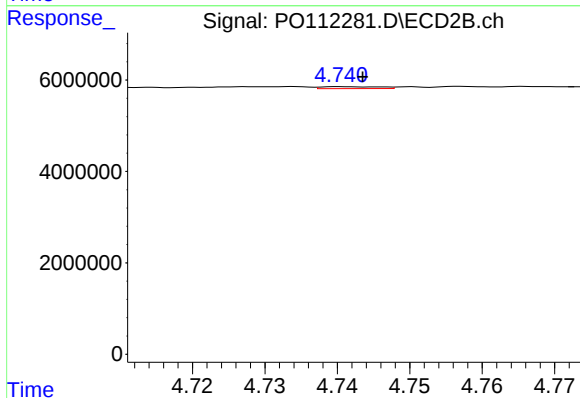


#21 AR-1248-1

R.T.: 4.741 min
Delta R.T.: -0.003 min
Response: 245811
Conc: 1.59 ng/ml

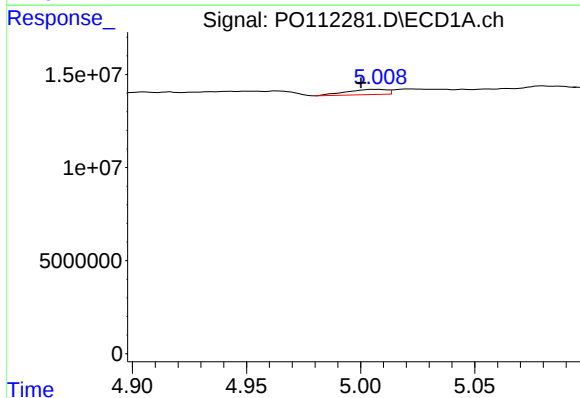


#22 AR-1248-2

R.T.: 5.007 min
Delta R.T.: 0.007 min
Response: 3426259
Conc: 11.11 ng/ml

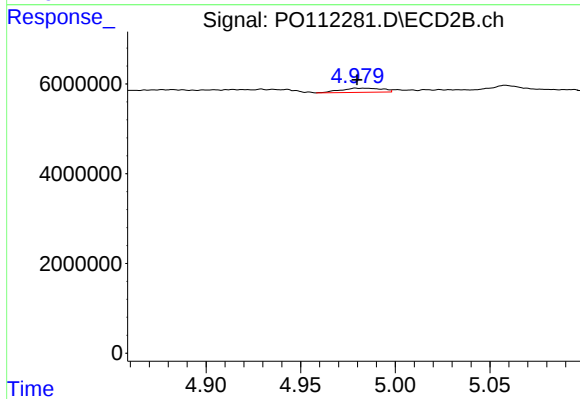

#22 AR-1248-2


R.T.: 4.979 min
Delta R.T.: 0.000 min
Response: 1407527
Conc: 6.84 ng/ml

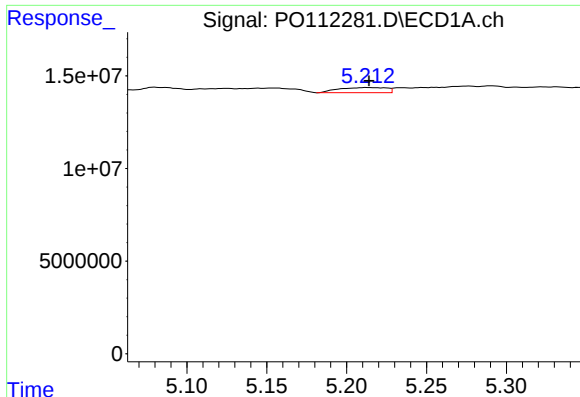

#23 AR-1248-3


R.T.: 5.213 min
Delta R.T.: -0.001 min
Response: 5770687
Conc: 14.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

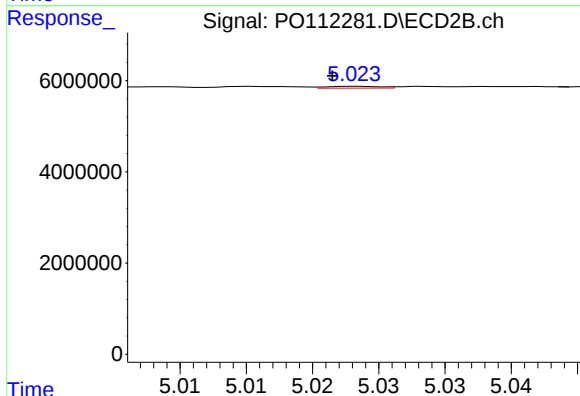


#23 AR-1248-3

R.T.: 5.023 min
Delta R.T.: 0.002 min
Response: 118356
Conc: 0.55 ng/ml

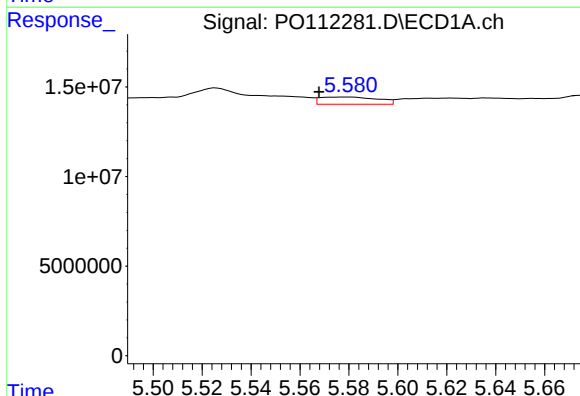


#24 AR-1248-4

R.T.: 5.580 min
Delta R.T.: 0.012 min
Response: 6578002
Conc: 11.40 ng/ml

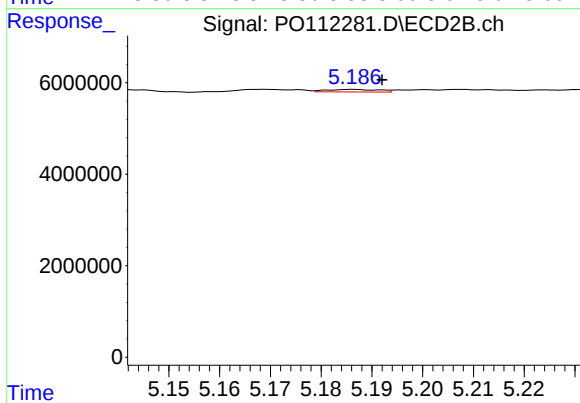

#24 AR-1248-4


R.T.: 5.186 min
Delta R.T.: -0.006 min
Response: 407869
Conc: 1.58 ng/ml

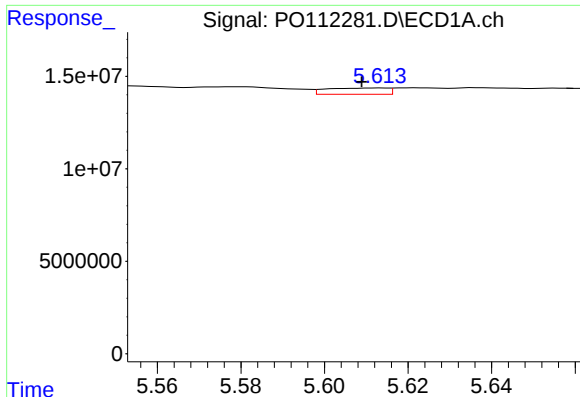

#25 AR-1248-5


R.T.: 5.613 min
Delta R.T.: 0.004 min
Response: 3431865
Conc: 8.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

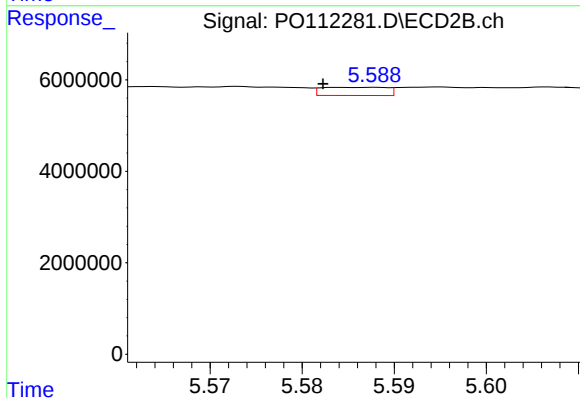


#25 AR-1248-5

R.T.: 5.588 min
Delta R.T.: 0.006 min
Response: 876912
Conc: 3.50 ng/ml

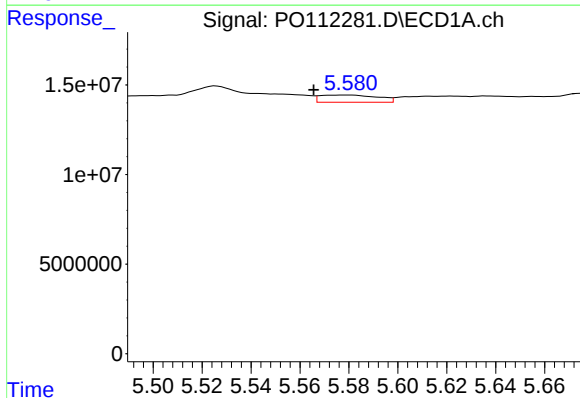


#26 AR-1254-1

R.T.: 5.580 min
Delta R.T.: 0.014 min
Response: 6578002
Conc: 10.69 ng/ml

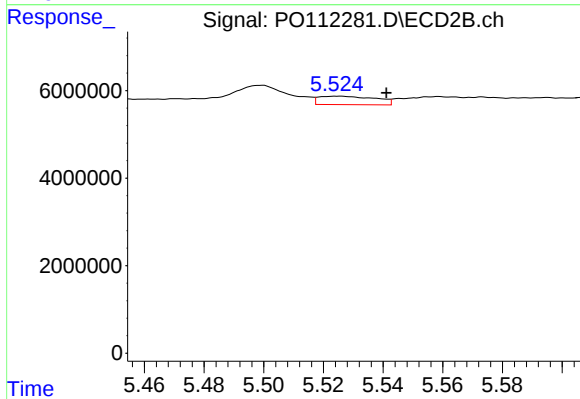

#26 AR-1254-1


R.T.: 5.524 min
Delta R.T.: -0.017 min
Response: 2551230
Conc: 6.69 ng/ml

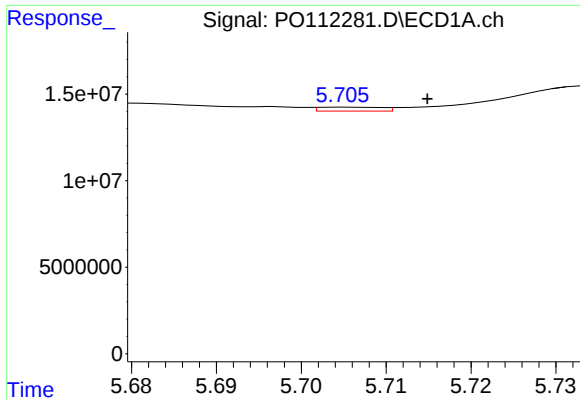

#27 AR-1254-2


R.T.: 5.705 min
Delta R.T.: -0.010 min
Response: 1175626
Conc: 2.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

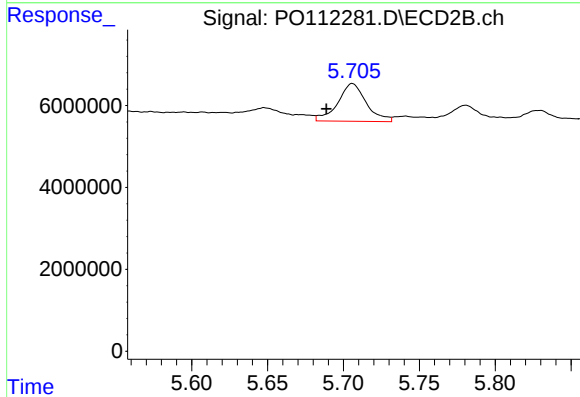


#27 AR-1254-2

R.T.: 5.706 min
Delta R.T.: 0.017 min
Response: 12012292
Conc: 36.20 ng/ml

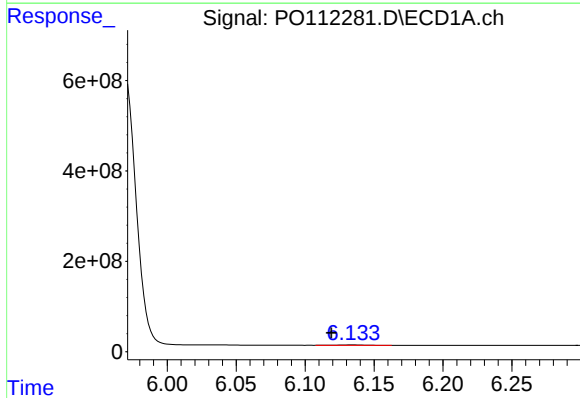


#28 AR-1254-3

R.T.: 6.134 min
Delta R.T.: 0.015 min
Response: 9209413
Conc: 10.97 ng/ml

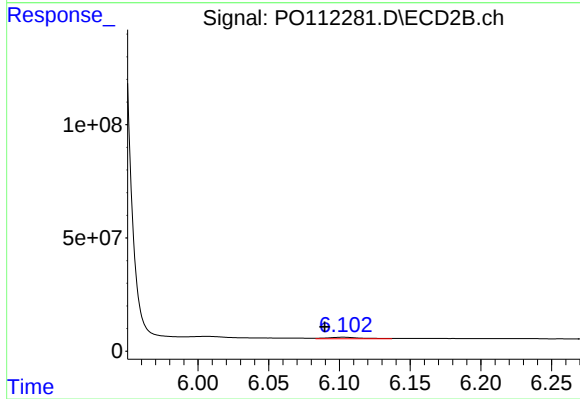

#28 AR-1254-3


R.T.: 6.103 min
Delta R.T.: 0.013 min
Response: 11974724
Conc: 24.84 ng/ml

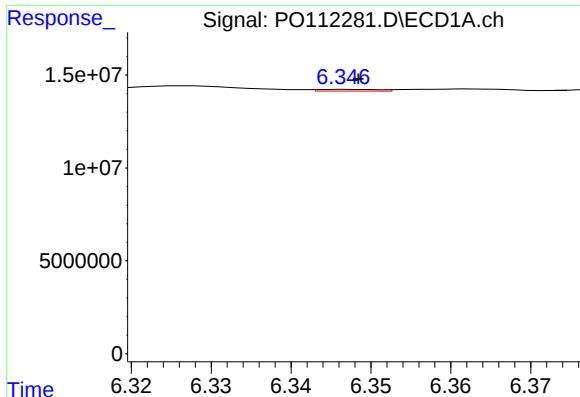

#29 AR-1254-4


R.T.: 6.347 min
Delta R.T.: -0.001 min
Response: 487844
Conc: 1.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

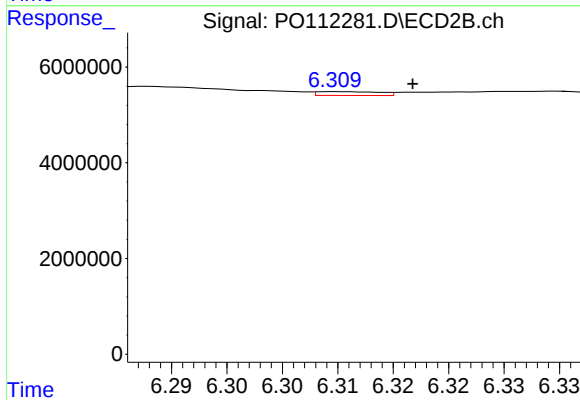


#29 AR-1254-4

R.T.: 6.310 min
Delta R.T.: -0.007 min
Response: 319304
Conc: 1.22 ng/ml

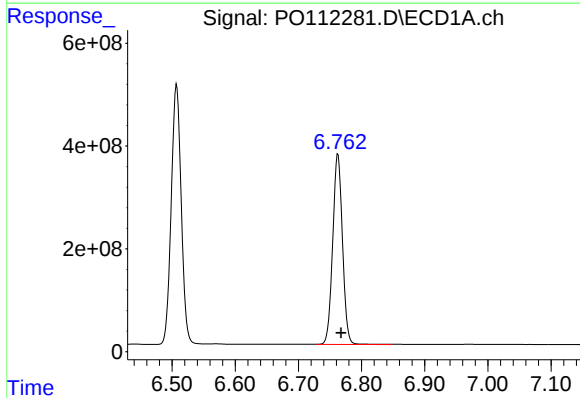


#30 AR-1254-5

R.T.: 6.763 min
Delta R.T.: -0.005 min
Response: 3980511743
Conc: 5143.13 ng/ml

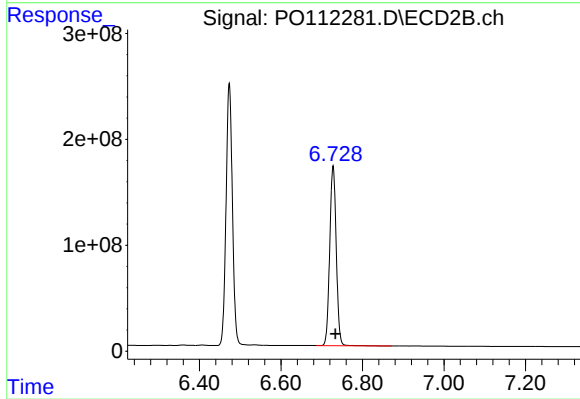

#30 AR-1254-5


R.T.: 6.728 min
Delta R.T.: -0.005 min
Response: 1881851788
Conc: 5280.82 ng/ml

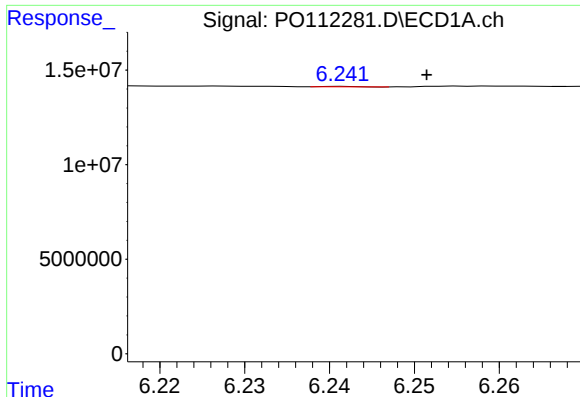

#31 AR-1260-1


R.T.: 6.242 min
Delta R.T.: -0.010 min
Response: 65296
Conc: 0.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

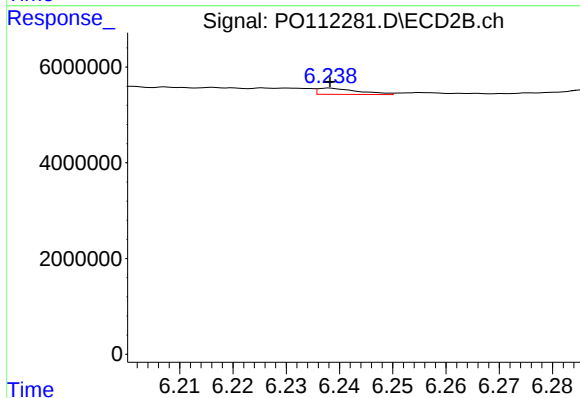


#31 AR-1260-1

R.T.: 6.238 min
Delta R.T.: 0.000 min
Response: 681926
Conc: 2.43 ng/ml

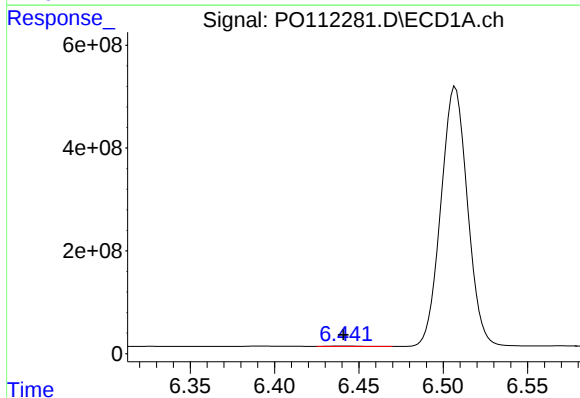


#32 AR-1260-2

R.T.: 6.441 min
Delta R.T.: 0.000 min
Response: 9102724
Conc: 12.33 ng/ml

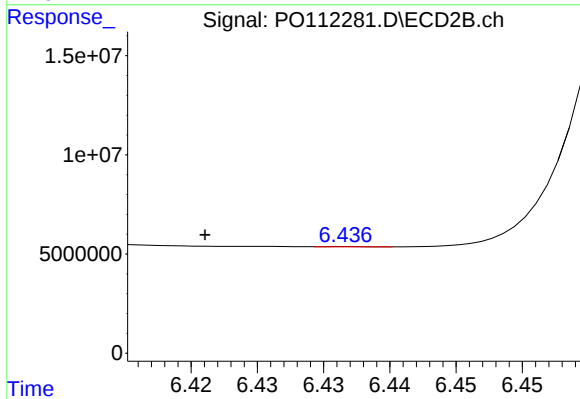

#32 AR-1260-2


R.T.: 6.437 min
Delta R.T.: 0.011 min
Response: 25987
Conc: 0.08 ng/ml

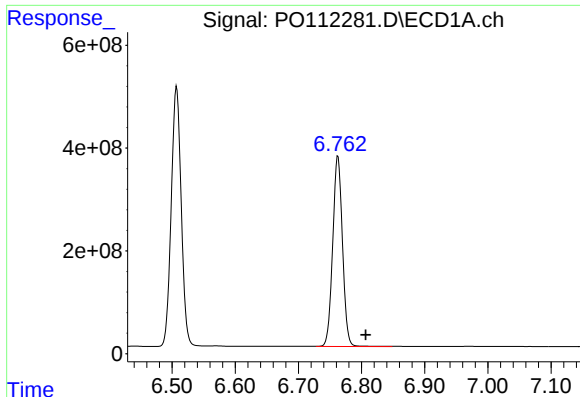

#33 AR-1260-3


R.T.: 6.763 min
Delta R.T.: -0.044 min
Response: 3980511743
Conc: 6072.65 ng/m

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

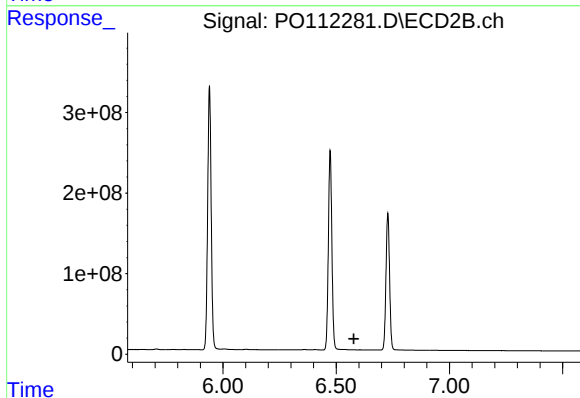


#33 AR-1260-3

R.T.: 6.601 min
Delta R.T.: 0.023 min
Response: -10698
Conc: N.D.

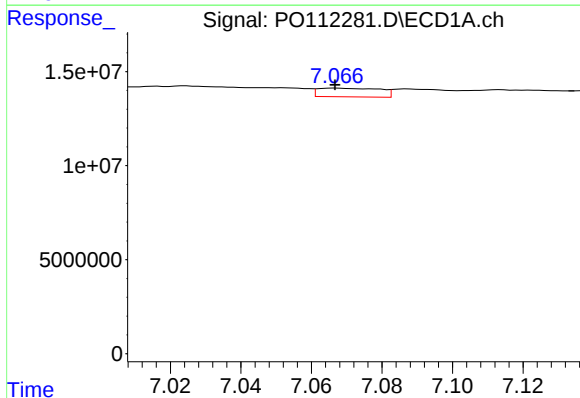


#34 AR-1260-4

R.T.: 7.067 min
Delta R.T.: 0.000 min
Response: 5623154
Conc: 12.92 ng/ml

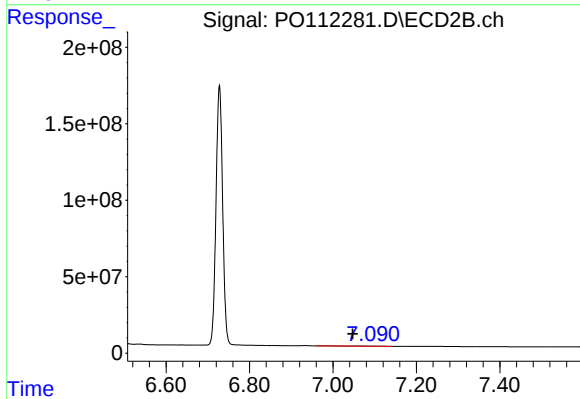

#34 AR-1260-4


R.T.: 6.987 min
Delta R.T.: -0.060 min
Response: 2545728
Conc: 12.69 ng/ml

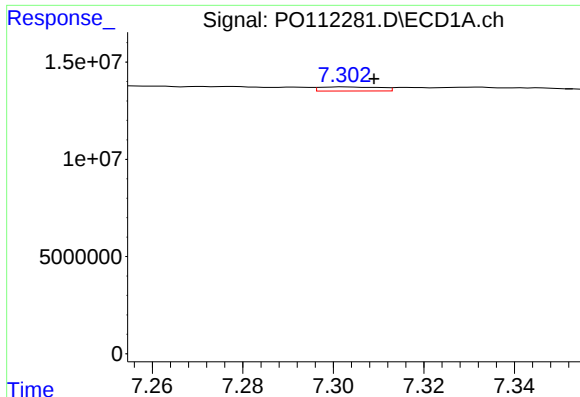

#35 AR-1260-5


R.T.: 7.303 min
Delta R.T.: -0.006 min
Response: 1929190
Conc: 1.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

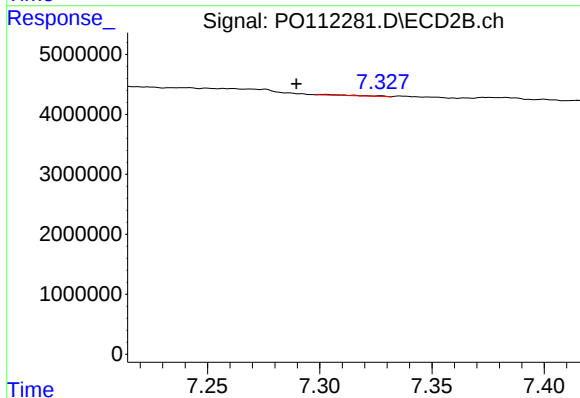


#35 AR-1260-5

R.T.: 7.303 min
Delta R.T.: 0.013 min
Response: 123738
Conc: 0.28 ng/ml

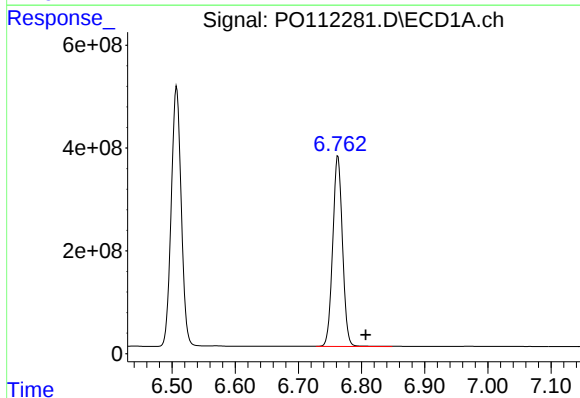


#36 AR-1262-1

R.T.: 6.763 min
Delta R.T.: -0.044 min
Response: 3980511743
Conc: 3896.02 ng/ml

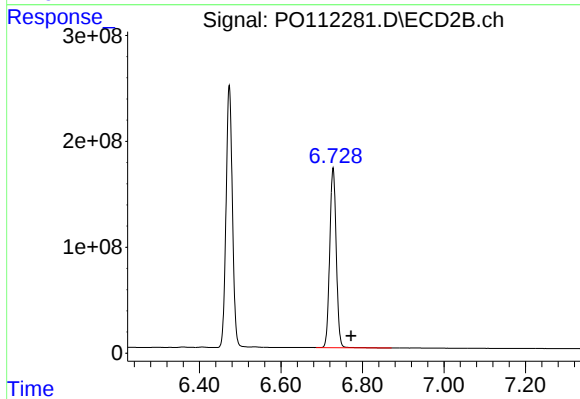

#36 AR-1262-1


R.T.: 6.728 min
Delta R.T.: -0.044 min
Response: 1881851788
Conc: 4620.07 ng/ml

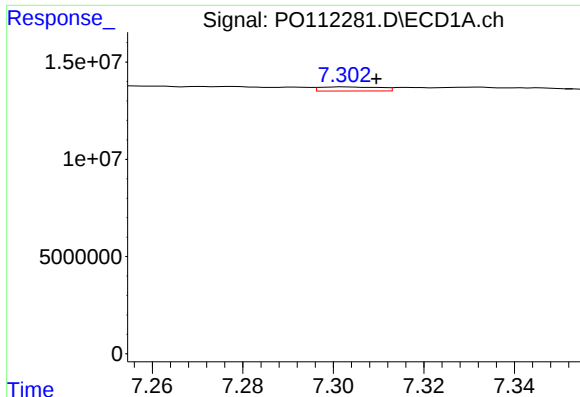

#37 AR-1262-2


R.T.: 7.303 min
Delta R.T.: -0.007 min
Response: 1929190
Conc: 1.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

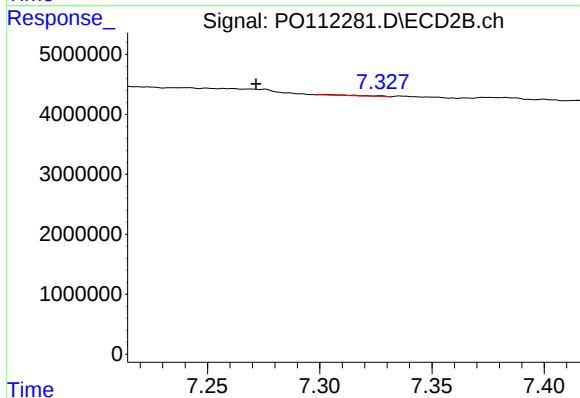


#37 AR-1262-2

R.T.: 7.303 min
Delta R.T.: 0.031 min
Response: 123738
Conc: 0.24 ng/ml

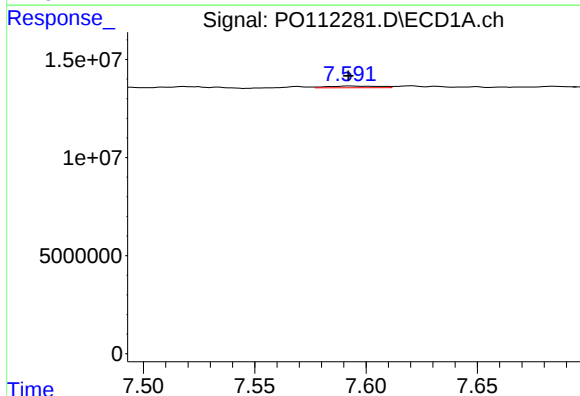


#38 AR-1262-3

R.T.: 7.592 min
Delta R.T.: 0.000 min
Response: 1377837
Conc: 2.15 ng/ml

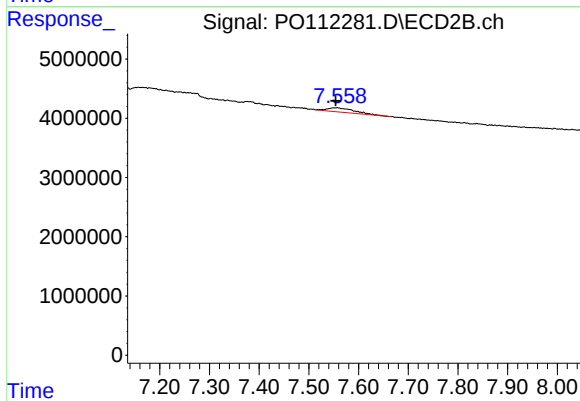

#38 AR-1262-3


R.T.: 7.557 min
Delta R.T.: 0.003 min
Response: 2627603
Conc: 14.64 ng/ml

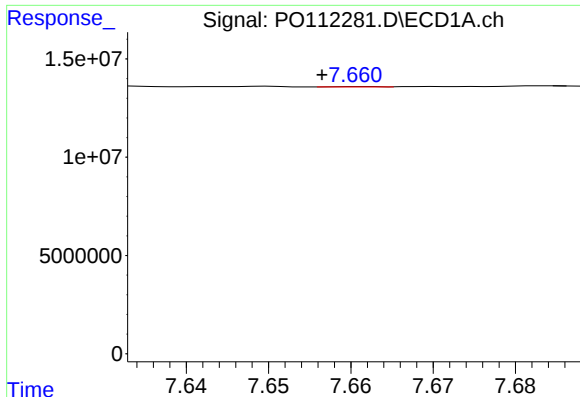

#39 AR-1262-4


R.T.: 7.662 min
Delta R.T.: 0.005 min
Response: 58965
Conc: 0.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

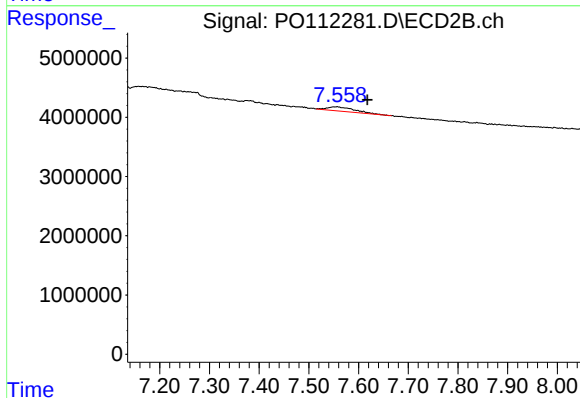


#39 AR-1262-4

R.T.: 7.557 min
Delta R.T.: -0.061 min
Response: 2627603
Conc: 9.03 ng/ml

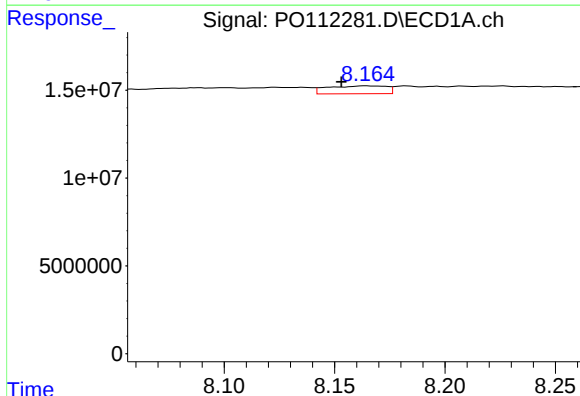


#40 AR-1262-5

R.T.: 8.164 min
Delta R.T.: 0.011 min
Response: 8391955
Conc: 18.73 ng/ml

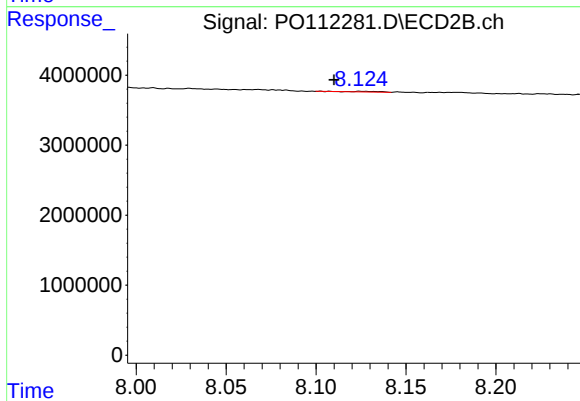

#40 AR-1262-5


R.T.: 8.125 min
Delta R.T.: 0.015 min
Response: 101137
Conc: 0.96 ng/ml

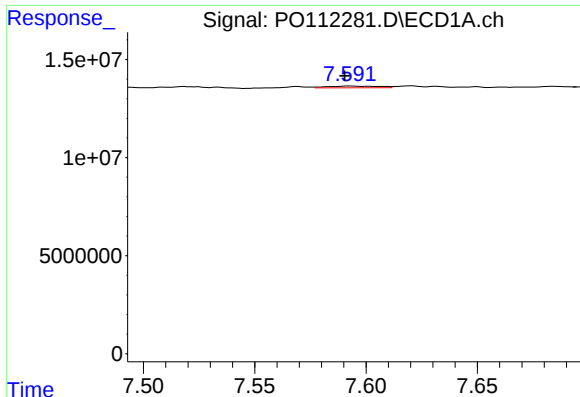

#41 AR-1268-1


R.T.: 7.592 min
Delta R.T.: 0.002 min
Response: 1377837
Conc: 0.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

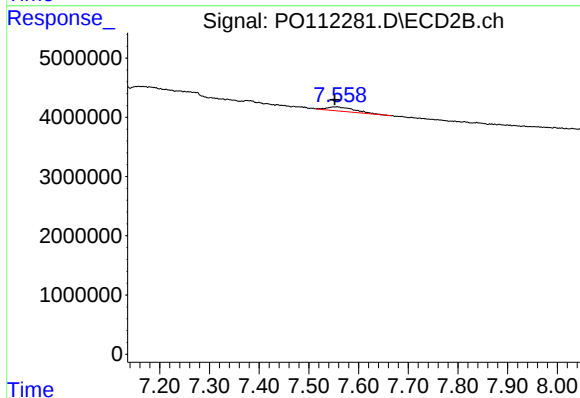


#41 AR-1268-1

R.T.: 7.557 min
Delta R.T.: 0.005 min
Response: 2627603
Conc: 5.35 ng/ml

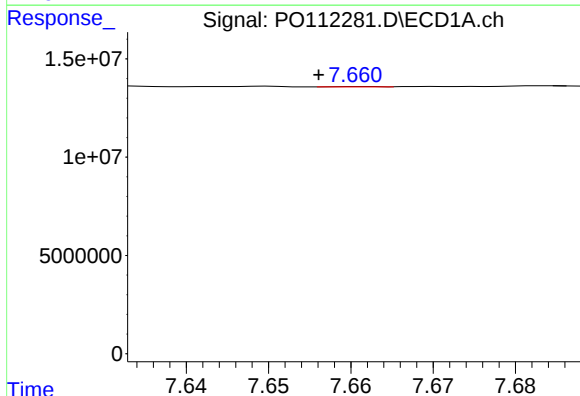


#42 AR-1268-2

R.T.: 7.662 min
Delta R.T.: 0.006 min
Response: 58965
Conc: 0.04 ng/ml

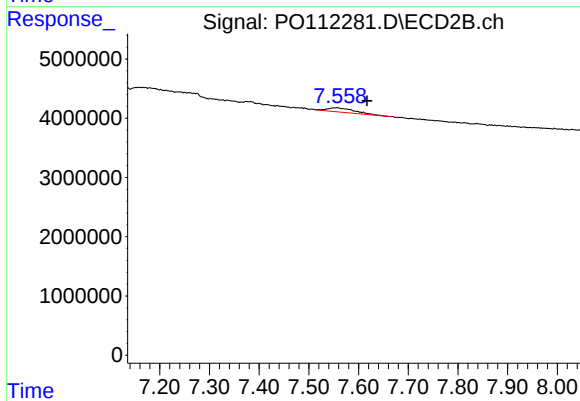

#42 AR-1268-2


R.T.: 7.557 min
Delta R.T.: -0.060 min
Response: 2627603
Conc: 6.30 ng/ml

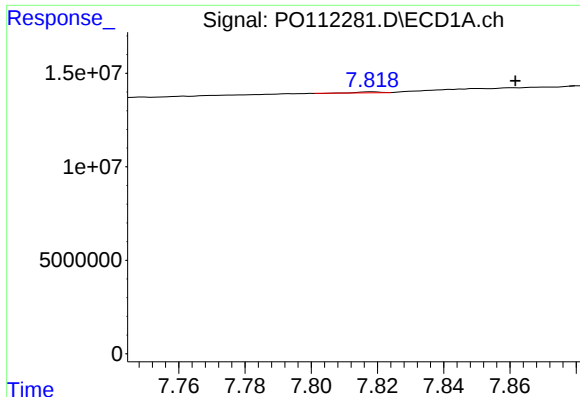

#43 AR-1268-3


R.T.: 7.818 min
Delta R.T.: -0.043 min
Response: 219678
Conc: 0.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

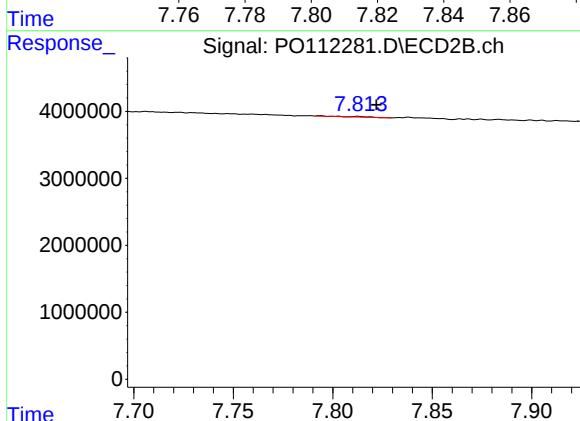


#43 AR-1268-3

R.T.: 7.813 min
Delta R.T.: -0.009 min
Response: 76874
Conc: 0.24 ng/ml

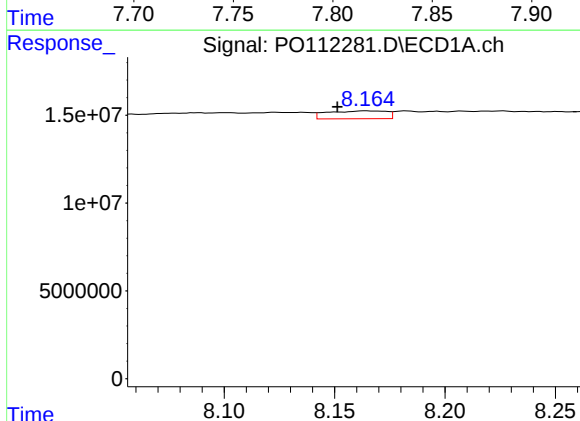


#44 AR-1268-4

R.T.: 8.164 min
Delta R.T.: 0.013 min
Response: 8391955
Conc: 17.47 ng/ml

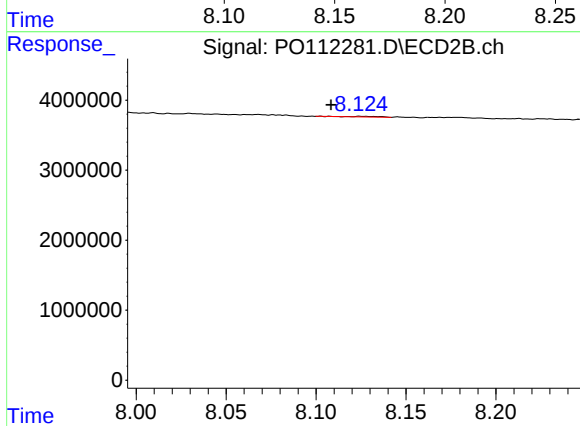

#44 AR-1268-4


R.T.: 8.125 min
Delta R.T.: 0.017 min
Response: 101137
Conc: 0.91 ng/ml

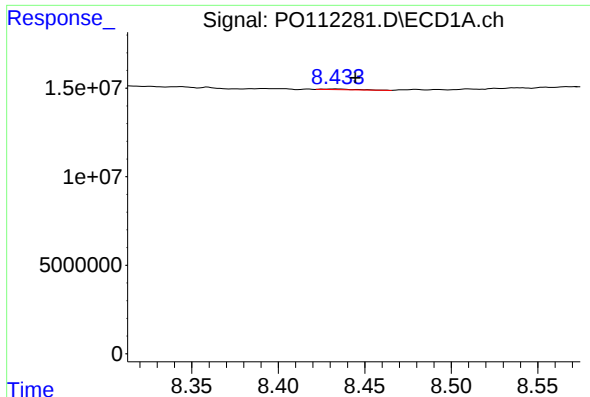

#45 AR-1268-5

R.T.: 8.433 min
Delta R.T.: -0.011 min
Response: 495364
Conc: 0.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

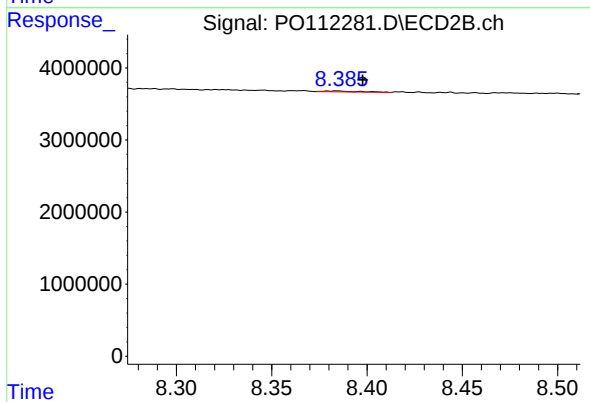

#45 AR-1268-5

R.T.: 8.384 min
Delta R.T.: -0.013 min
Response: 153498
Conc: 0.21 ng/ml