

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0071618\
Data File : P0046743.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Jul 2018 12:50
Operator : SM/SJ
Sample : J3948-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-ST-PH4-AREA

Manual Integrations
APPROVED

Sohil
7/17/2018 4:25:30 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 14:24:18 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.197	3.521	3290470	3735708	13.769m	17.588 #
2) SA Decachlor...	9.721	8.449	2901775	2734302	15.224m	14.096

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0071618\
Data File : P0046743.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Jul 2018 12:50
Operator : SM/SJ
Sample : J3948-03
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-ST-PH4-AREA


Manual Integrations
APPROVED

Sohil
7/17/2018 4:25:30 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 14:24:18 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

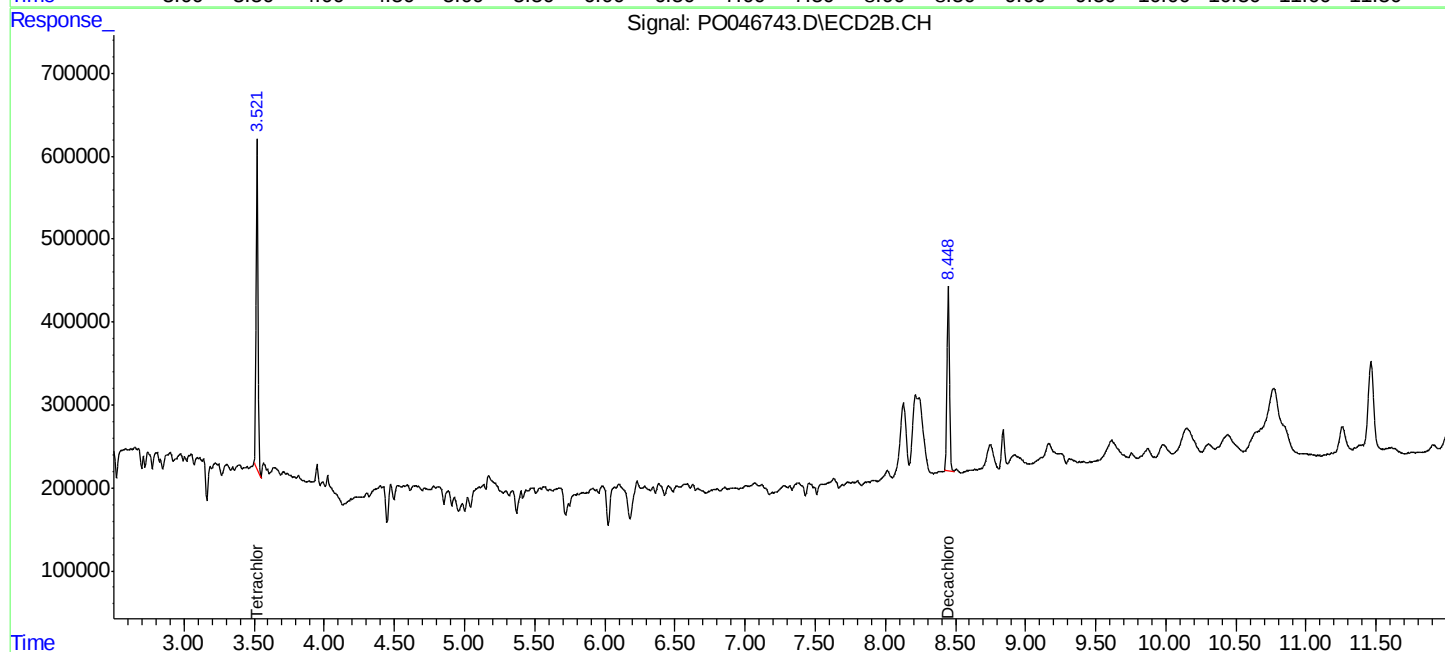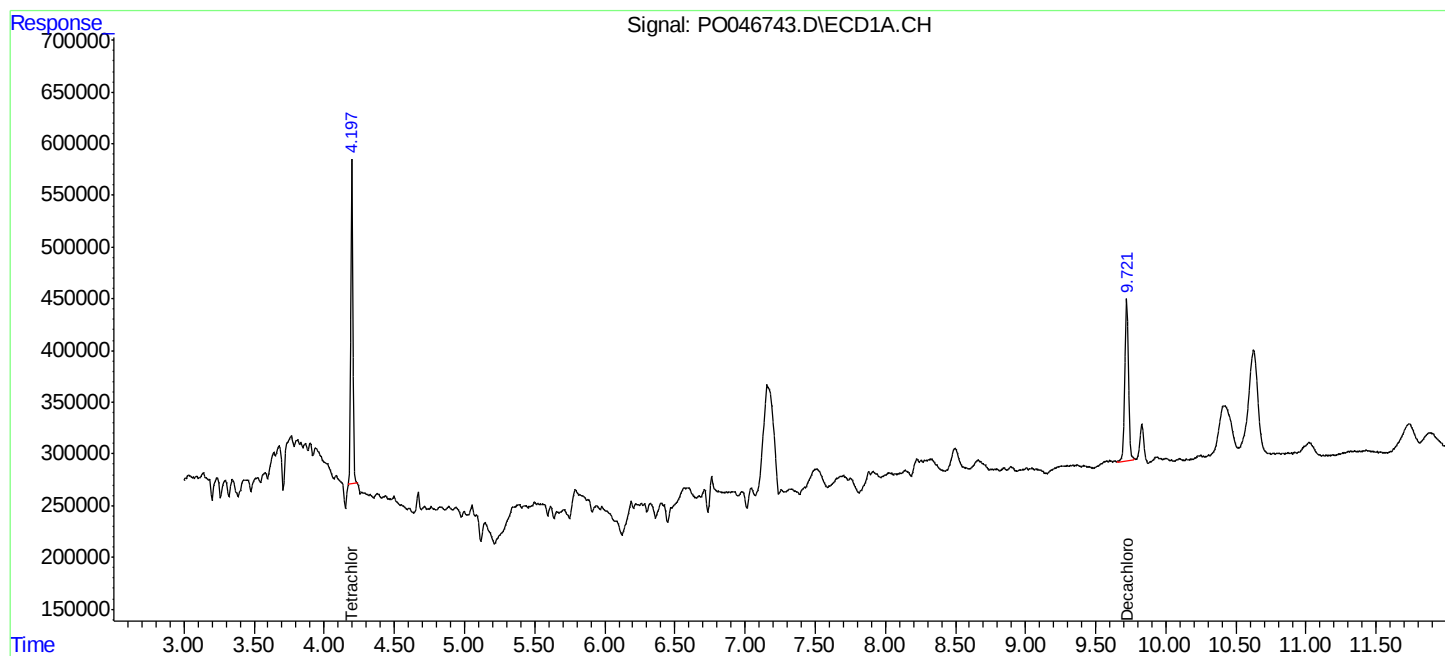

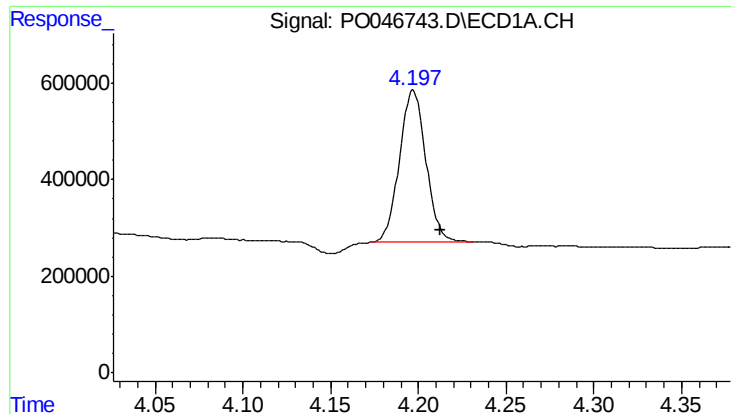


#1 Tetrachloro-m-xylene

R.T.: 4.197 min
Delta R.T.: -0.016 min
Response: 3290470
Conc: 13.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
2018-NYSEG-CLARK-ST-PH4-AREA


Manual Integrations
APPROVED

Sohil
7/17/2018 4:25:30 PM

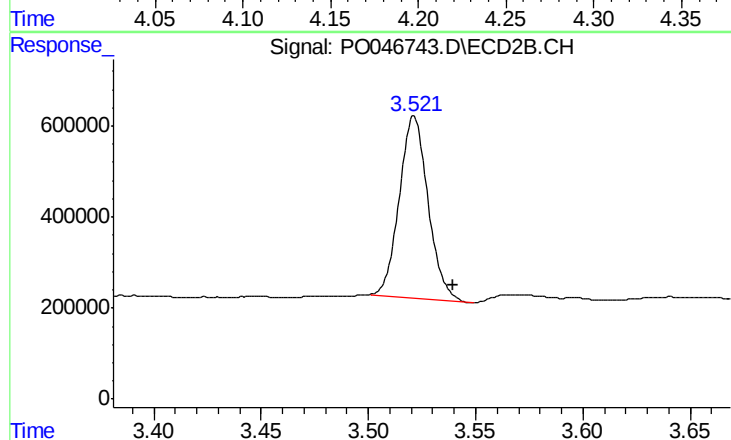


#1 Tetrachloro-m-xylene

R.T.: 3.521 min
Delta R.T.: -0.018 min
Response: 3735708
Conc: 17.59 ng/ml

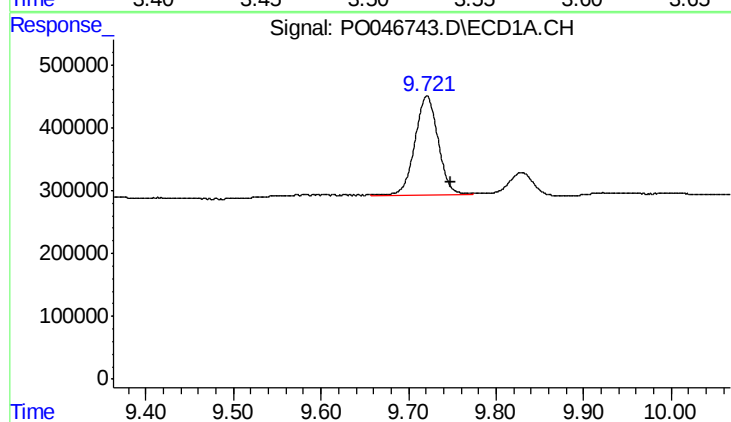

#2 Decachlorobiphenyl

R.T.: 9.721 min
Delta R.T.: -0.027 min
Response: 2901775
Conc: 15.22 ng/ml m

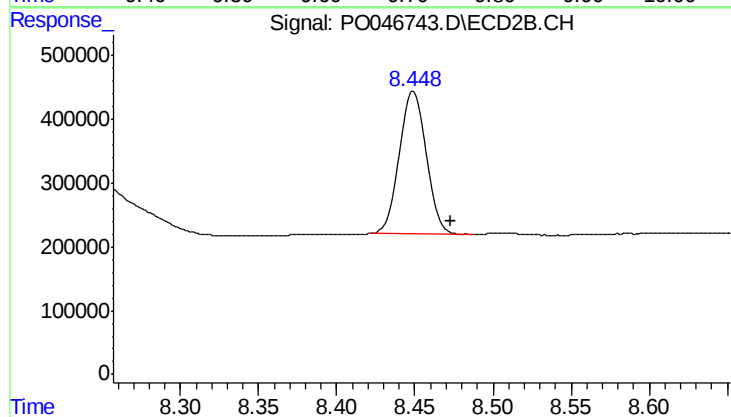

#2 Decachlorobiphenyl

R.T.: 8.449 min
Delta R.T.: -0.024 min
Response: 2734302
Conc: 14.10 ng/ml