

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0071618\
 Data File : P0046756.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Jul 2018 16:17
 Operator : SM/SJ
 Sample : J4009-01 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 A403672

Manual Integrations
 APPROVED

Sohil
 7/17/2018 4:25:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 11:45:35 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 09 15:27:34 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.197	3.524	322942	347115	1.351m	1.634m
2) SA Decachlor...	9.720	8.478	328128	28474	1.722m	0.147m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0071618\
Data File : P0046756.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Jul 2018 16:17
Operator : SM/SJ
Sample : J4009-01 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
A403672


Manual Integrations
APPROVED

Sohil
7/17/2018 4:25:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 11:45:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

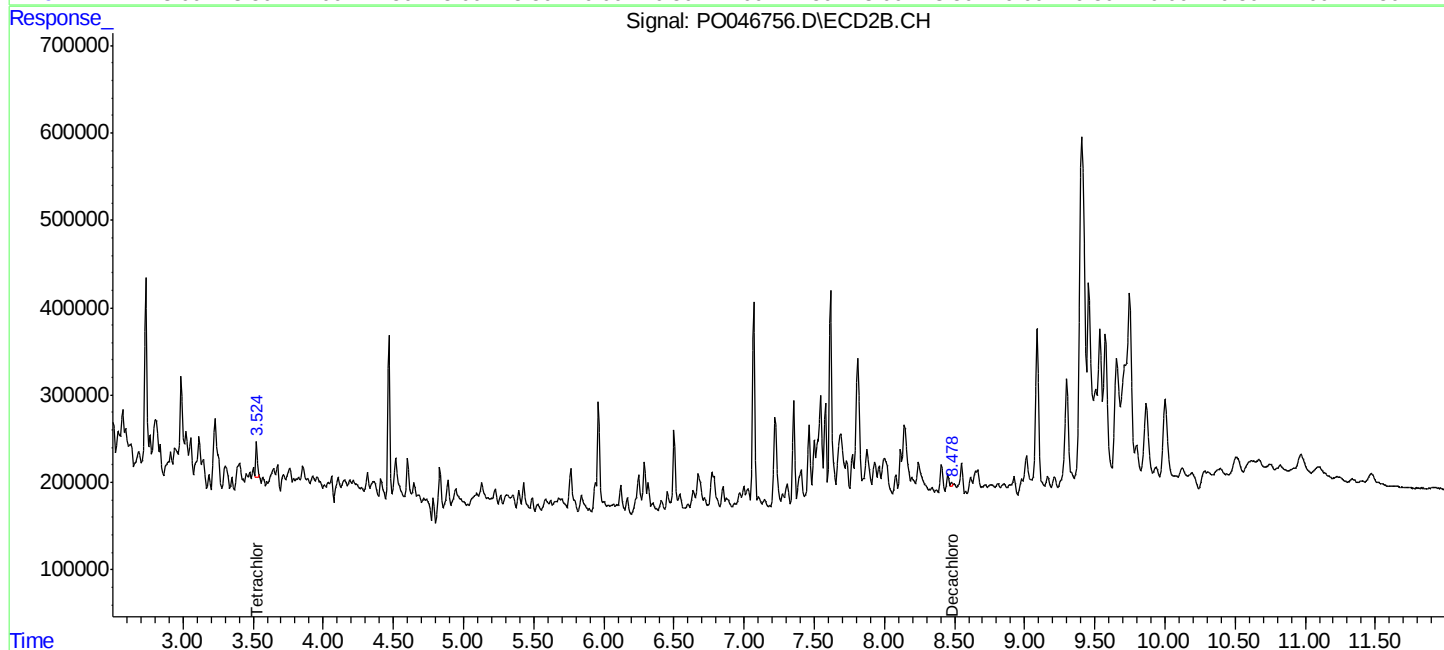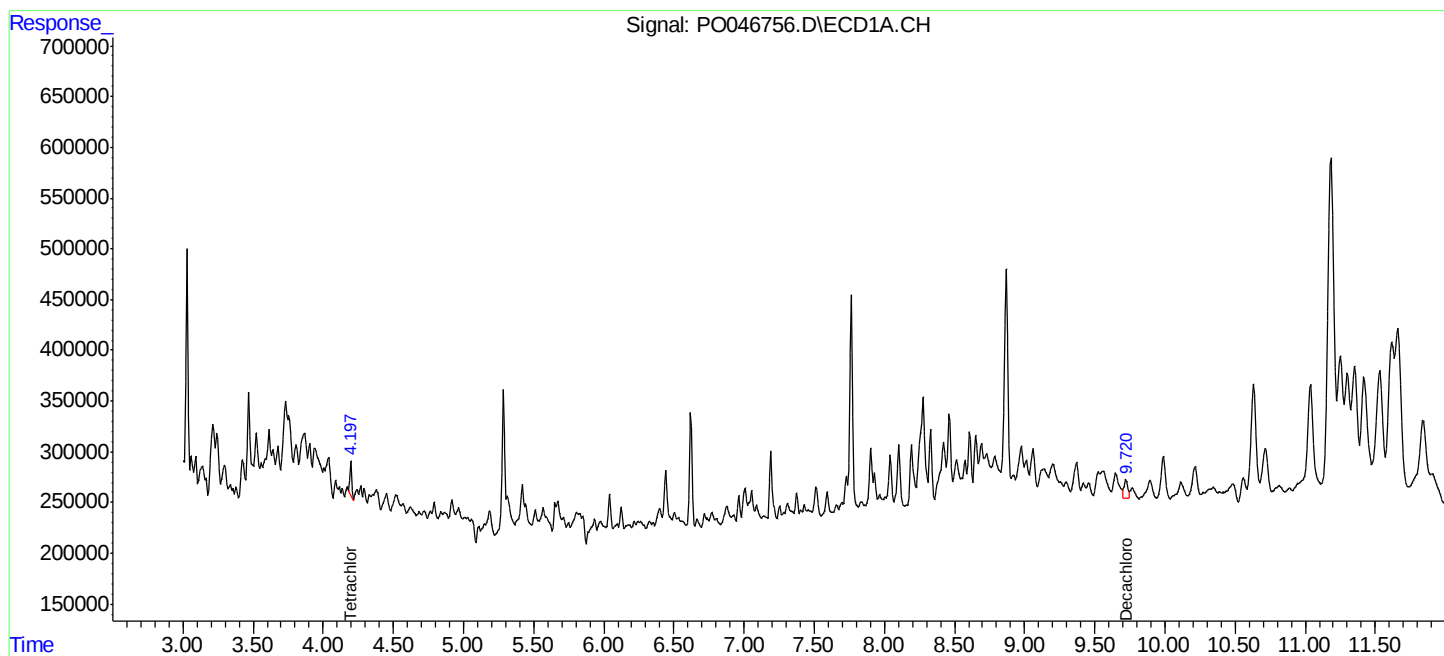

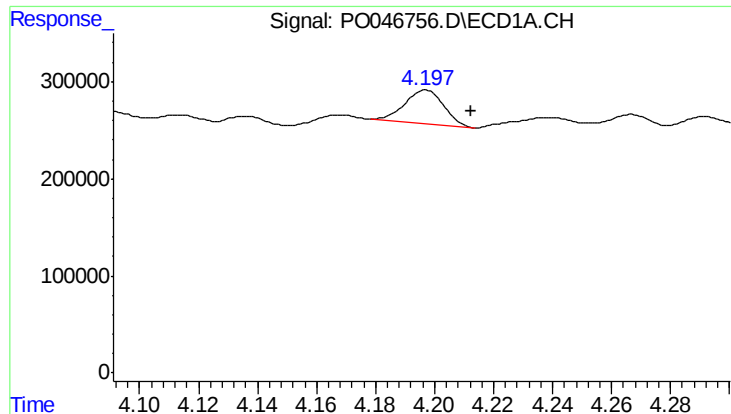


#1 Tetrachloro-m-xylene

R.T.: 4.197 min
Delta R.T.: -0.015 min
Response: 322942
Conc: 1.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
A403672


Manual Integrations
APPROVED

Sohil
7/17/2018 4:25:41 PM

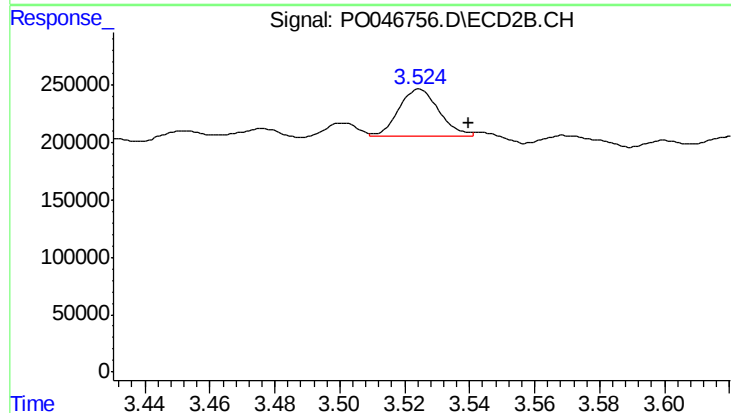


#1 Tetrachloro-m-xylene

R.T.: 3.524 min
Delta R.T.: -0.016 min
Response: 347115
Conc: 1.63 ng/ml m

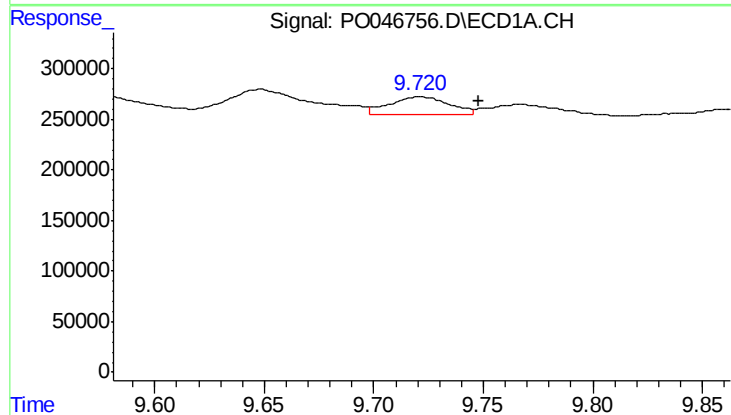

#2 Decachlorobiphenyl

R.T.: 9.720 min
Delta R.T.: -0.028 min
Response: 328128
Conc: 1.72 ng/ml m

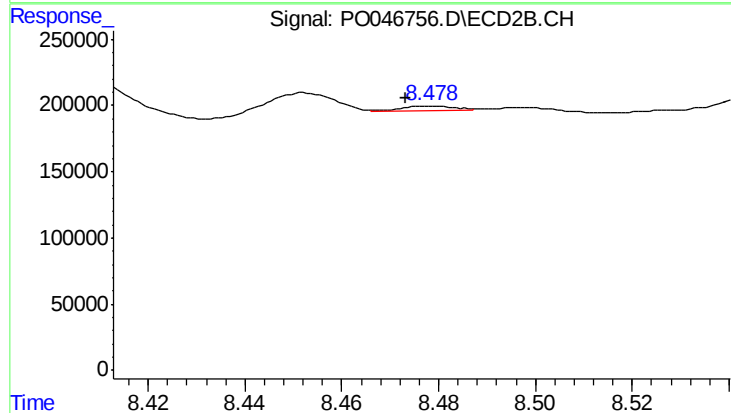

#2 Decachlorobiphenyl

R.T.: 8.478 min
Delta R.T.: 0.005 min
Response: 28474
Conc: 0.15 ng/ml m