

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0071618\
Data File : P0046772.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Jul 2018 21:35
Operator : SM/SJ
Sample : J3976-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-033

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 06:06:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

	System Monitoring Compounds						
1)	SA Tetrachlo...	4.194	3.519	3919092	4432156	16.399	20.866 #
2)	SA Decachlor...	9.716	8.445	2408090	2386904	12.634	12.305

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0071618\
Data File : P0046772.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Jul 2018 21:35
Operator : SM/SJ
Sample : J3976-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-033

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 06:06:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

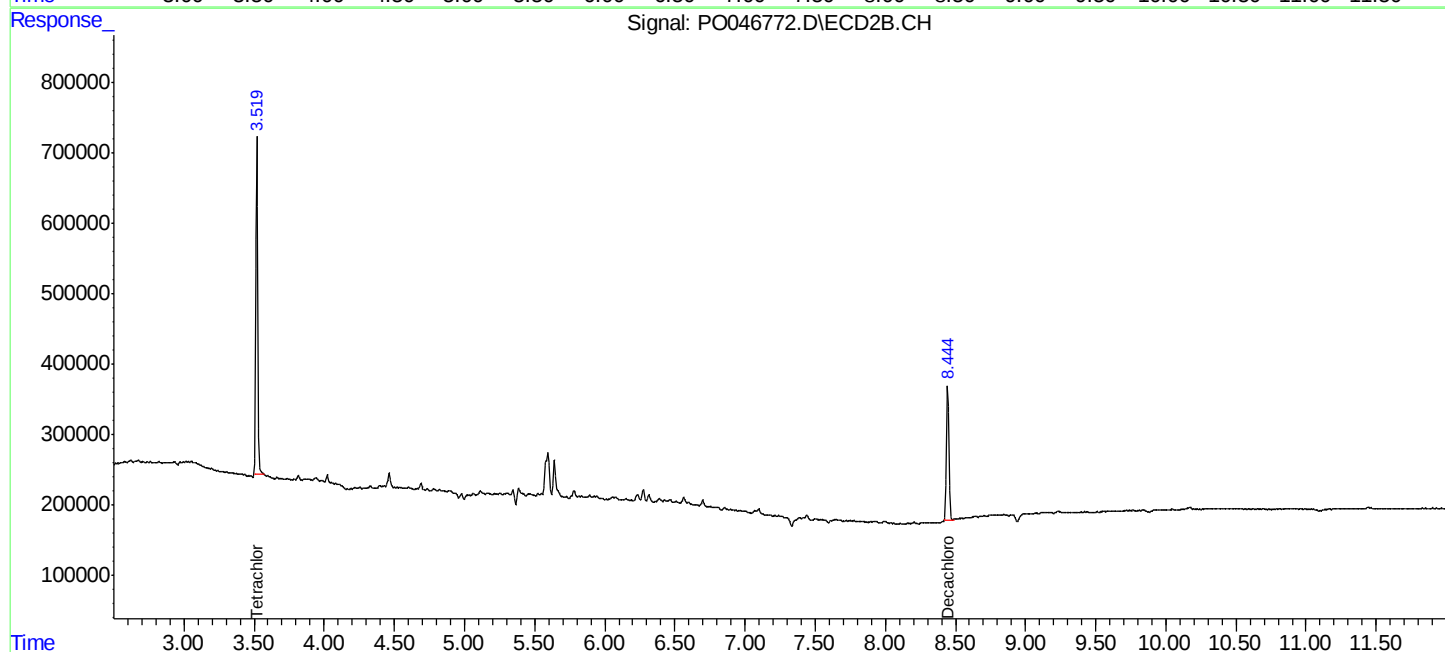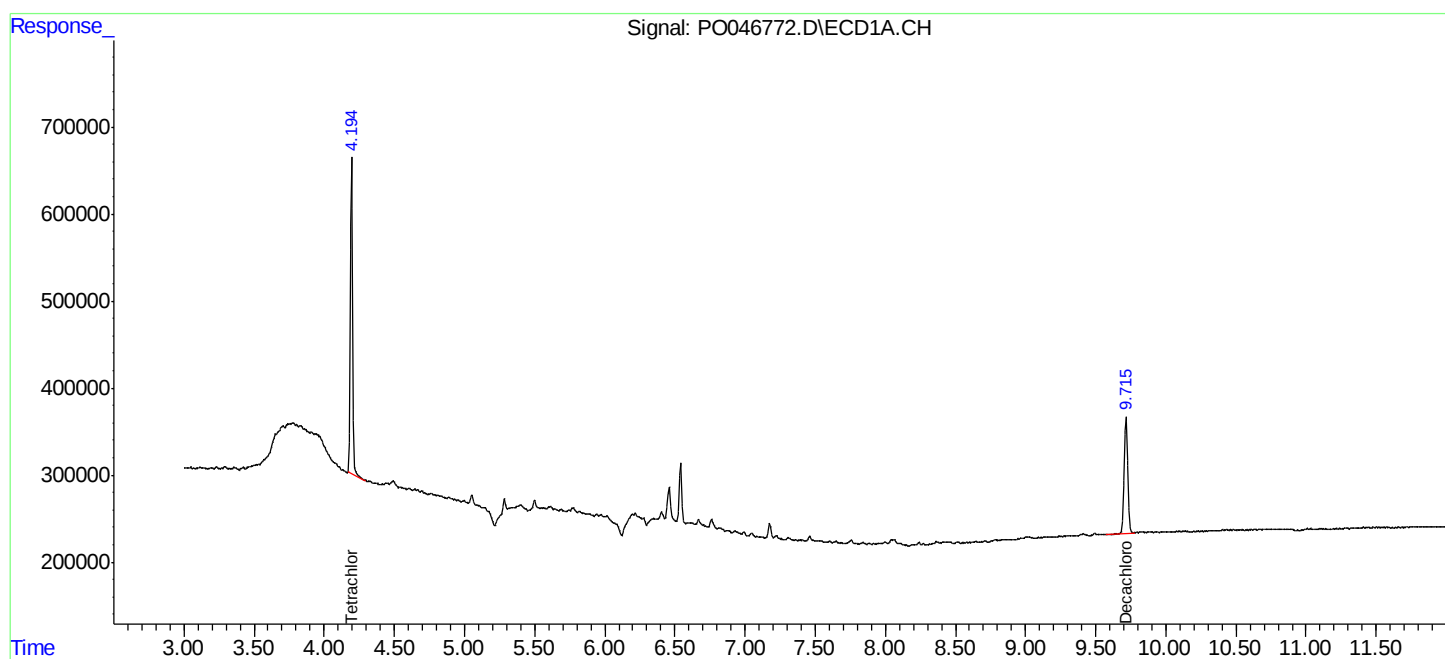


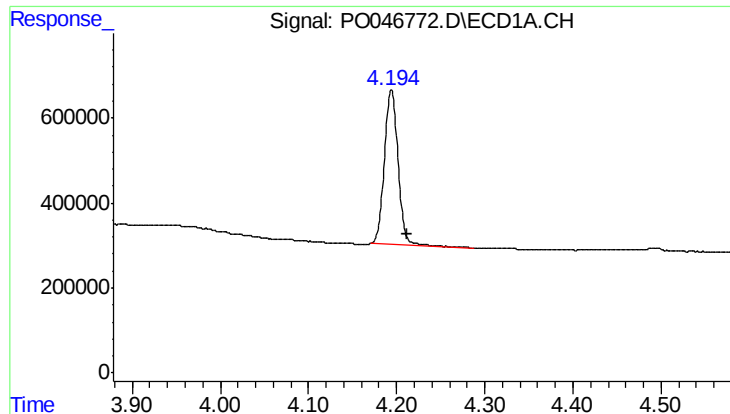

#1 Tetrachloro-m-xylene


R.T.: 4.194 min
Delta R.T.: -0.018 min
Response: 3919092
Conc: 16.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-033

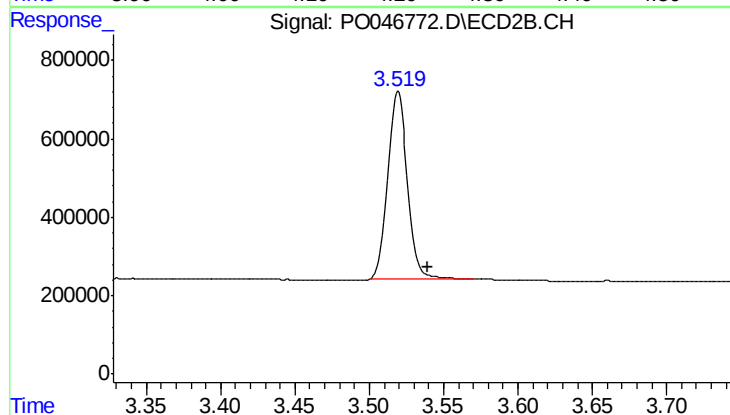


#1 Tetrachloro-m-xylene

R.T.: 3.519 min
Delta R.T.: -0.020 min
Response: 4432156
Conc: 20.87 ng/ml

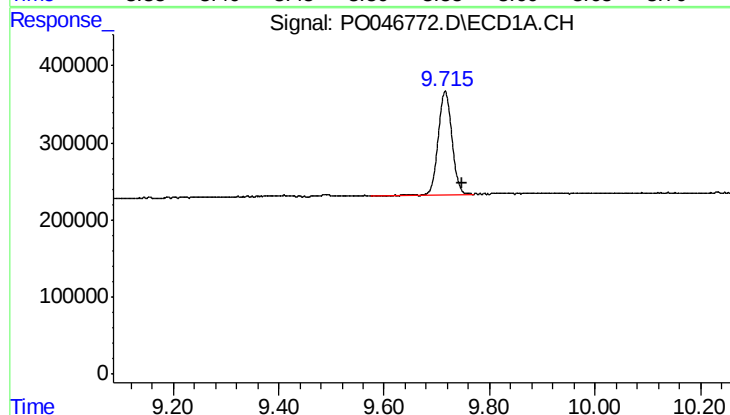

#2 Decachlorobiphenyl

R.T.: 9.716 min
Delta R.T.: -0.032 min
Response: 2408090
Conc: 12.63 ng/ml

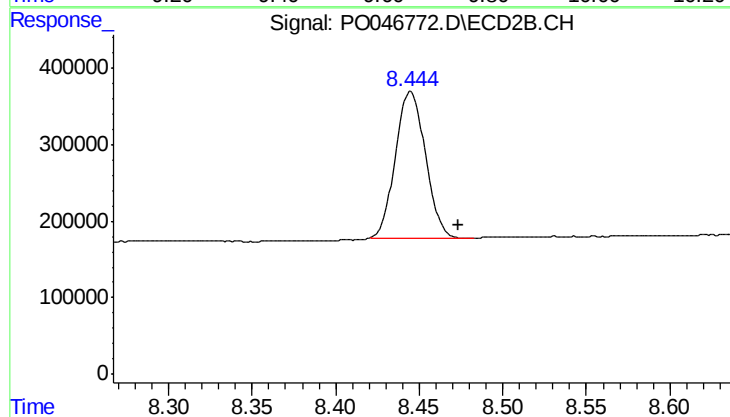

#2 Decachlorobiphenyl

R.T.: 8.445 min
Delta R.T.: -0.029 min
Response: 2386904
Conc: 12.30 ng/ml