

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071620\
 Data File : P0069725.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Jul 2020 13:28
 Operator : DD\AJ
 Sample : L3301-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CARLSTADT-SAMPLE-2020

Manual Integrations
 APPROVED

Ankita
 7/17/2020 11:39:13 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 16 15:35:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 08 16:12:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.389	3.564	1143865	1205255	30.637	30.286
2) SA Decachlor...	10.045	8.769	945169	860807	15.709	15.167m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071620\
Data File : P0069725.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Jul 2020 13:28
Operator : DD\AJ
Sample : L3301-01
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CARLSTADT-SAMPLE-2020


Manual Integrations
APPROVED

Ankita
7/17/2020 11:39:13 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 16 15:35:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 08 16:12:41 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

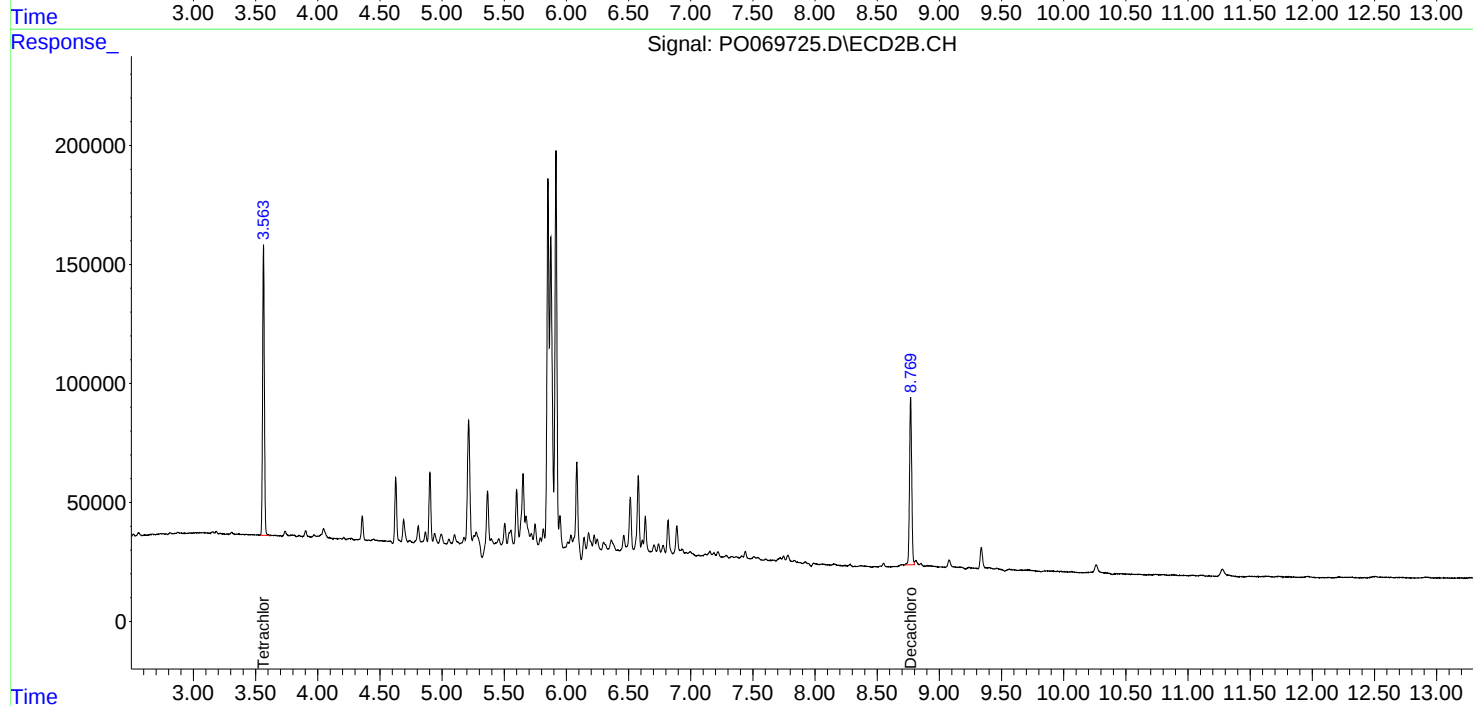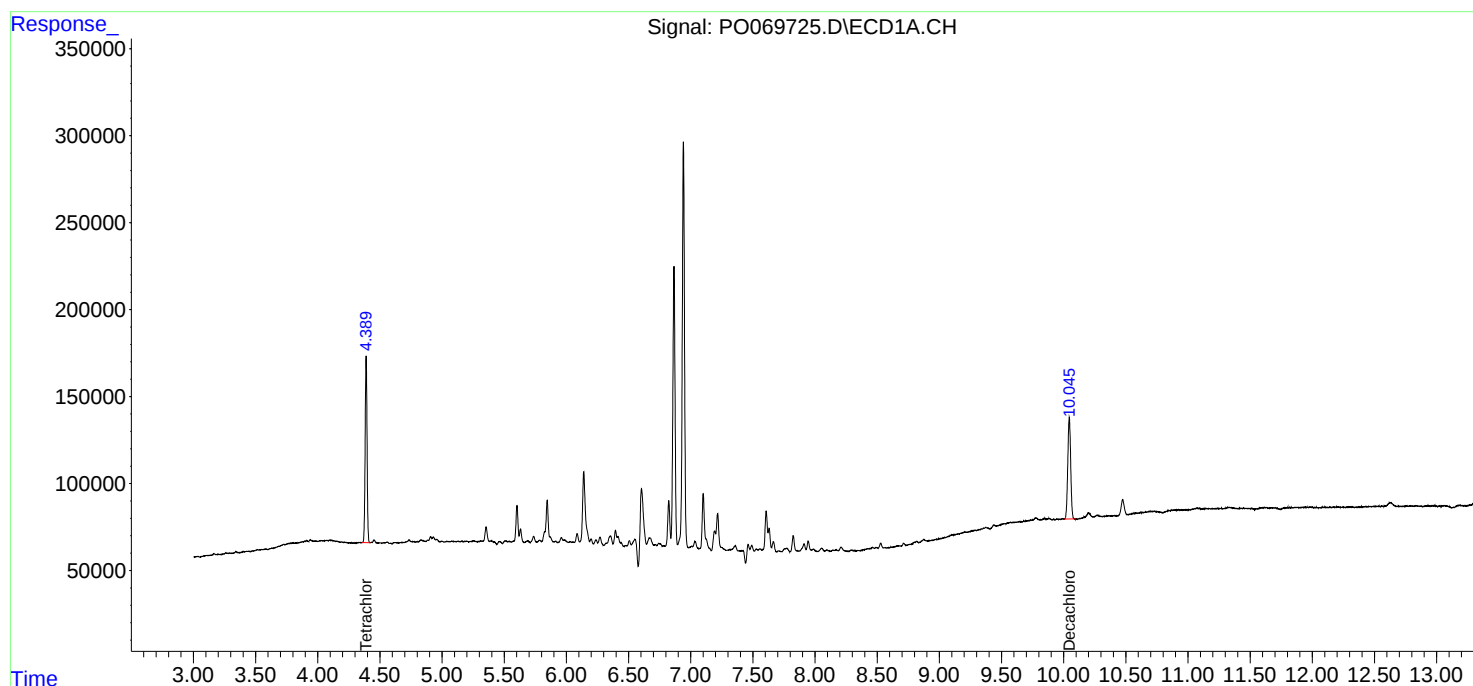

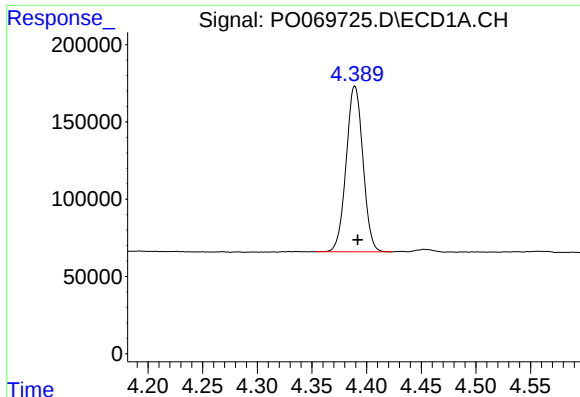


#1 Tetrachloro-m-xylene

R.T.: 4.389 min
Delta R.T.: -0.003 min
Response: 1143865
Conc: 30.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
CARLSTADT-SAMPLE-2020


Manual Integrations
APPROVED

Ankita
7/17/2020 11:39:13 AM

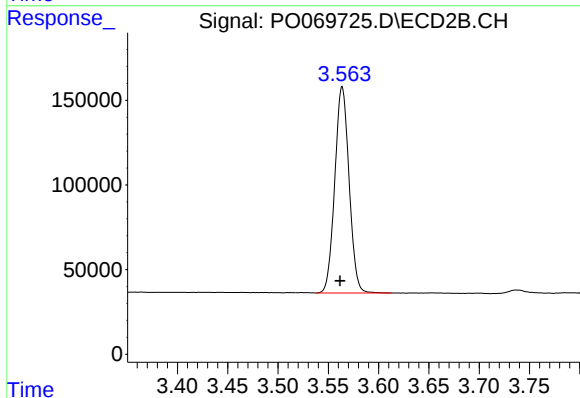


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: 0.002 min
Response: 1205255
Conc: 30.29 ng/ml

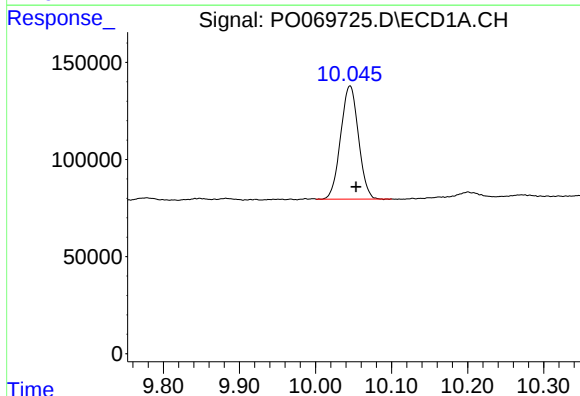

#2 Decachlorobiphenyl

R.T.: 10.045 min
Delta R.T.: -0.008 min
Response: 945169
Conc: 15.71 ng/ml

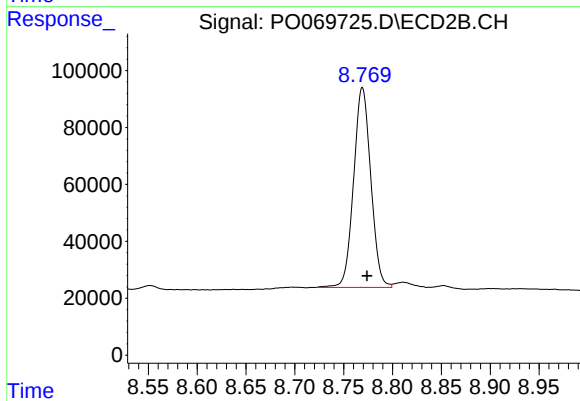

#2 Decachlorobiphenyl

R.T.: 8.769 min
Delta R.T.: -0.005 min
Response: 860807
Conc: 15.17 ng/ml m