

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071620\
 Data File : P0069734.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 Jul 2020 16:02
 Operator : DD\AJ
 Sample : L3183-11
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OK-03-071520

Manual Integrations
 APPROVED

Ankita
 7/17/2020 11:39:34 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 01:34:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 08 16:12:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.388	3.563	1120832	1216294	30.020m	30.563
2) SA Decachlor...	10.044	8.770	1088800	925893	18.097	16.314

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071620\
Data File : P0069734.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 Jul 2020 16:02
Operator : DD\AJ
Sample : L3183-11
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OK-03-071520


Manual Integrations
APPROVED

Ankita
7/17/2020 11:39:34 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 01:34:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 08 16:12:41 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

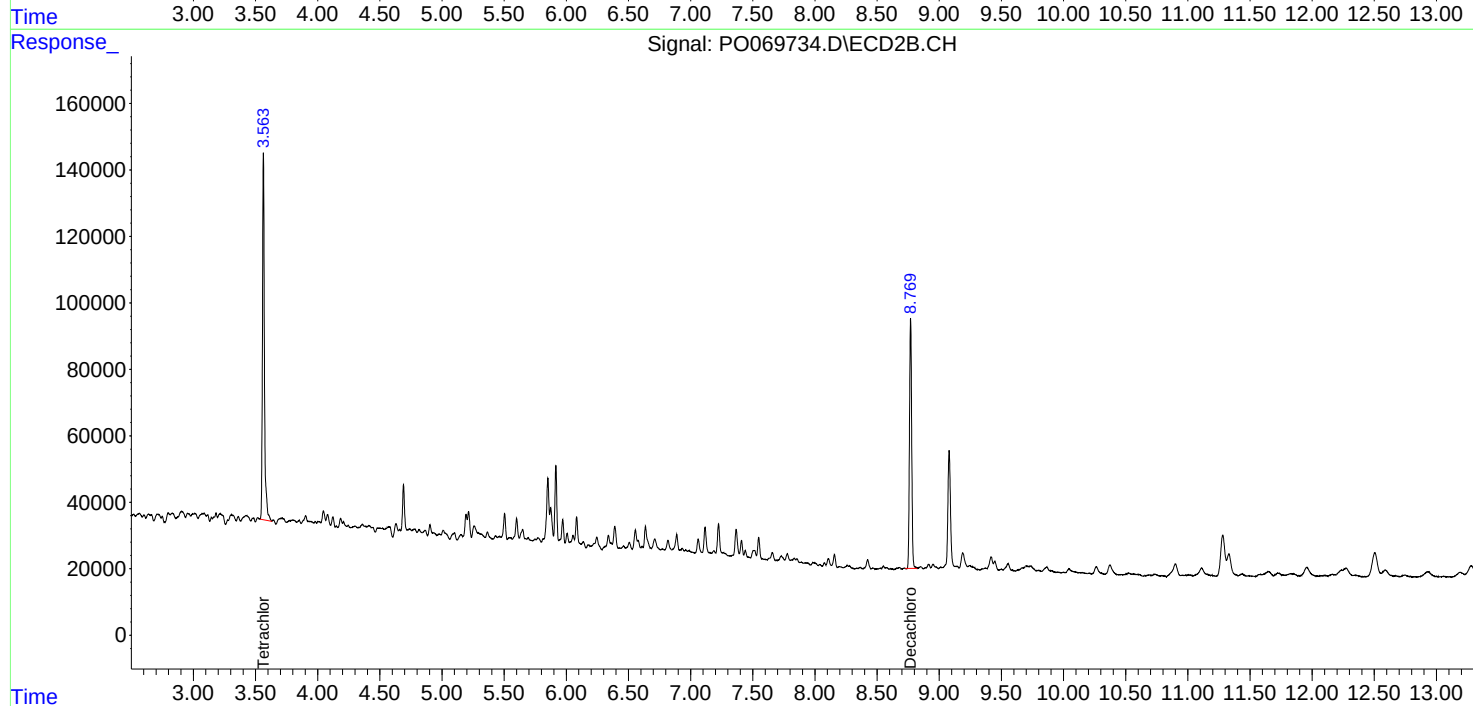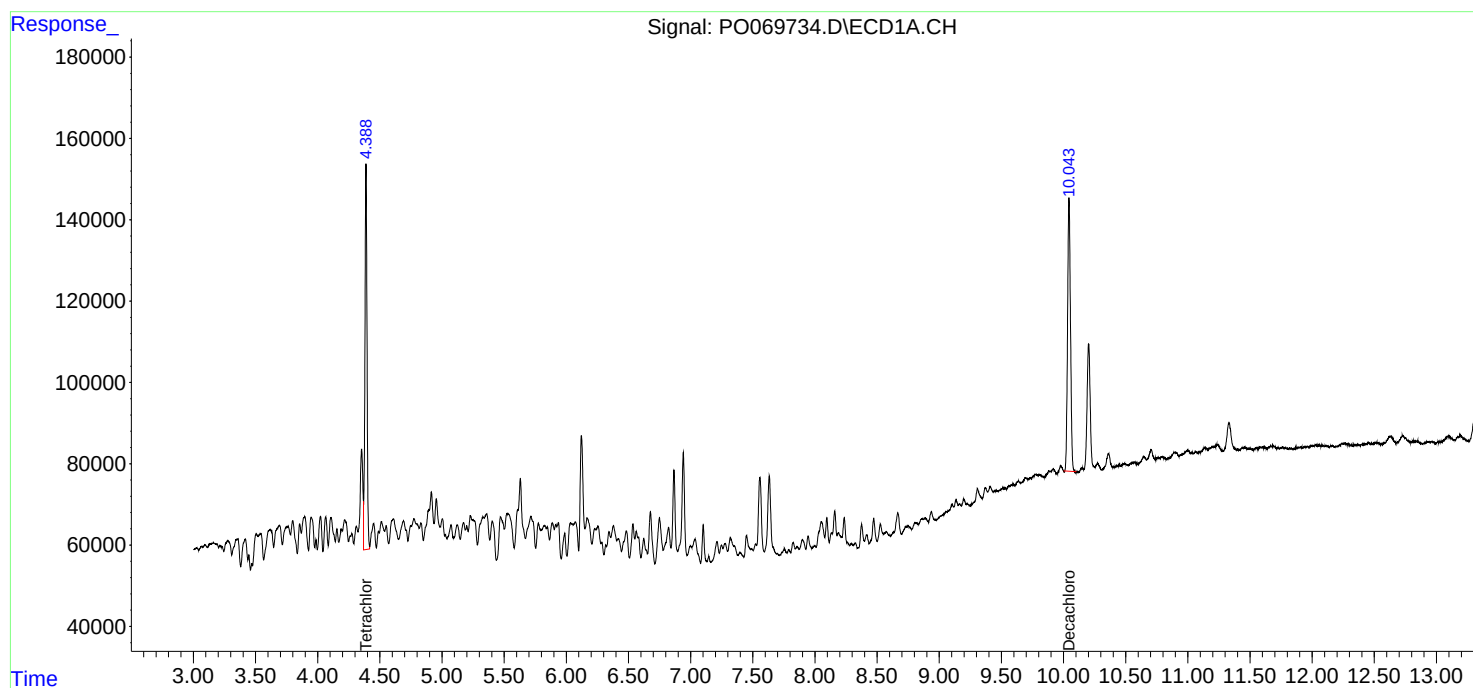

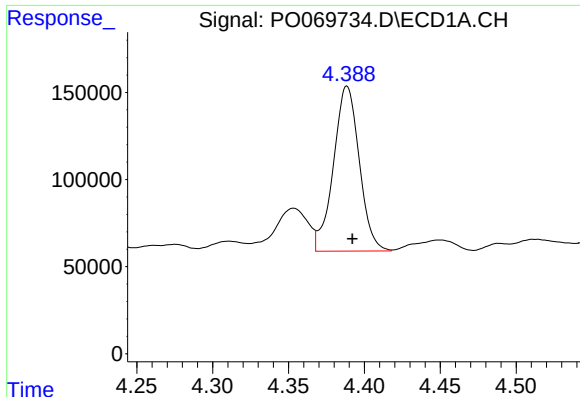


#1 Tetrachloro-m-xylene

R.T.: 4.388 min
Delta R.T.: -0.004 min
Response: 1120832
Conc: 30.02 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OK-03-071520


Manual Integrations
APPROVED

Ankita
7/17/2020 11:39:34 AM

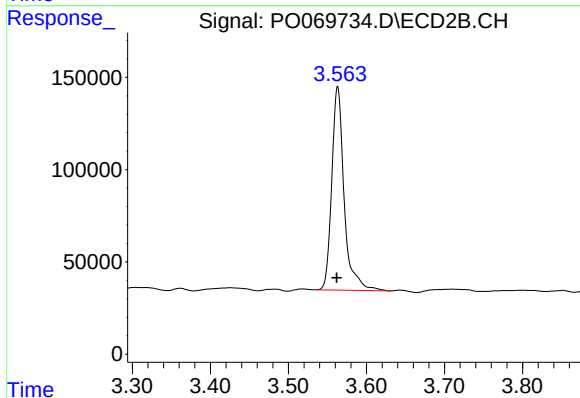


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: 0.001 min
Response: 1216294
Conc: 30.56 ng/ml

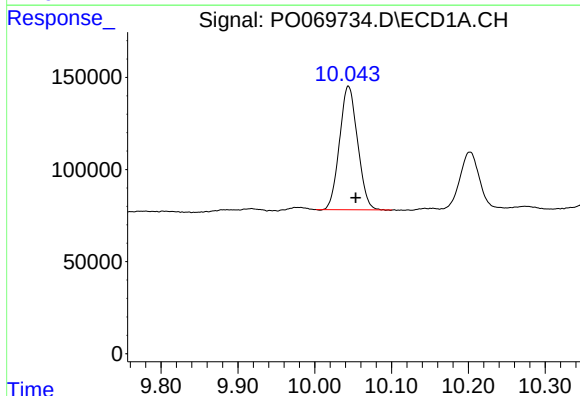

#2 Decachlorobiphenyl

R.T.: 10.044 min
Delta R.T.: -0.009 min
Response: 1088800
Conc: 18.10 ng/ml

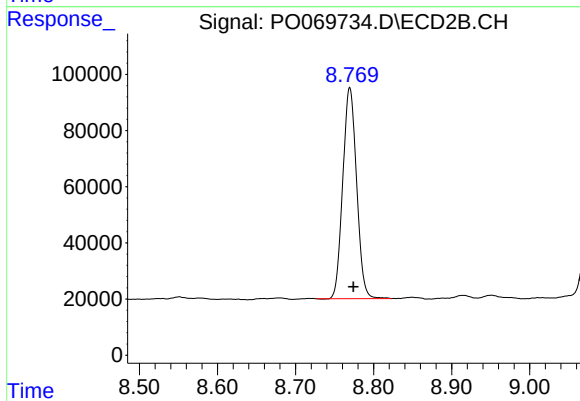

#2 Decachlorobiphenyl

R.T.: 8.770 min
Delta R.T.: -0.004 min
Response: 925893
Conc: 16.31 ng/ml