

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0071718\
 Data File : P0046849.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jul 2018 2:06
 Operator : SM/SJ
 Sample : J4013-05
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-ID

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 07:42:14 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 09 15:27:34 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.200	3.525	2559439	2743166	10.710	12.915
2)	SA Decachlor...	9.727	8.451	1502404	1471156	7.882	7.584
Target Compounds							
27)	L6 AR-1254-2	6.766	0.000	263431	0	29.907	N.D. #
28)	L6 AR-1254-3	6.766	0.000	263431	0	17.230	N.D. #
29)	L6 AR-1254-4	0.000	6.233	0	352491	N.D.	27.955 #
32)	L7 AR-1260-2	0.000	6.233	0	352491	N.D.	22.106 #
35)	L7 AR-1260-5	0.000	7.446	0	21911	N.D.	1.141 #
36)	L8 AR-1262-1	0.000	6.233	0	352491	N.D.	26.913 #
41)	L9 AR-1268-1	0.000	7.446	0	21911	N.D.	0.783 #
42)	L9 AR-1268-2	0.000	7.446	0	21911	N.D.	0.795 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071718\
Data File : P0046849.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jul 2018 2:06
Operator : SM/SJ
Sample : J4013-05
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-I-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 07:42:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

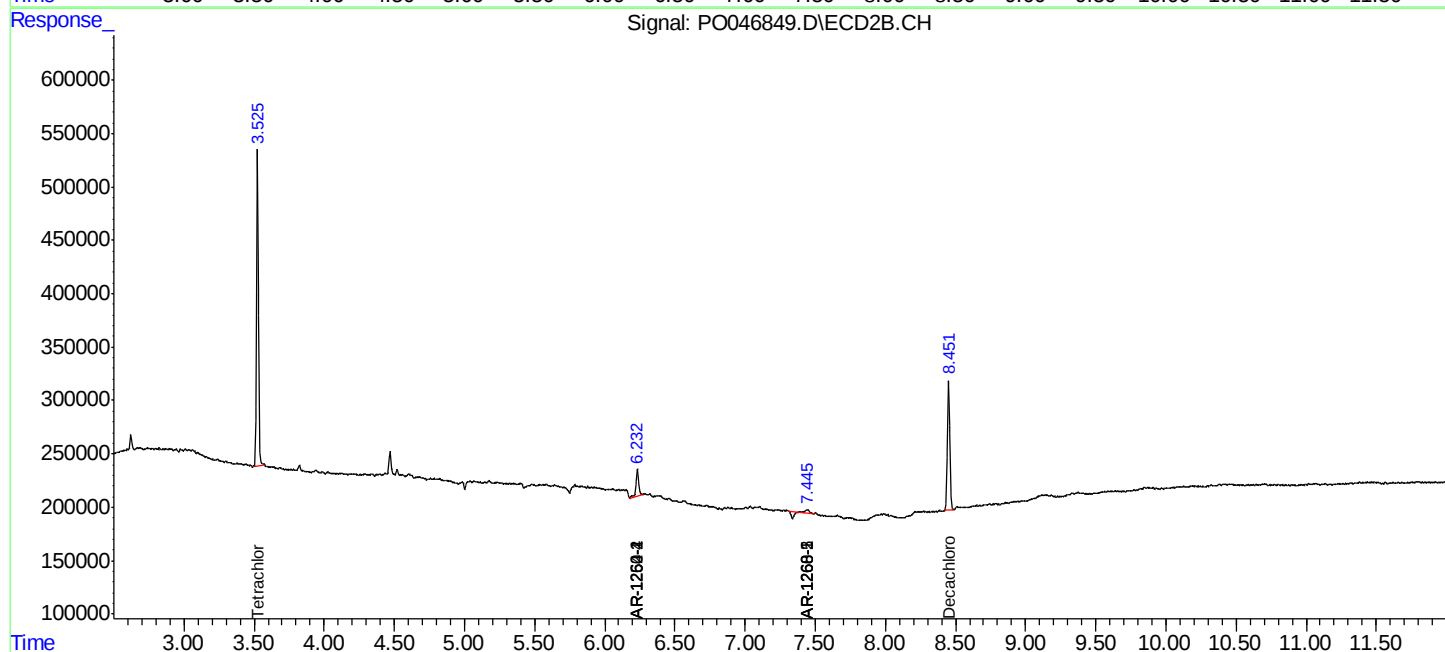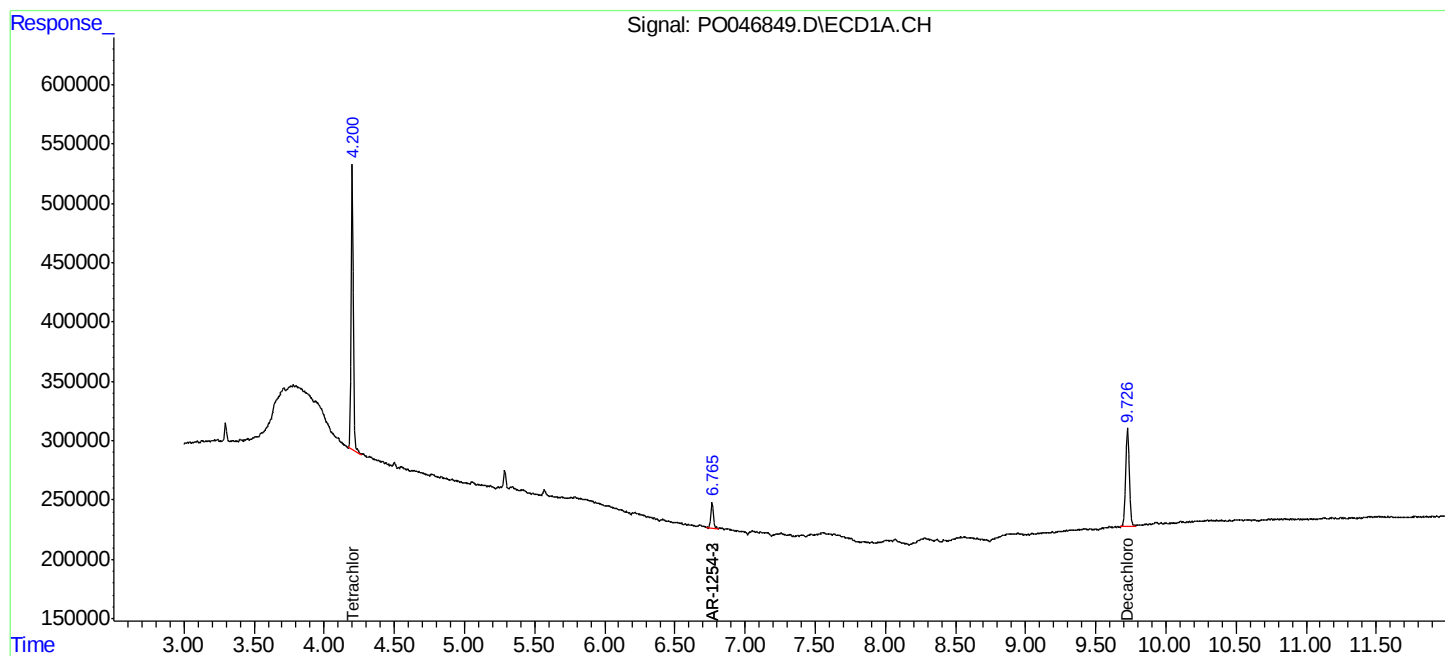


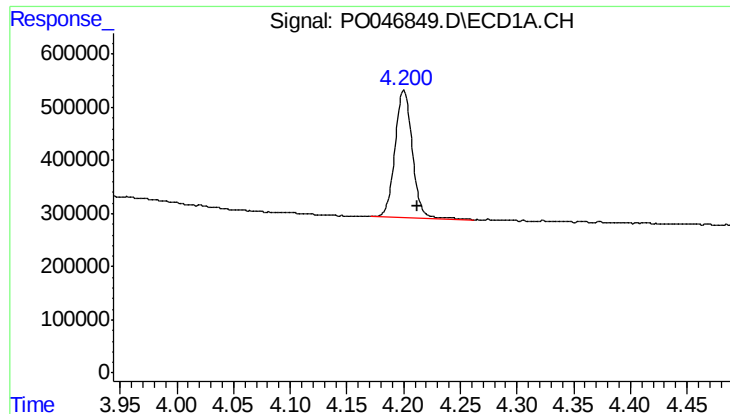

#1 Tetrachloro-m-xylene


R.T.: 4.200 min
Delta R.T.: -0.012 min
Response: 2559439
Conc: 10.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-ID

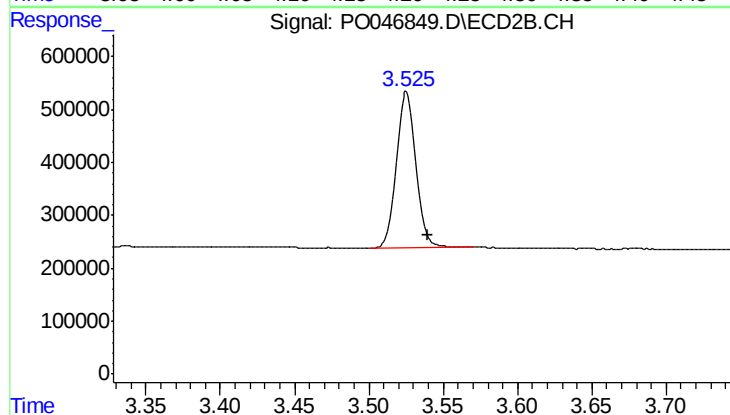


#1 Tetrachloro-m-xylene

R.T.: 3.525 min
Delta R.T.: -0.014 min
Response: 2743166
Conc: 12.91 ng/ml

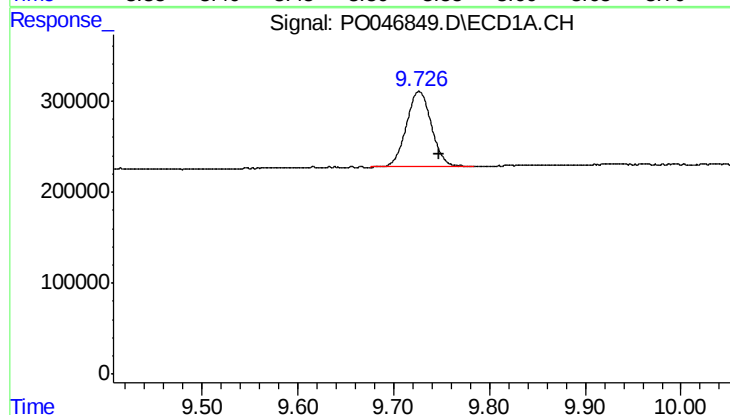


#2 Decachlorobiphenyl

R.T.: 9.727 min
Delta R.T.: -0.021 min
Response: 1502404
Conc: 7.88 ng/ml

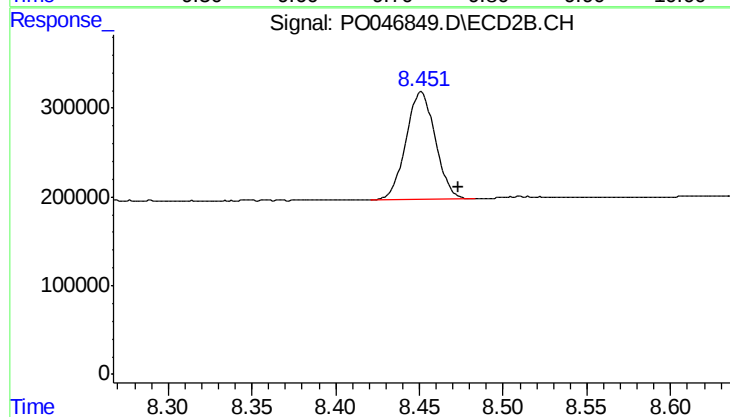

#2 Decachlorobiphenyl


R.T.: 8.451 min
Delta R.T.: -0.022 min
Response: 1471156
Conc: 7.58 ng/ml

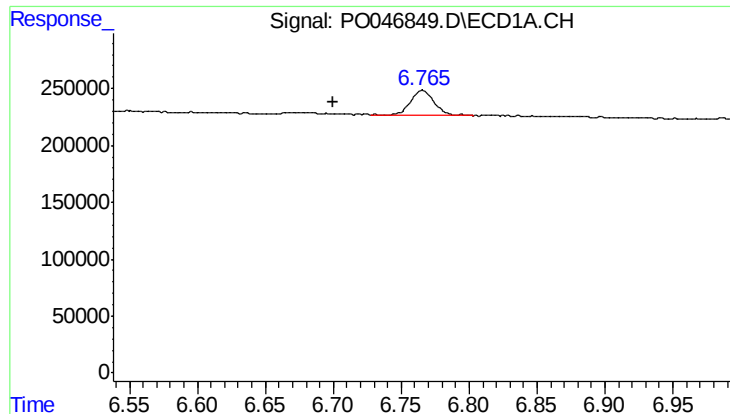

#27 AR-1254-2


R.T.: 6.766 min
Delta R.T.: 0.066 min
Response: 263431
Conc: 29.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-ID

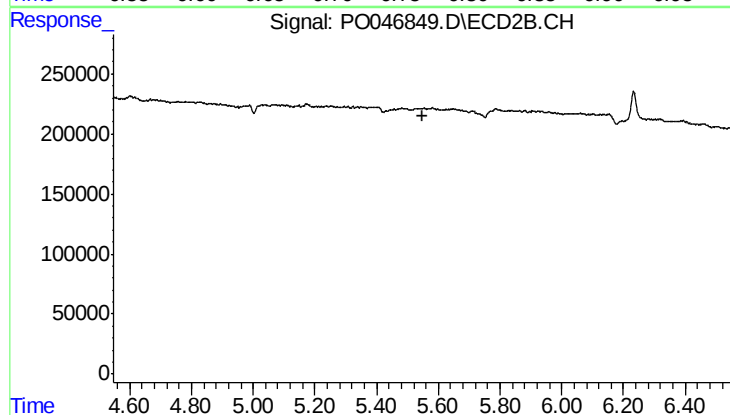


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T.: 5.547 min
Response: 0
Conc: N.D.

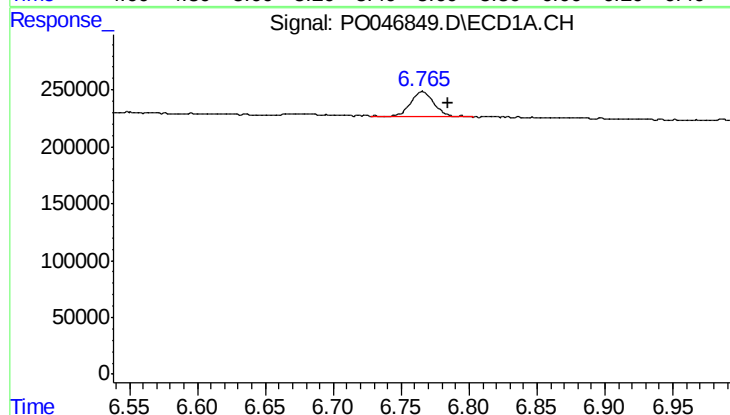


#28 AR-1254-3

R.T.: 6.766 min
Delta R.T.: -0.018 min
Response: 263431
Conc: 17.23 ng/ml

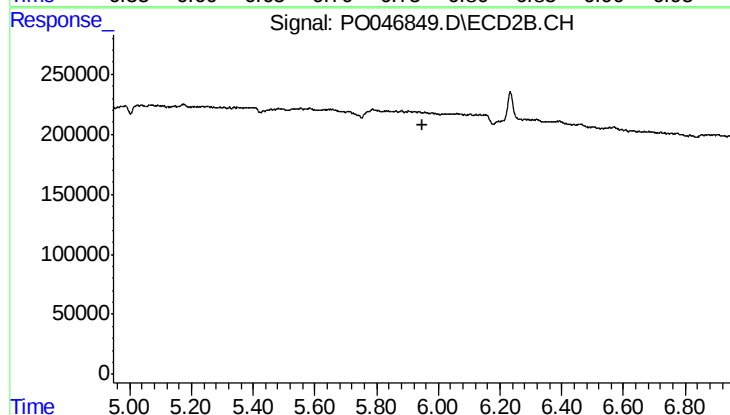

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 5.947 min
Response: 0
Conc: N.D.

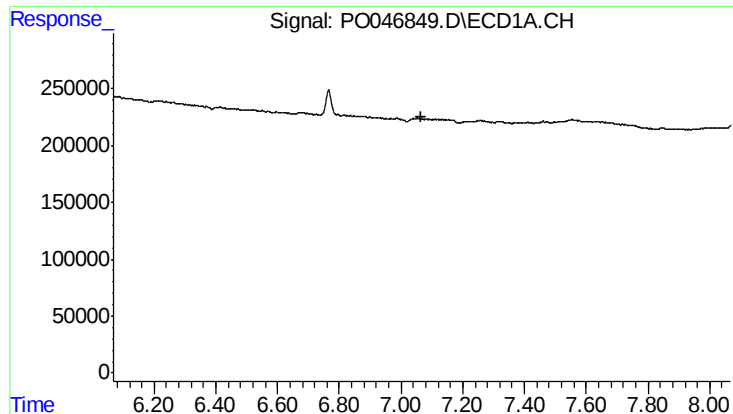

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.068 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-ID

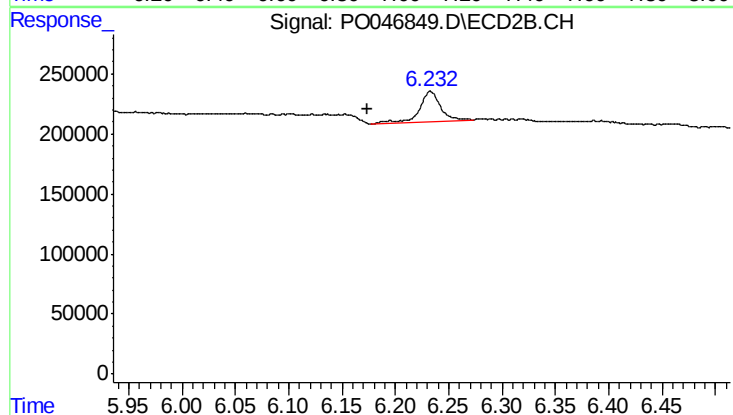


#29 AR-1254-4

R.T.: 6.233 min
Delta R.T.: 0.059 min
Response: 352491
Conc: 27.95 ng/ml

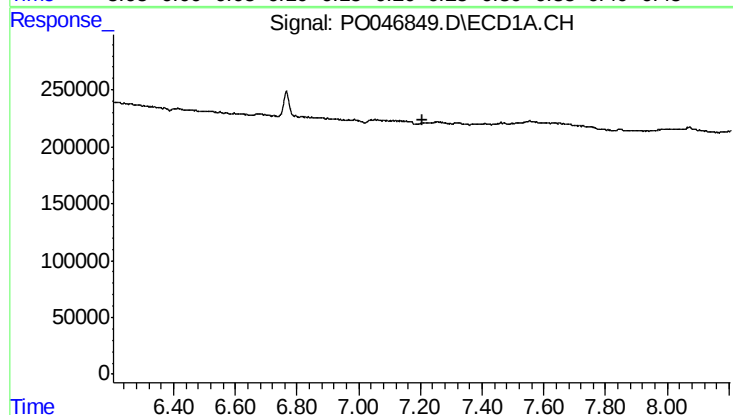


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.205 min
Response: 0
Conc: N.D.

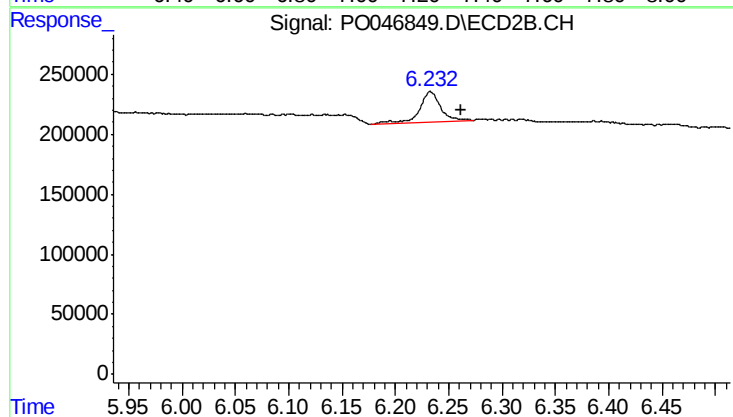

#32 AR-1260-2


R.T.: 6.233 min
Delta R.T.: -0.029 min
Response: 352491
Conc: 22.11 ng/ml

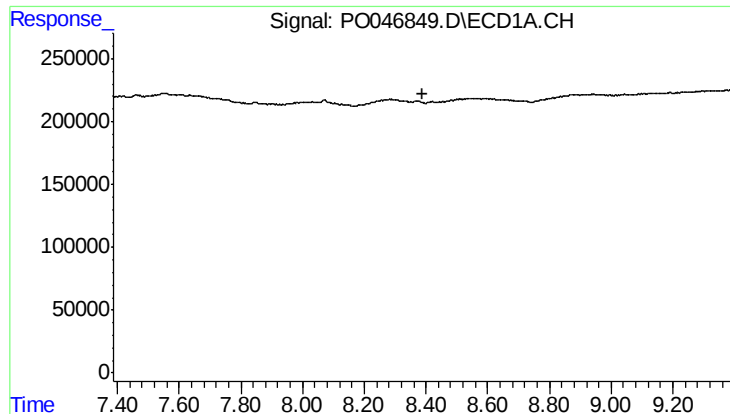

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.387 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-ID

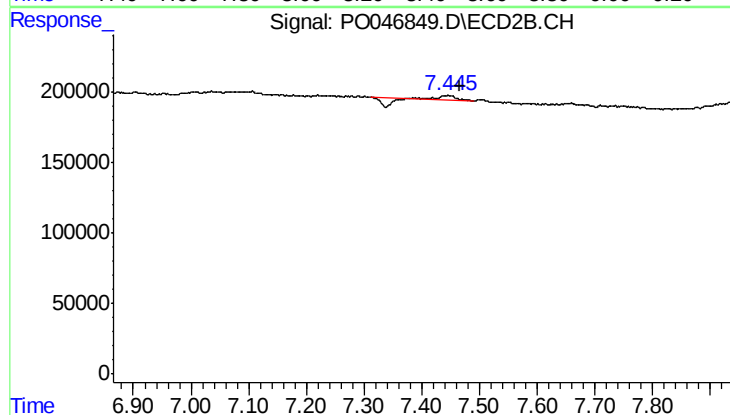


#35 AR-1260-5

R.T.: 7.446 min
Delta R.T.: -0.021 min
Response: 21911
Conc: 1.14 ng/ml

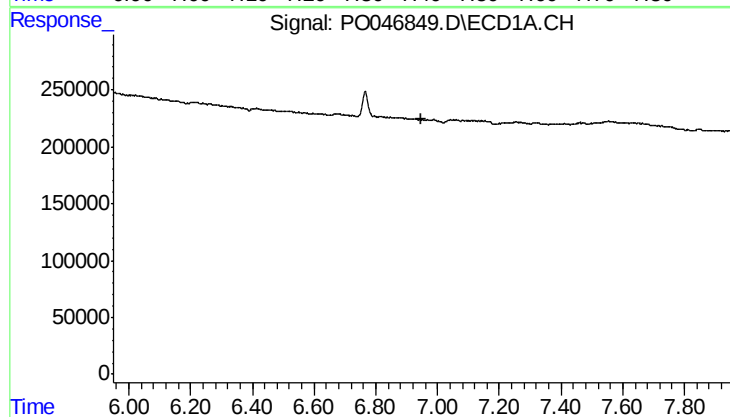


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 6.949 min
Response: 0
Conc: N.D.

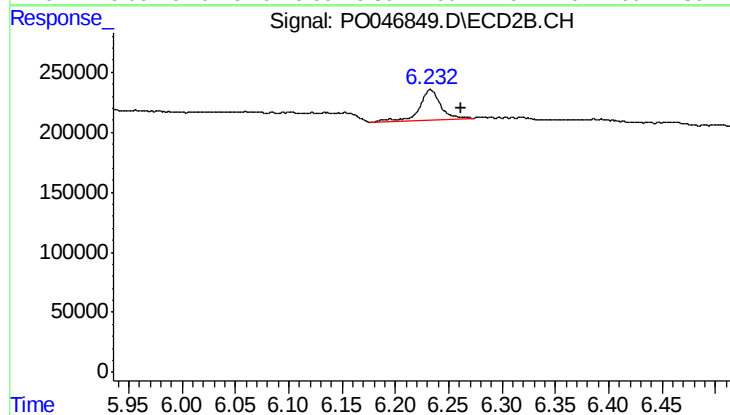

#36 AR-1262-1


R.T.: 6.233 min
Delta R.T.: -0.029 min
Response: 352491
Conc: 26.91 ng/ml

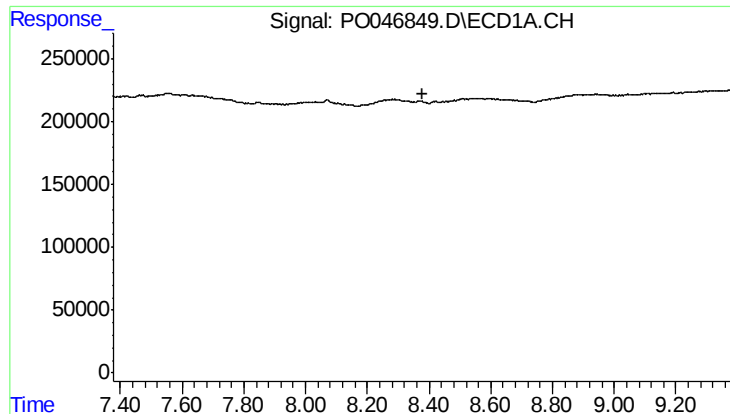

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.377 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-ID

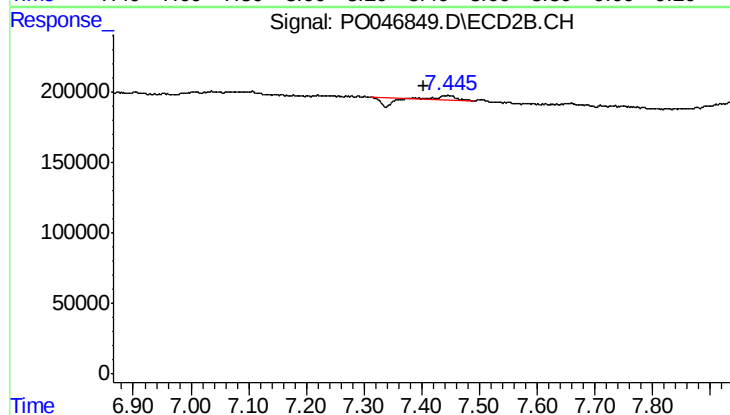


#41 AR-1268-1

R.T.: 7.446 min
Delta R.T.: 0.042 min
Response: 21911
Conc: 0.78 ng/ml

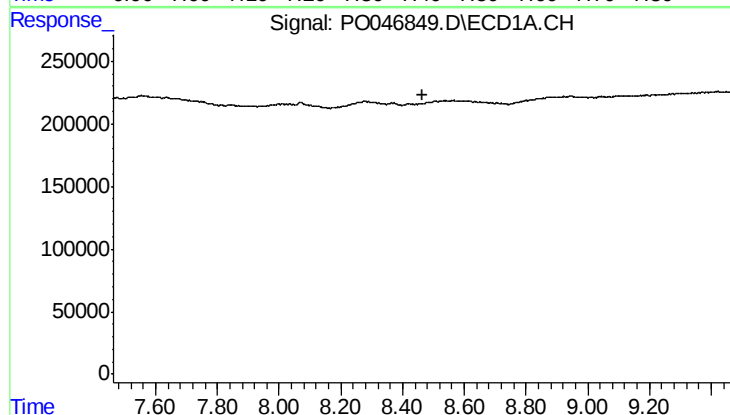

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.463 min
Response: 0
Conc: N.D.

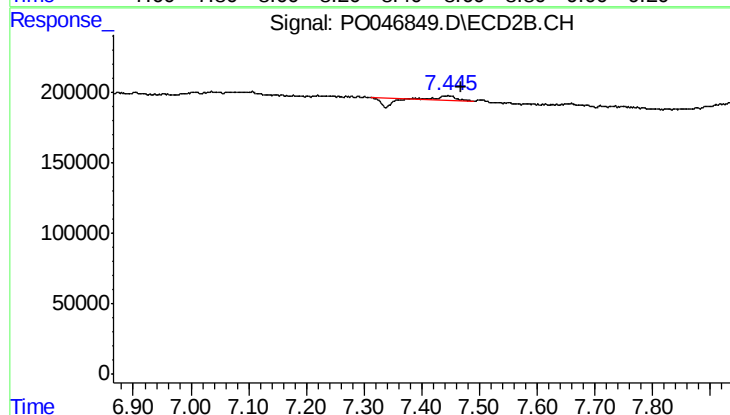

#42 AR-1268-2

R.T.: 7.446 min
Delta R.T.: -0.022 min
Response: 21911
Conc: 0.80 ng/ml