

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0071718\
 Data File : P0046833.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Jul 2018 21:51
 Operator : SM/SJ
 Sample : J3826-03
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OK-01-071618

Manual Integrations
 APPROVED

Sohil
 7/18/2018 1:43:48 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 08:26:49 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 09 15:27:34 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.200	3.525	3172321	3474190	13.274m	16.356
2) SA Decachlor...	9.727	8.452	1895879	1490745	9.947	7.685

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0071718\
Data File : P0046833.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Jul 2018 21:51
Operator : SM/SJ
Sample : J3826-03
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OK-01-071618


Manual Integrations
APPROVED

Sohil
7/18/2018 1:43:48 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 08:26:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

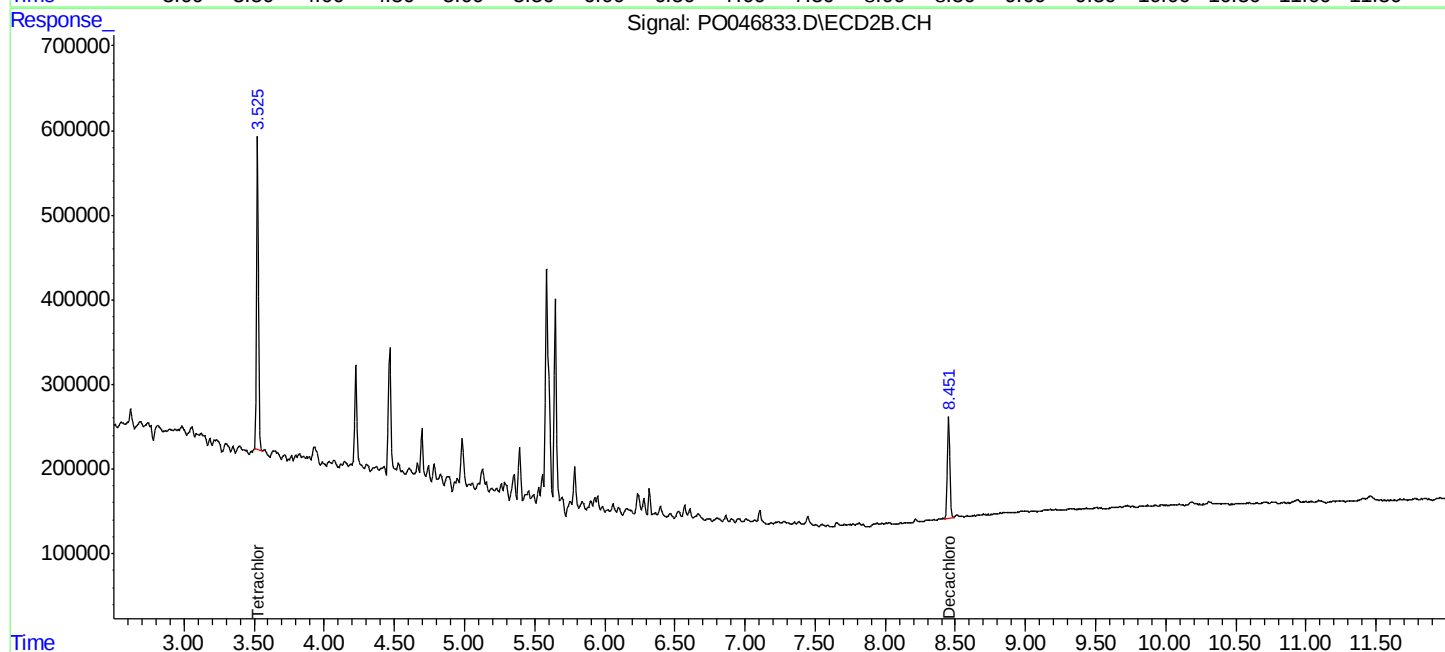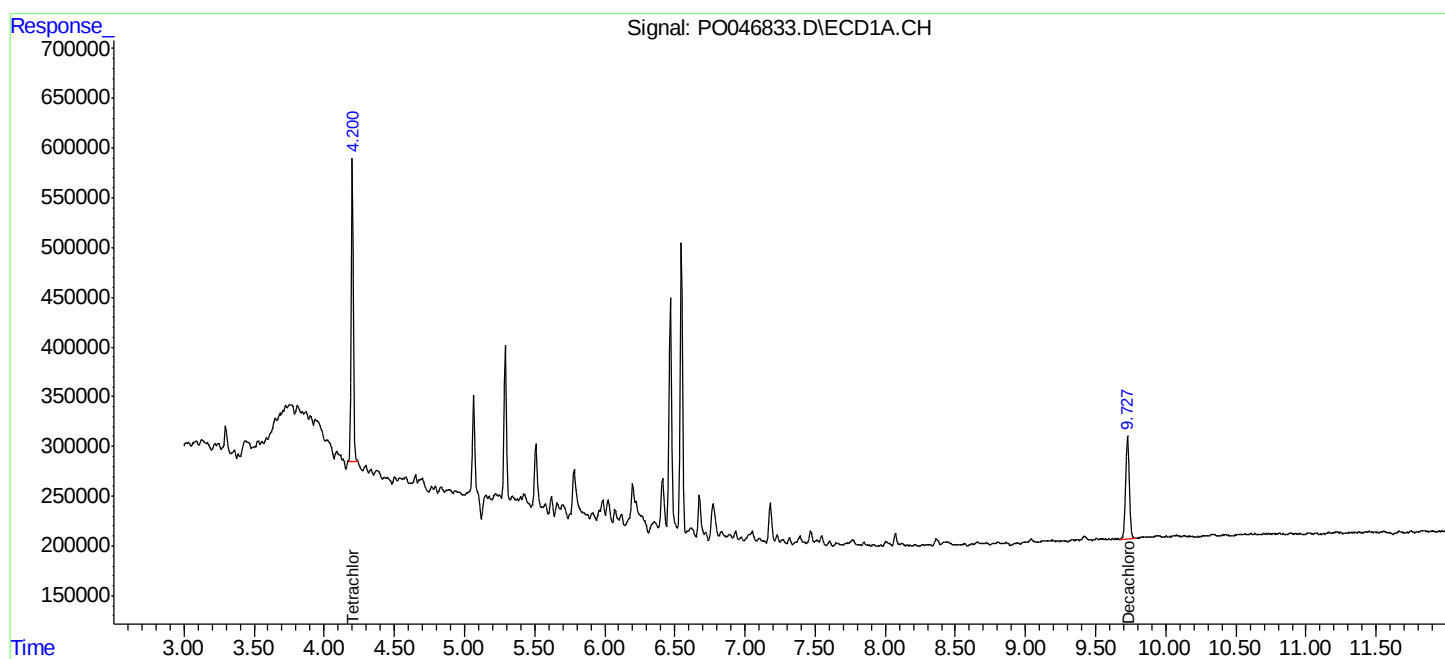

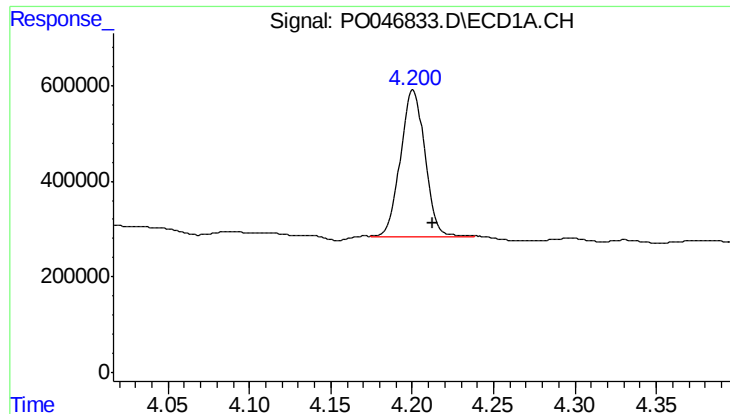


#1 Tetrachloro-m-xylene

R.T.: 4.200 min
Delta R.T.: -0.012 min
Response: 3172321
Conc: 13.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
OK-01-071618


Manual Integrations
APPROVED

Sohil
7/18/2018 1:43:48 PM

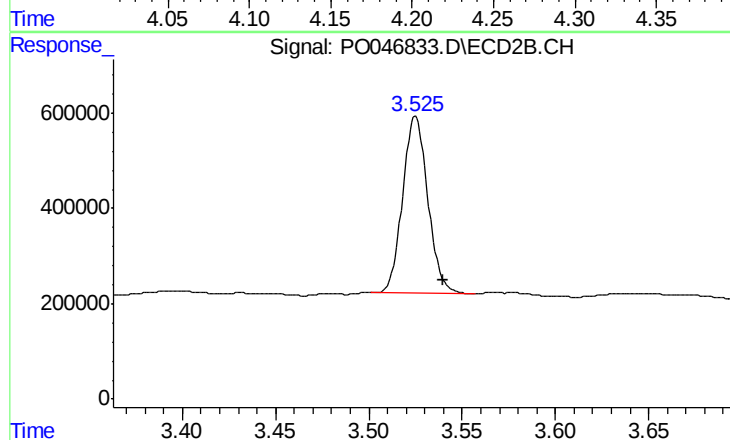


#1 Tetrachloro-m-xylene

R.T.: 3.525 min
Delta R.T.: -0.015 min
Response: 3474190
Conc: 16.36 ng/ml

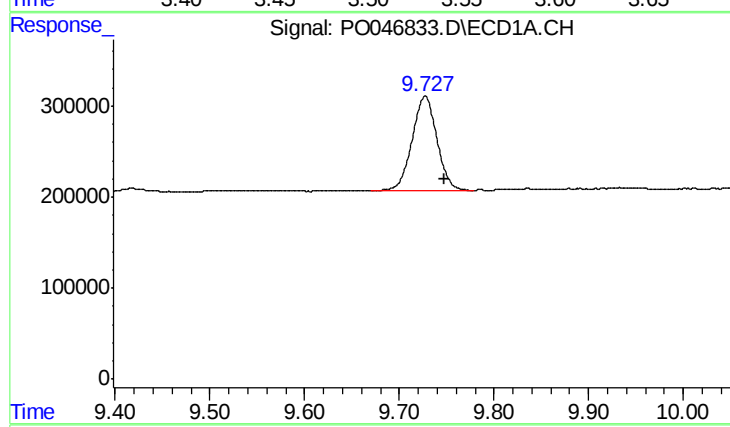

#2 Decachlorobiphenyl

R.T.: 9.727 min
Delta R.T.: -0.021 min
Response: 1895879
Conc: 9.95 ng/ml

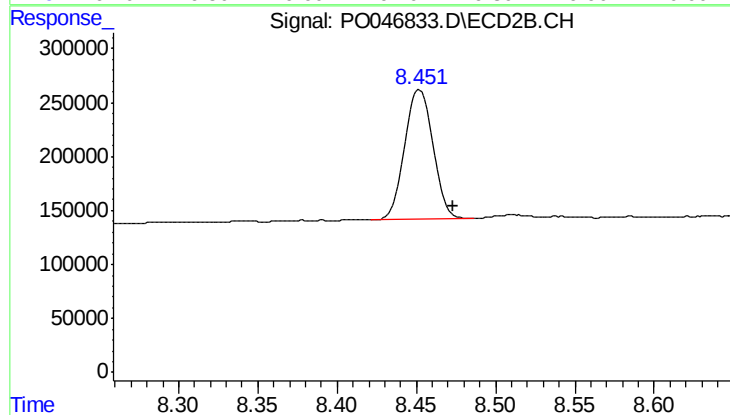

#2 Decachlorobiphenyl

R.T.: 8.452 min
Delta R.T.: -0.021 min
Response: 1490745
Conc: 7.68 ng/ml