

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0071718\
Data File : P0046848.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jul 2018 1:50
Operator : SM/SJ
Sample : J4013-01
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-I-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 08:36:24 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.201	3.525	5642479	6209325	23.610	29.233
2) SA Decachlor...	9.728	8.451	3140460	3134390	16.476	16.158

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0071718\
Data File : P0046848.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jul 2018 1:50
Operator : SM/SJ
Sample : J4013-01
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-I-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 08:36:24 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

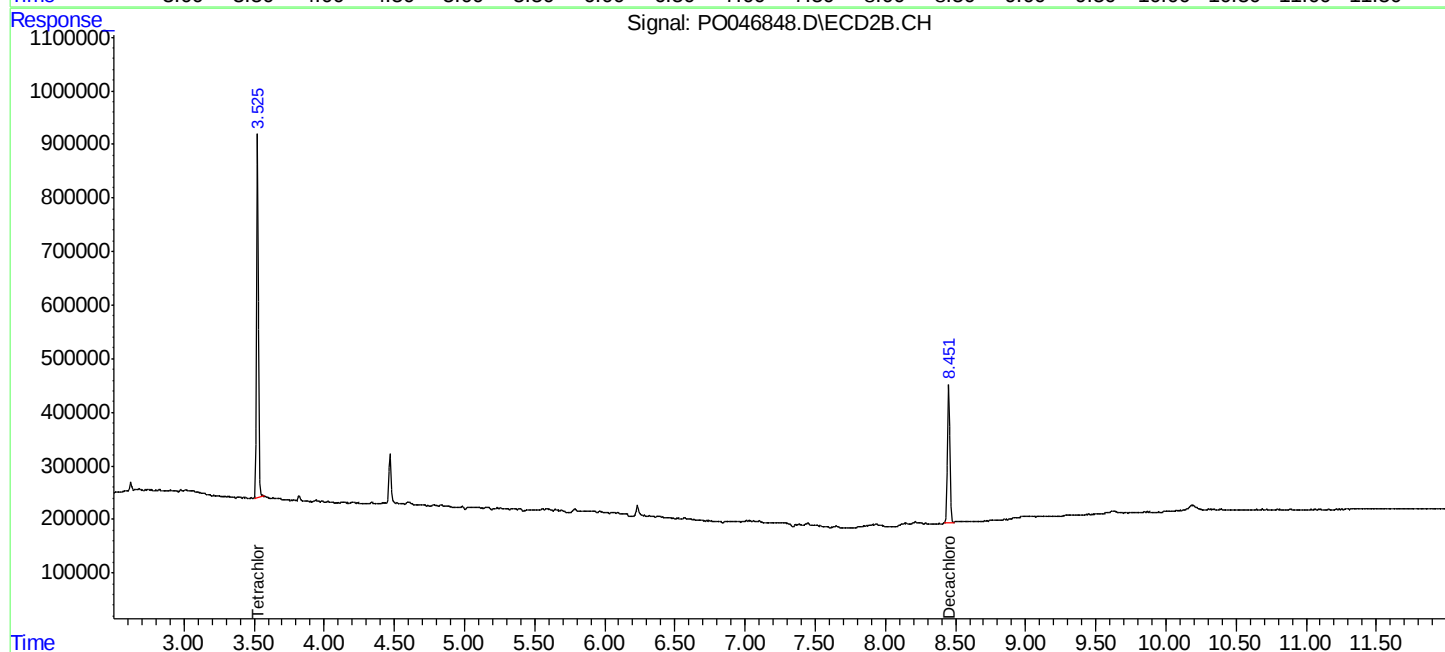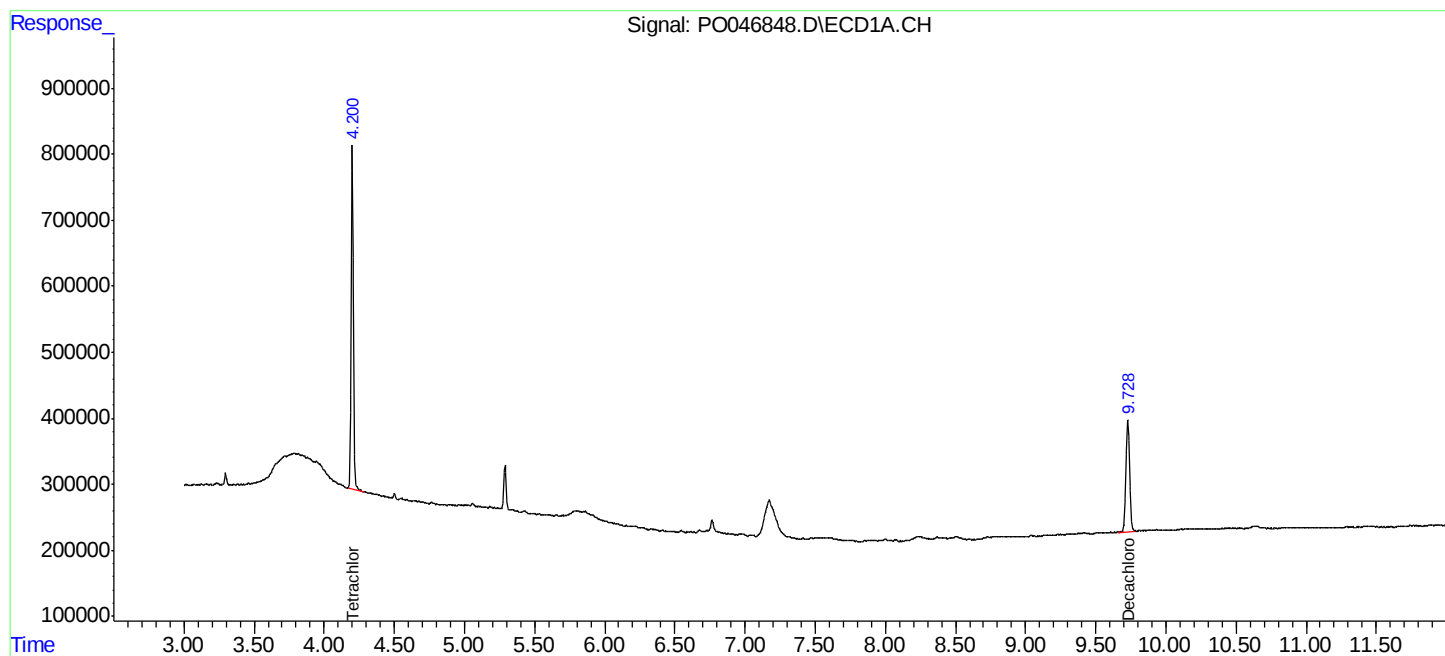


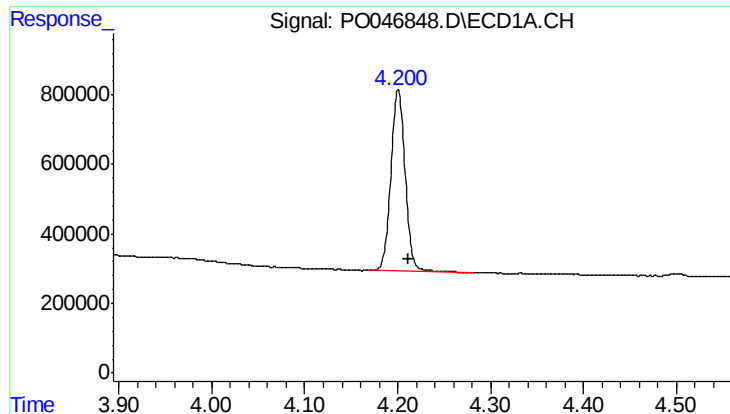

#1 Tetrachloro-m-xylene


R.T.: 4.201 min
Delta R.T.: -0.012 min
Response: 5642479
Conc: 23.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-I-S

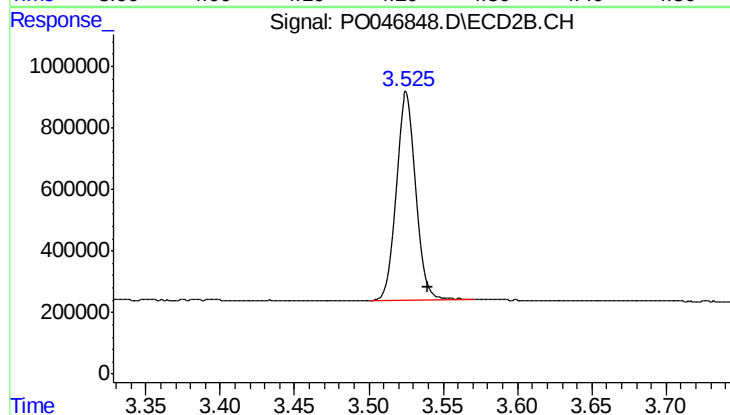


#1 Tetrachloro-m-xylene

R.T.: 3.525 min
Delta R.T.: -0.014 min
Response: 6209325
Conc: 29.23 ng/ml

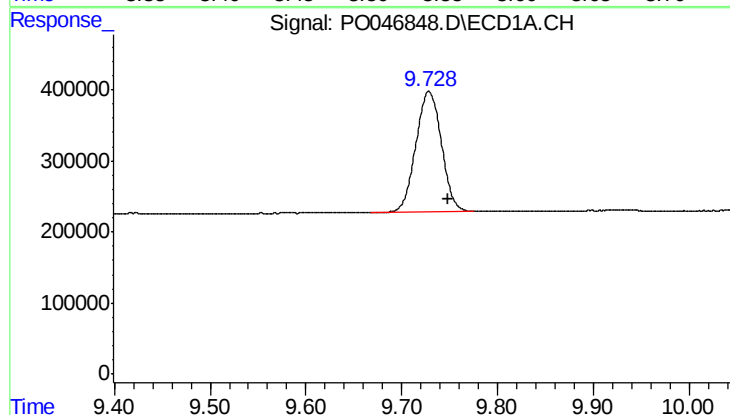

#2 Decachlorobiphenyl

R.T.: 9.728 min
Delta R.T.: -0.019 min
Response: 3140460
Conc: 16.48 ng/ml

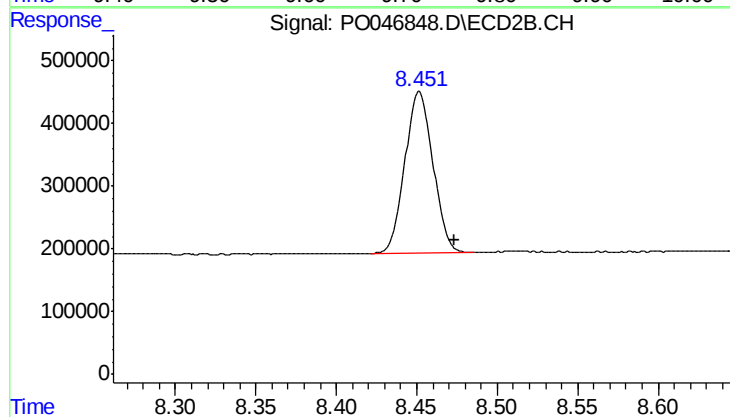

#2 Decachlorobiphenyl

R.T.: 8.451 min
Delta R.T.: -0.022 min
Response: 3134390
Conc: 16.16 ng/ml