

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071720\
 Data File : P0069785.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Jul 2020 16:28
 Operator : DD\AJ
 Sample : L3324-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CHRT-26948

Manual Integrations
 APPROVED

Sohil
 7/20/2020 3:07:10 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 17:59:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 08 16:12:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.391	3.566	791844	1023690	21.209m	25.723
2)	SA Decachlor...	10.047	8.772	1004944	974124	16.703	17.164

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071720\
Data File : PO069785.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Jul 2020 16:28
Operator : DD\AJ
Sample : L3324-03
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
CHRT-26948


Manual Integrations
APPROVED

Sohil
7/20/2020 3:07:10 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 17:59:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO070820.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 08 16:12:41 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

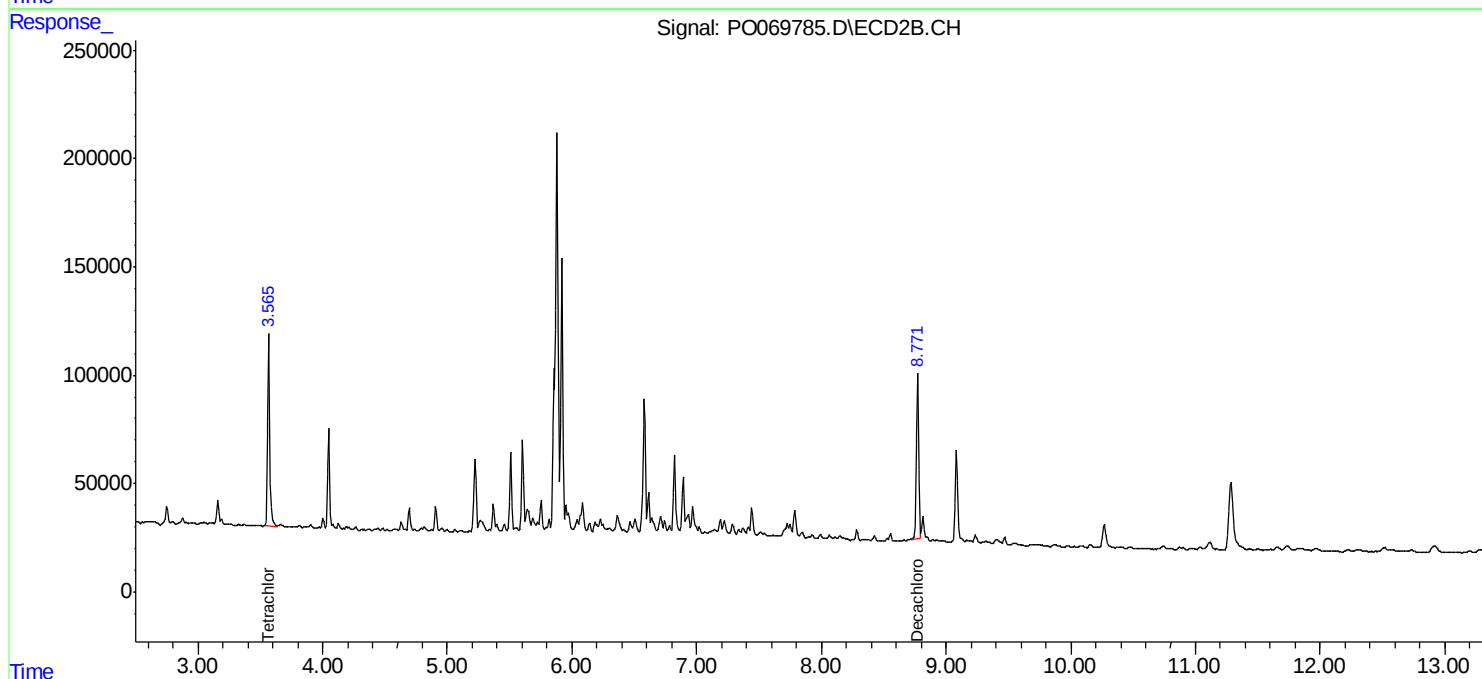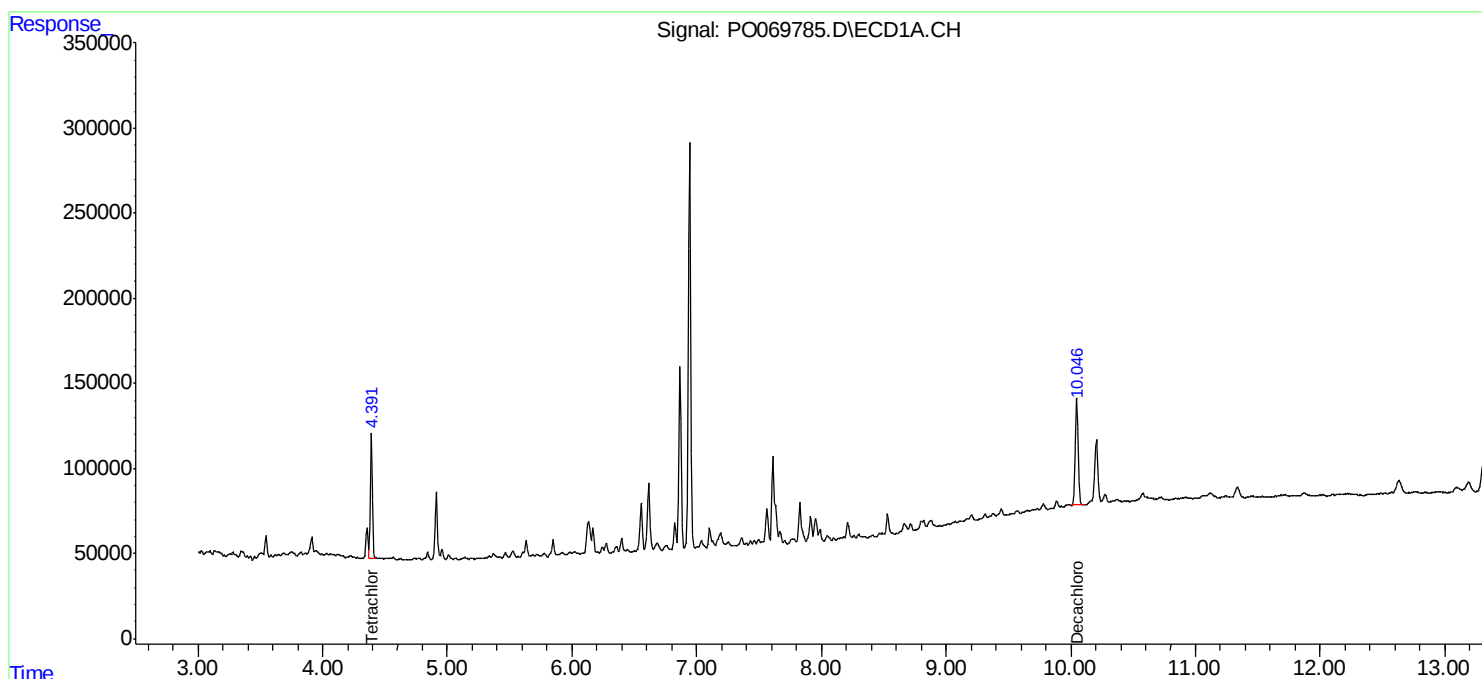

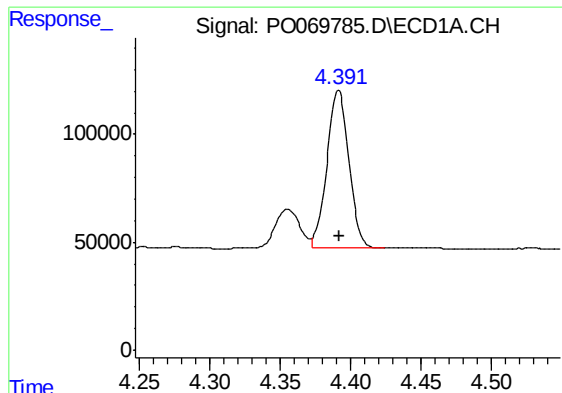


#1 Tetrachloro-m-xylene

R.T.: 4.391 min
Delta R.T.: 0.000 min
Response: 791844
Conc: 21.21 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CHRT-26948


Manual Integrations
APPROVED

Sohil
7/20/2020 3:07:10 PM

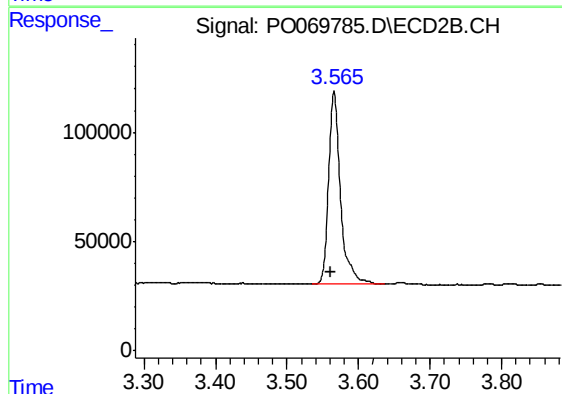


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: 0.004 min
Response: 1023690
Conc: 25.72 ng/ml

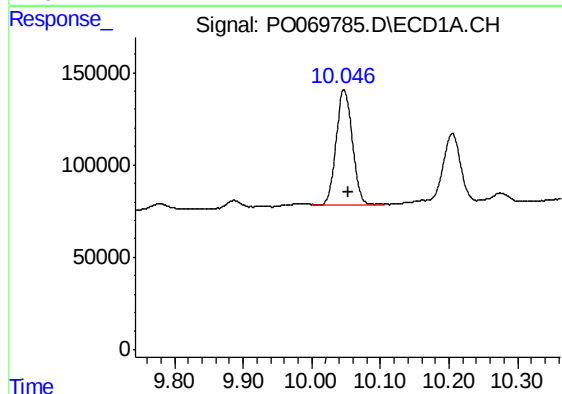

#2 Decachlorobiphenyl

R.T.: 10.047 min
Delta R.T.: -0.007 min
Response: 1004944
Conc: 16.70 ng/ml

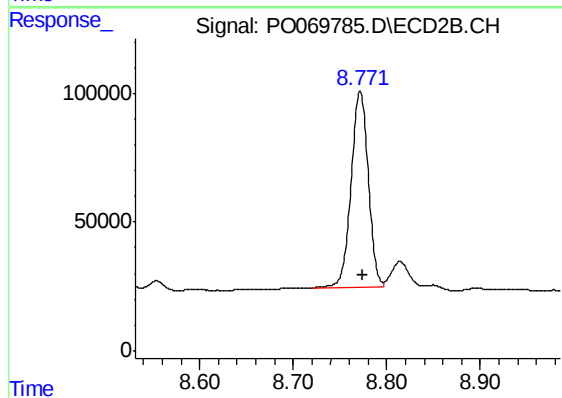

#2 Decachlorobiphenyl

R.T.: 8.772 min
Delta R.T.: -0.002 min
Response: 974124
Conc: 17.16 ng/ml