

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071724\
 Data File : P0104792.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2024 11:28
 Operator : YP/AJ
 Sample : P3248-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 B-120-SB02

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/18/2024
 Supervised By :Ankita Jodhani 07/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 12:19:37 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070224.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 02 16:29:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.428	3.542	165.1E6	62605941	18.435	19.189
2) SA Decachlor...	10.218	8.440	76347552	27344090	12.450m	13.039

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071724\
Data File : PO104792.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2024 11:28
Operator : YP/AJ
Sample : P3248-02
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
B-120-SB02


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :Ankita Jodhani 07/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 12:19:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO070224.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 02 16:29:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

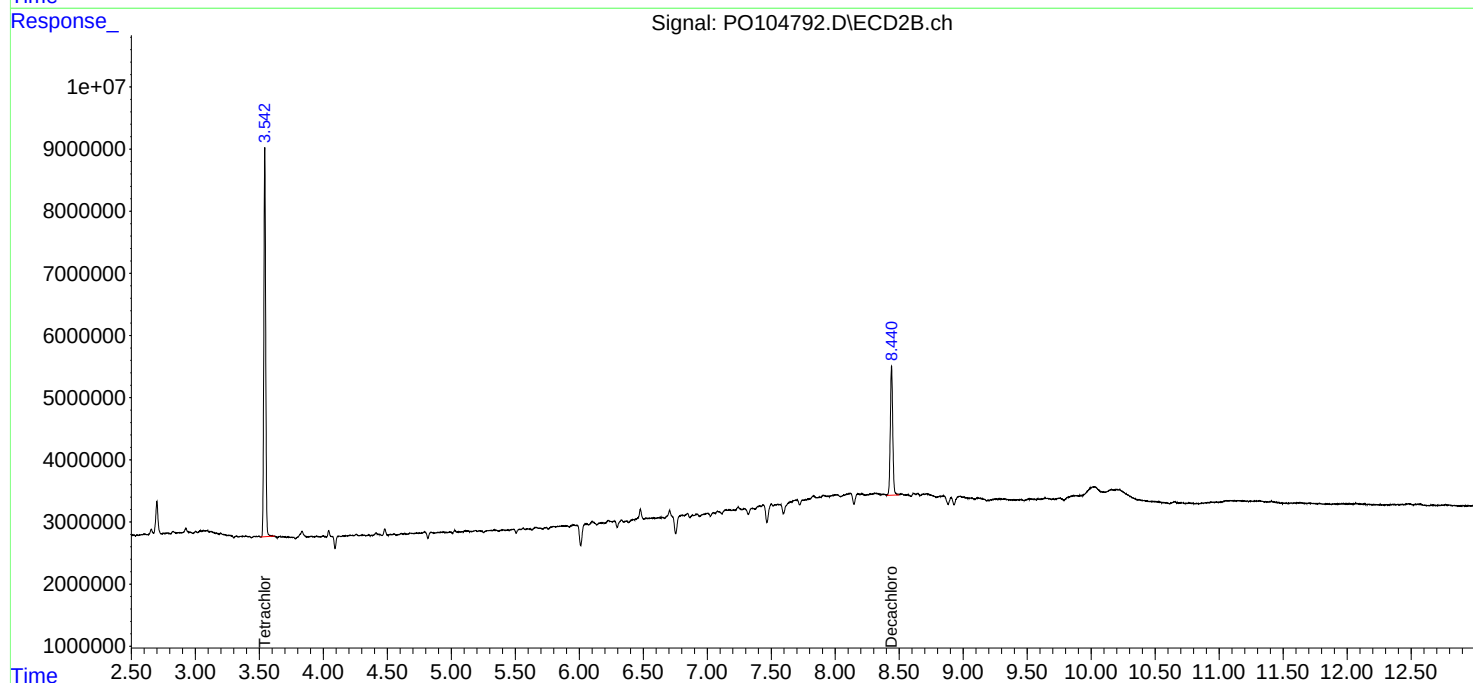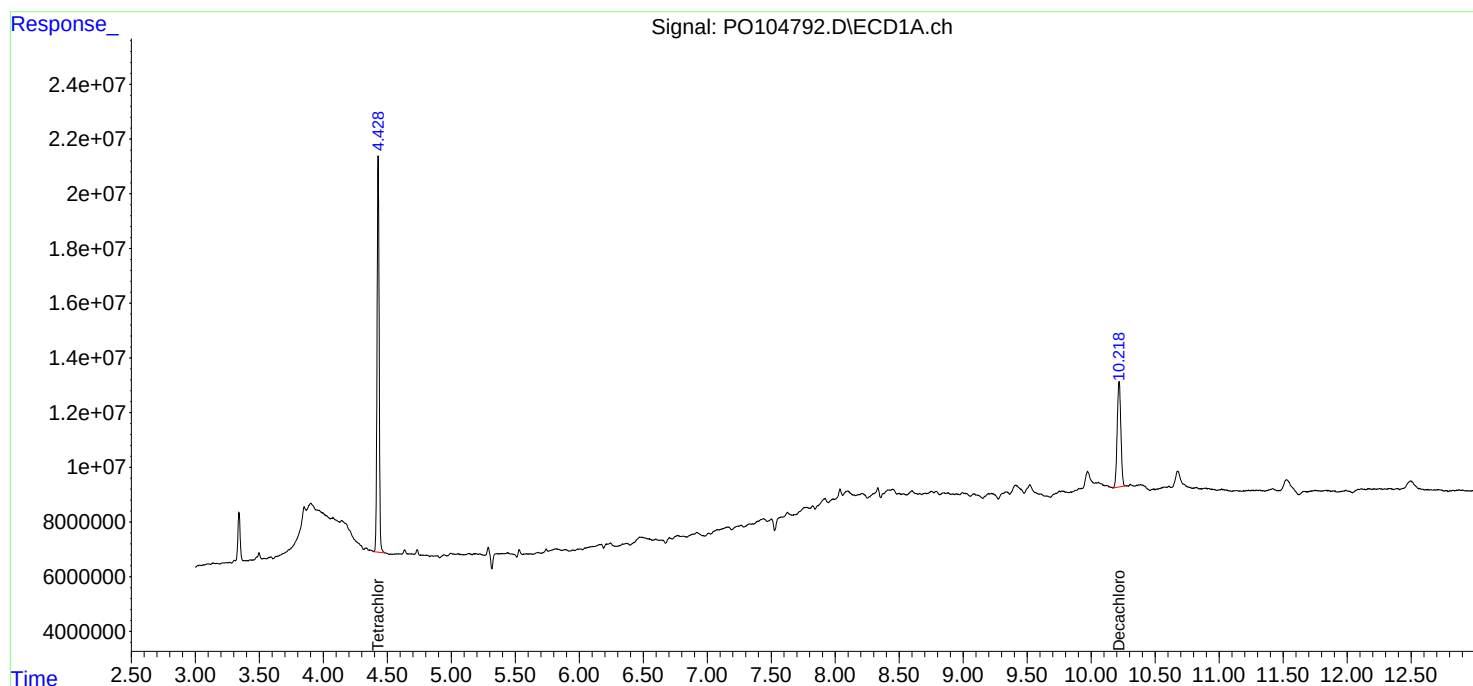

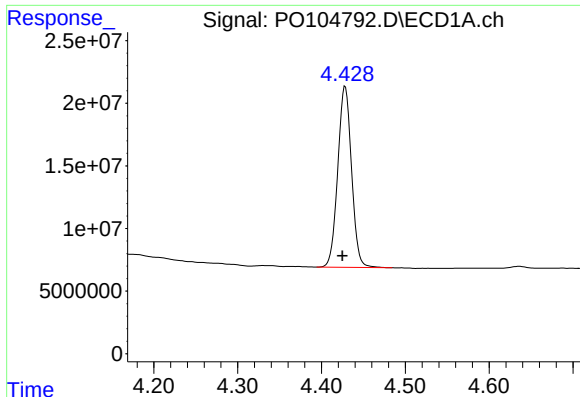

#1 Tetrachloro-m-xylene

R.T.: 4.428 min
Delta R.T.: 0.003 min
Response: 165053875
Conc: 18.43 ng/ml

Instrument :

ECD_O


ClientSampleId :

B-120-SB02

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :Ankita Jodhani 07/19/2024

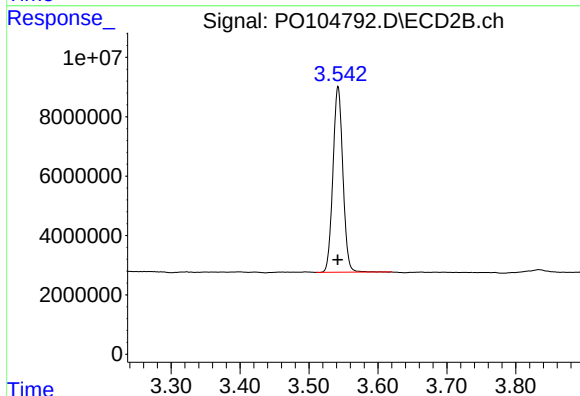


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: 0.000 min
Response: 62605941
Conc: 19.19 ng/ml

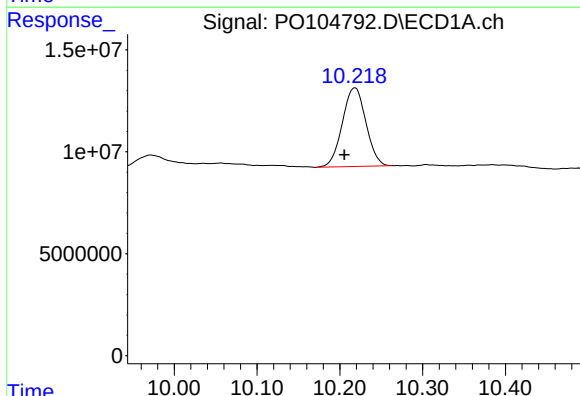

#2 Decachlorobiphenyl

R.T.: 10.218 min
Delta R.T.: 0.012 min
Response: 76347552
Conc: 12.45 ng/ml m

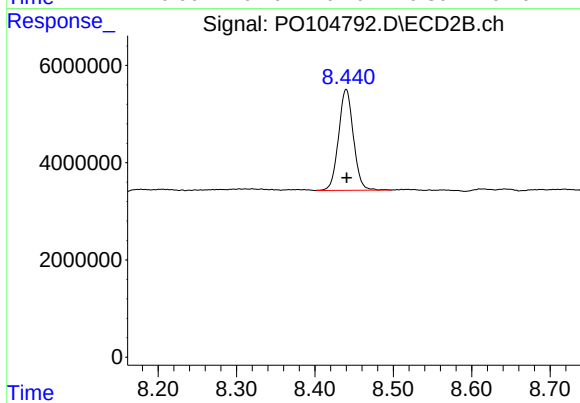

#2 Decachlorobiphenyl

R.T.: 8.440 min
Delta R.T.: 0.000 min
Response: 27344090
Conc: 13.04 ng/ml